


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070720\
 Data File : BG045952.D
 Acq On : 7 Jul 2020 8:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG070620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 07 09:58:42 2020

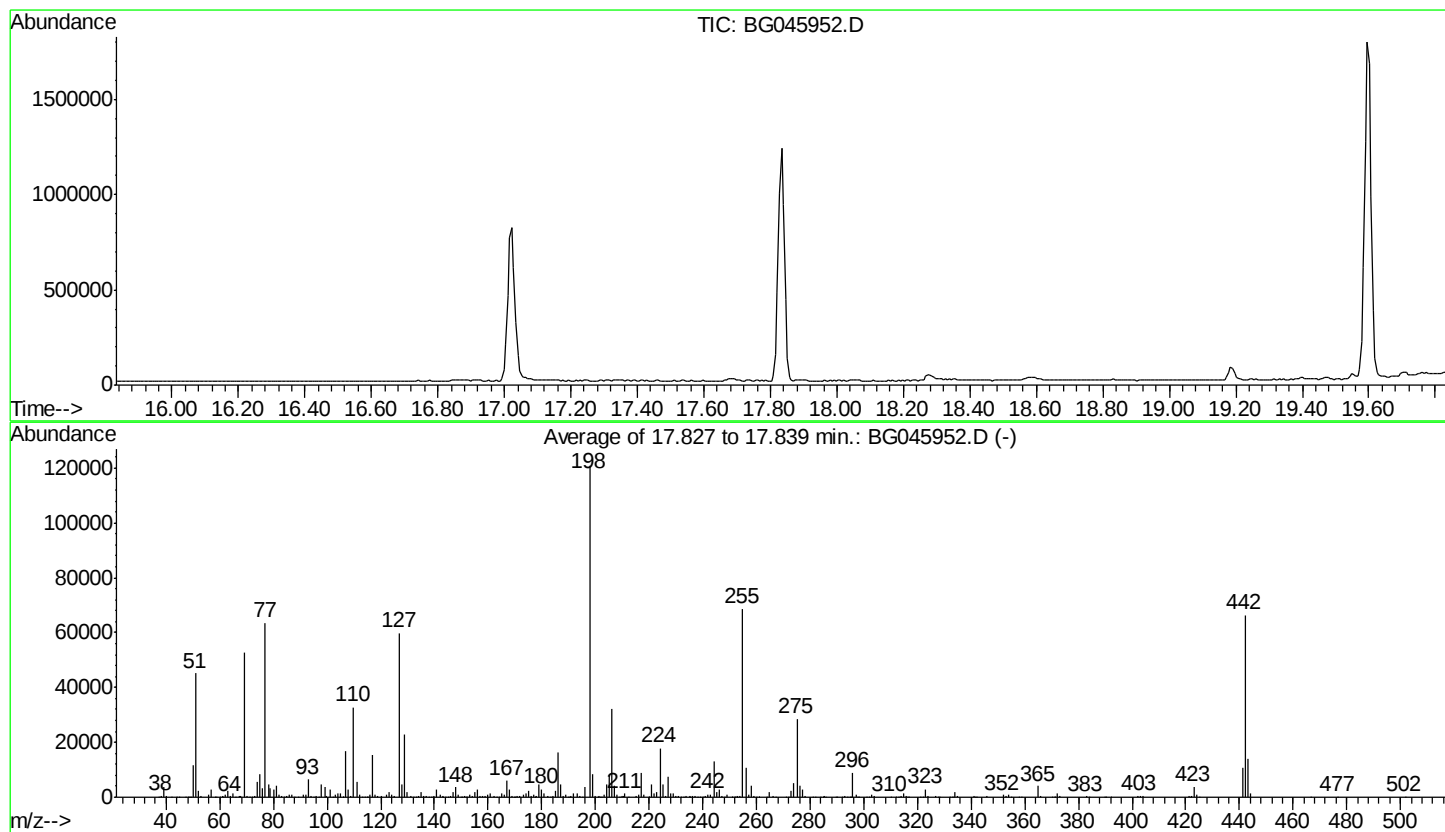

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	45052	PASS
68	69	0.00	2	0.7	380	PASS
69	198	0.00	100	43.6	52734	PASS
70	69	0.00	2	0.9	457	PASS
127	198	10	80	49.6	59937	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	120842	PASS
199	198	5	9	6.9	8360	PASS
275	198	10	60	23.6	28464	PASS
365	198	1	100	3.4	4099	PASS
441	198	0.01	100	8.8	10577	PASS
442	198	50	100	54.9	66325	PASS
443	442	15	24	20.9	13831	PASS