


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG070720\
 Data File : BG045960.D
 Acq On : 7 Jul 2020 15:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG070620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 07 09:58:42 2020

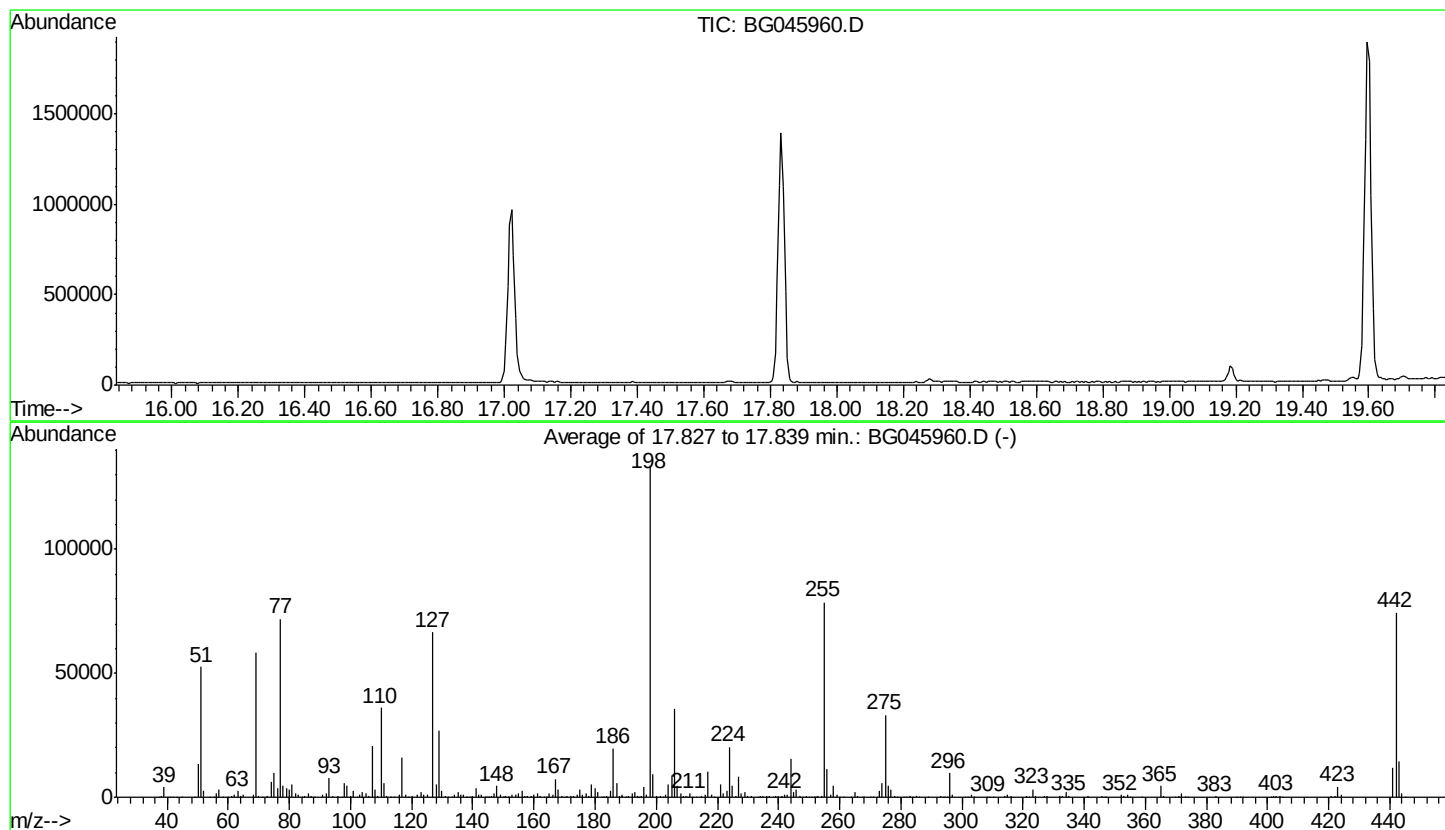

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	52533	PASS
68	69	0.00	2	1.4	816	PASS
69	198	0.00	100	43.5	58273	PASS
70	69	0.00	2	0.6	376	PASS
127	198	10	80	49.7	66576	PASS
197	198	0.00	2	0.7	906	PASS
198	198	100	100	100.0	133832	PASS
199	198	5	9	7.1	9470	PASS
275	198	10	60	24.8	33250	PASS
365	198	1	100	3.3	4439	PASS
441	198	0.01	100	8.9	11957	PASS
442	198	50	100	55.7	74568	PASS
443	442	15	24	19.5	14573	PASS