
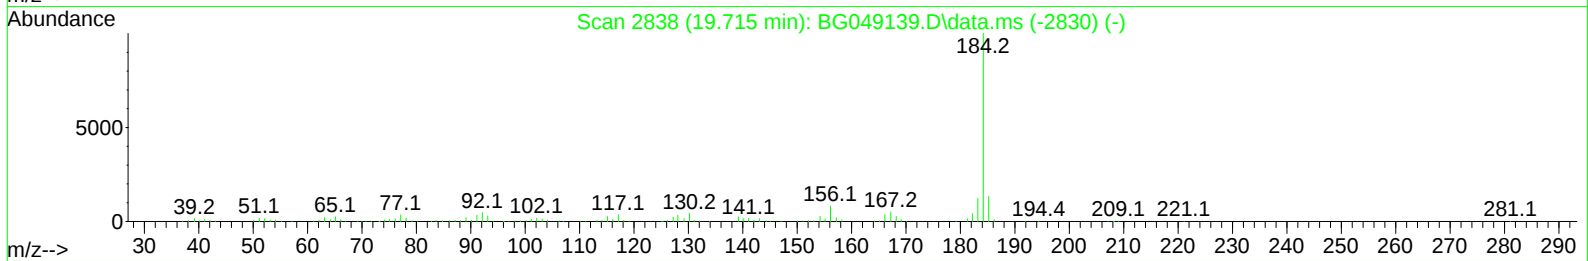
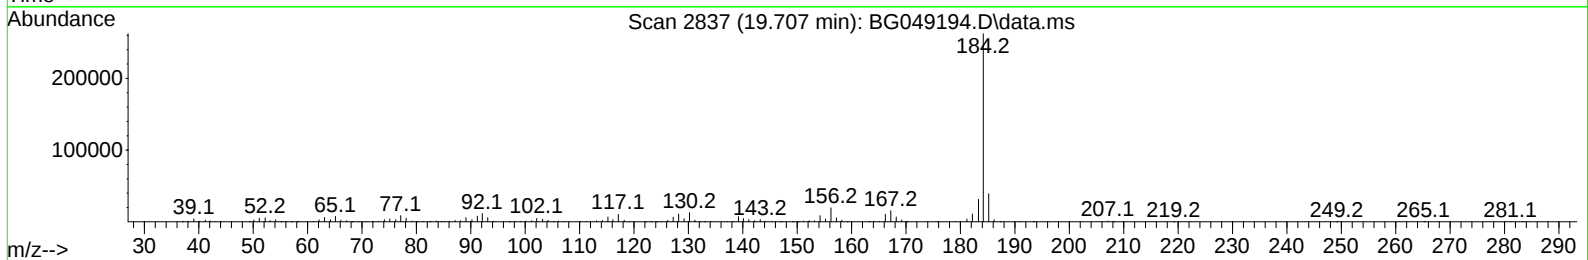


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070721\
Data File : BG049194.D
Acq On : 7 Jul 2021 11:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 07 11:58:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 06 10:59:02 2021
Response via : Initial Calibration

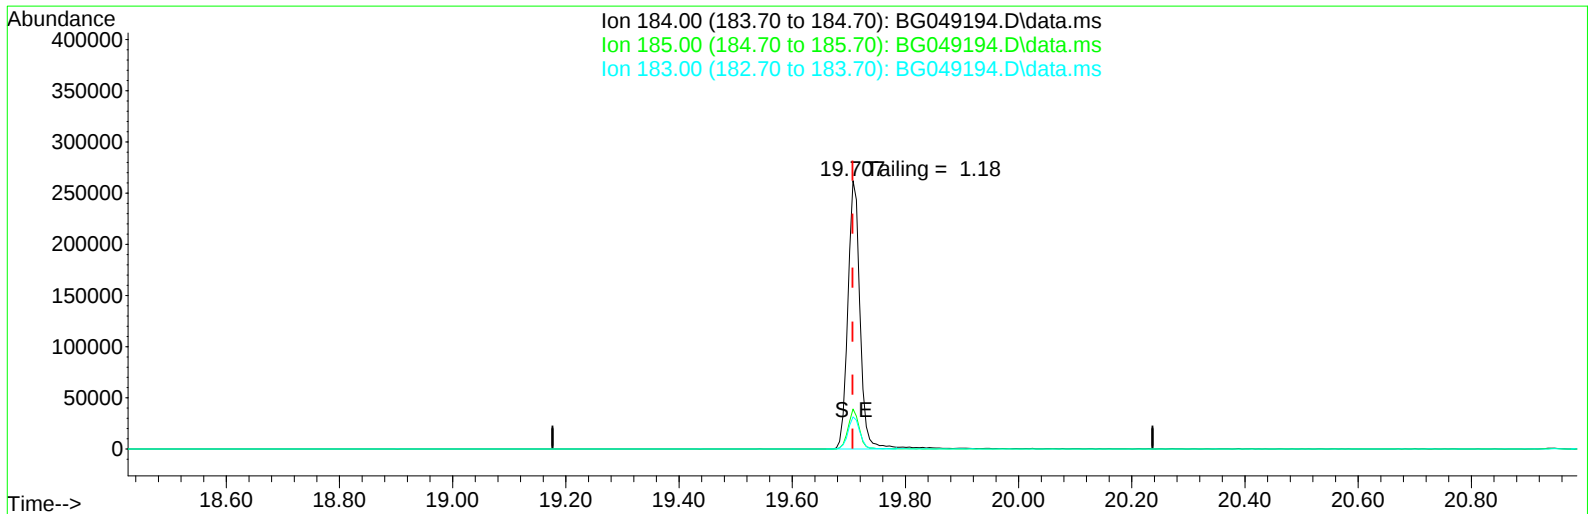




TIC: BG049194.D\data.ms

(77) Benzidine**19.707min (+ 0.001) 328478.20 ng****response 388059**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.93
183.00	11.70	11.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070721\
Data File : BG049194.D
Acq On : 7 Jul 2021 11:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 07 11:58:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 06 10:59:02 2021
Response via : Initial Calibration

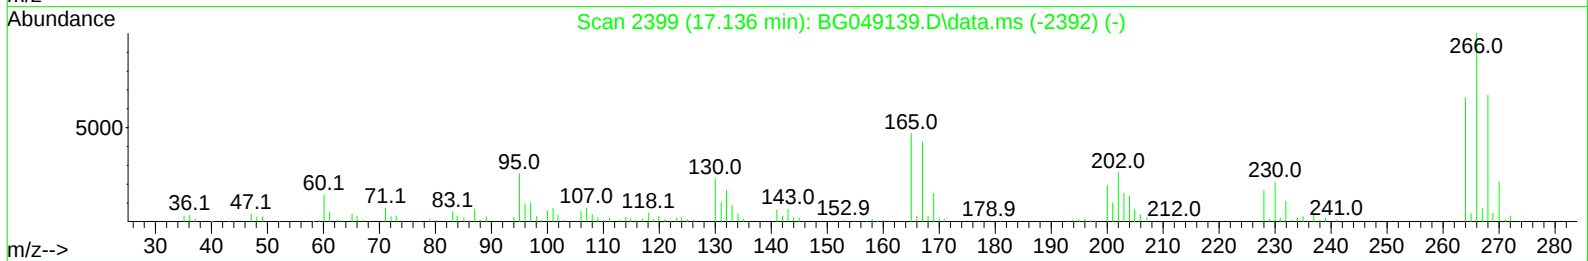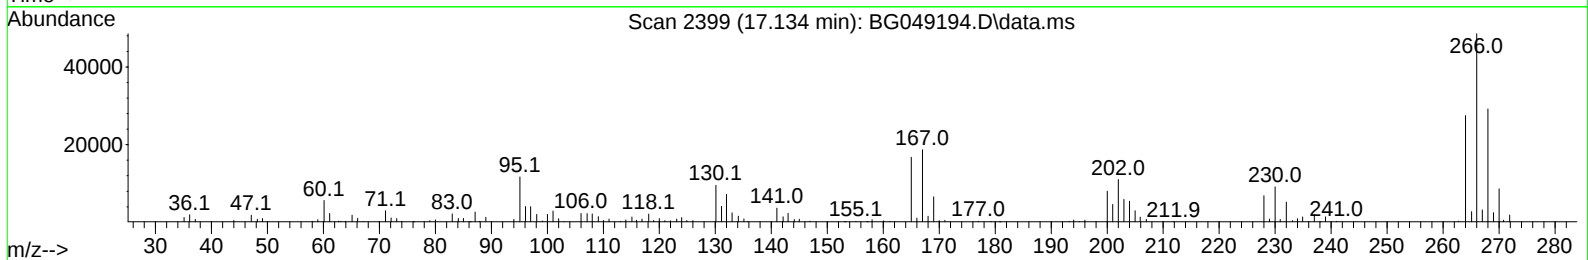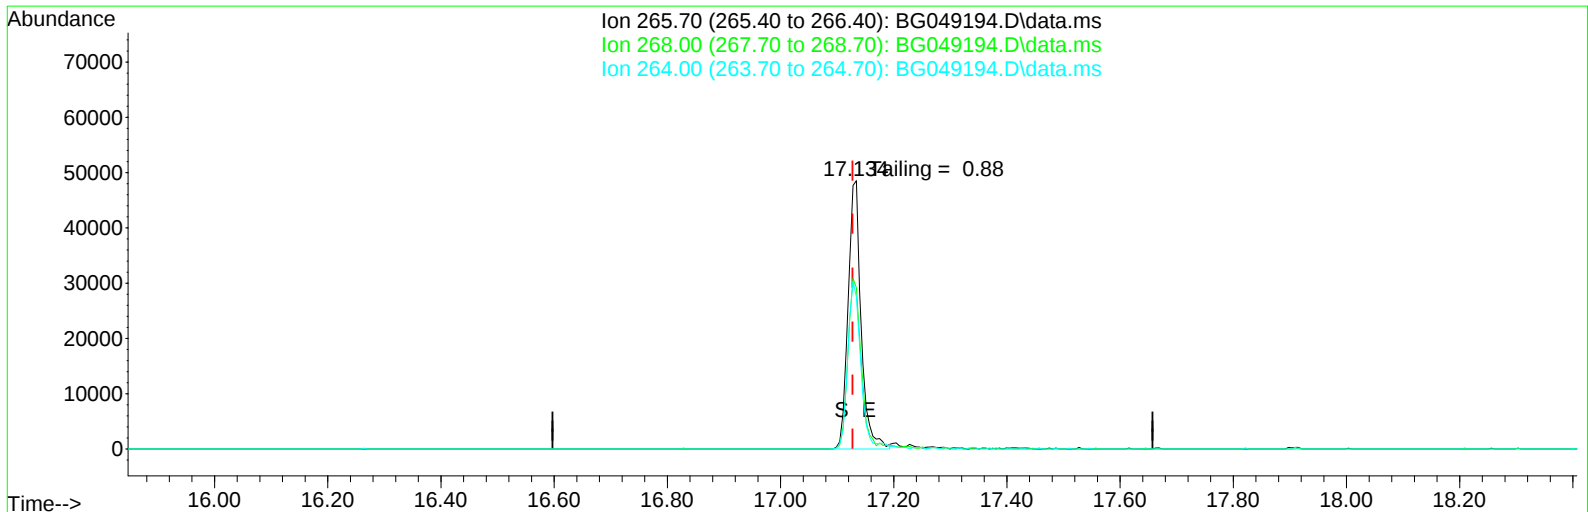

TIC: BG049194.D\data.ms

(70) Pentachlorophenol (C)

17.134min (+ 0.007) 27119.77 ng

response 77460

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	60.09
264.00	61.30	56.65
0.00	0.00	0.00