

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070721\
 Data File : BG049200.D
 Acq On : 7 Jul 2021 15:21
 Operator : CG/JU
 Sample : M2936-01 2X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TR-05-070221

Manual Integrations
 APPROVED

mohammad
 7/8/2021 12:40:22 PM

Quant Time: Jul 07 16:11:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 06 10:59:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.088	152	48495	20.000	ng	0.00
21) Naphthalene-d8	10.908	136	185178	20.000	ng	# 0.00
39) Acenaphthene-d10	14.733	164	121673	20.000	ng	0.00
64) Phenanthrene-d10	17.477	188	242221	20.000	ng	# 0.00
76) Chrysene-d12	21.760	240	237606	20.000	ng	0.00
86) Perylene-d12	25.074	264	254671	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.644	112	97823	31.595	ng	0.00
7) Phenol-d6	7.242	99	130649	29.597	ng	0.00
23) Nitrobenzene-d5	9.251	82	90159	20.642	ng	0.00
42) 2,4,6-Tribromophenol	16.214	330	56965	27.007	ng	0.00
45) 2-Fluorobiphenyl	13.347	172	168886	18.727	ng	0.00
79) Terphenyl-d14	20.086	244	218337	15.571	ng	0.00
Target Compounds						Qvalue
50) Dimethylphthalate	14.175	163	23531	2.410	ng	97
58) Fluorene	15.773	166	26650	2.693	ng	96
71) Phenanthrene	17.518	178	198093	14.202	ng	97
72) Anthracene	17.612	178	52966	3.809	ng	99
75) Fluoranthene	19.528	202	245461	14.057	ng	98
78) Pyrene	19.892	202	244082	13.831	ng	97
81) Benzo(a)anthracene	21.743	228	112097	6.325	ng	96
83) Chrysene	21.813	228	106729	6.339	ng	99
87) Indeno(1,2,3-cd)pyrene	28.840	276	63476	3.124	ng	99
88) Benzo(b)fluoranthene	24.022	252	127545	6.940	ng	# 91
89) Benzo(k)fluoranthene	24.081	252	44239m	2.523	ng	
90) Benzo(a)pyrene	24.910	252	98825	5.829	ng	# 94
92) Benzo(g,h,i)perylene	30.033	276	62428	3.692	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070721\
Data File : BG049200.D
Acq On : 7 Jul 2021 15:21
Operator : CG/JU
Sample : M2936-01 2X
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
TR-05-070221

Manual Integrations
APPROVED

mohammad
7/8/2021 12:40:22 PM


Quant Time: Jul 07 16:11:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 06 10:59:02 2021
Response via : Initial Calibration

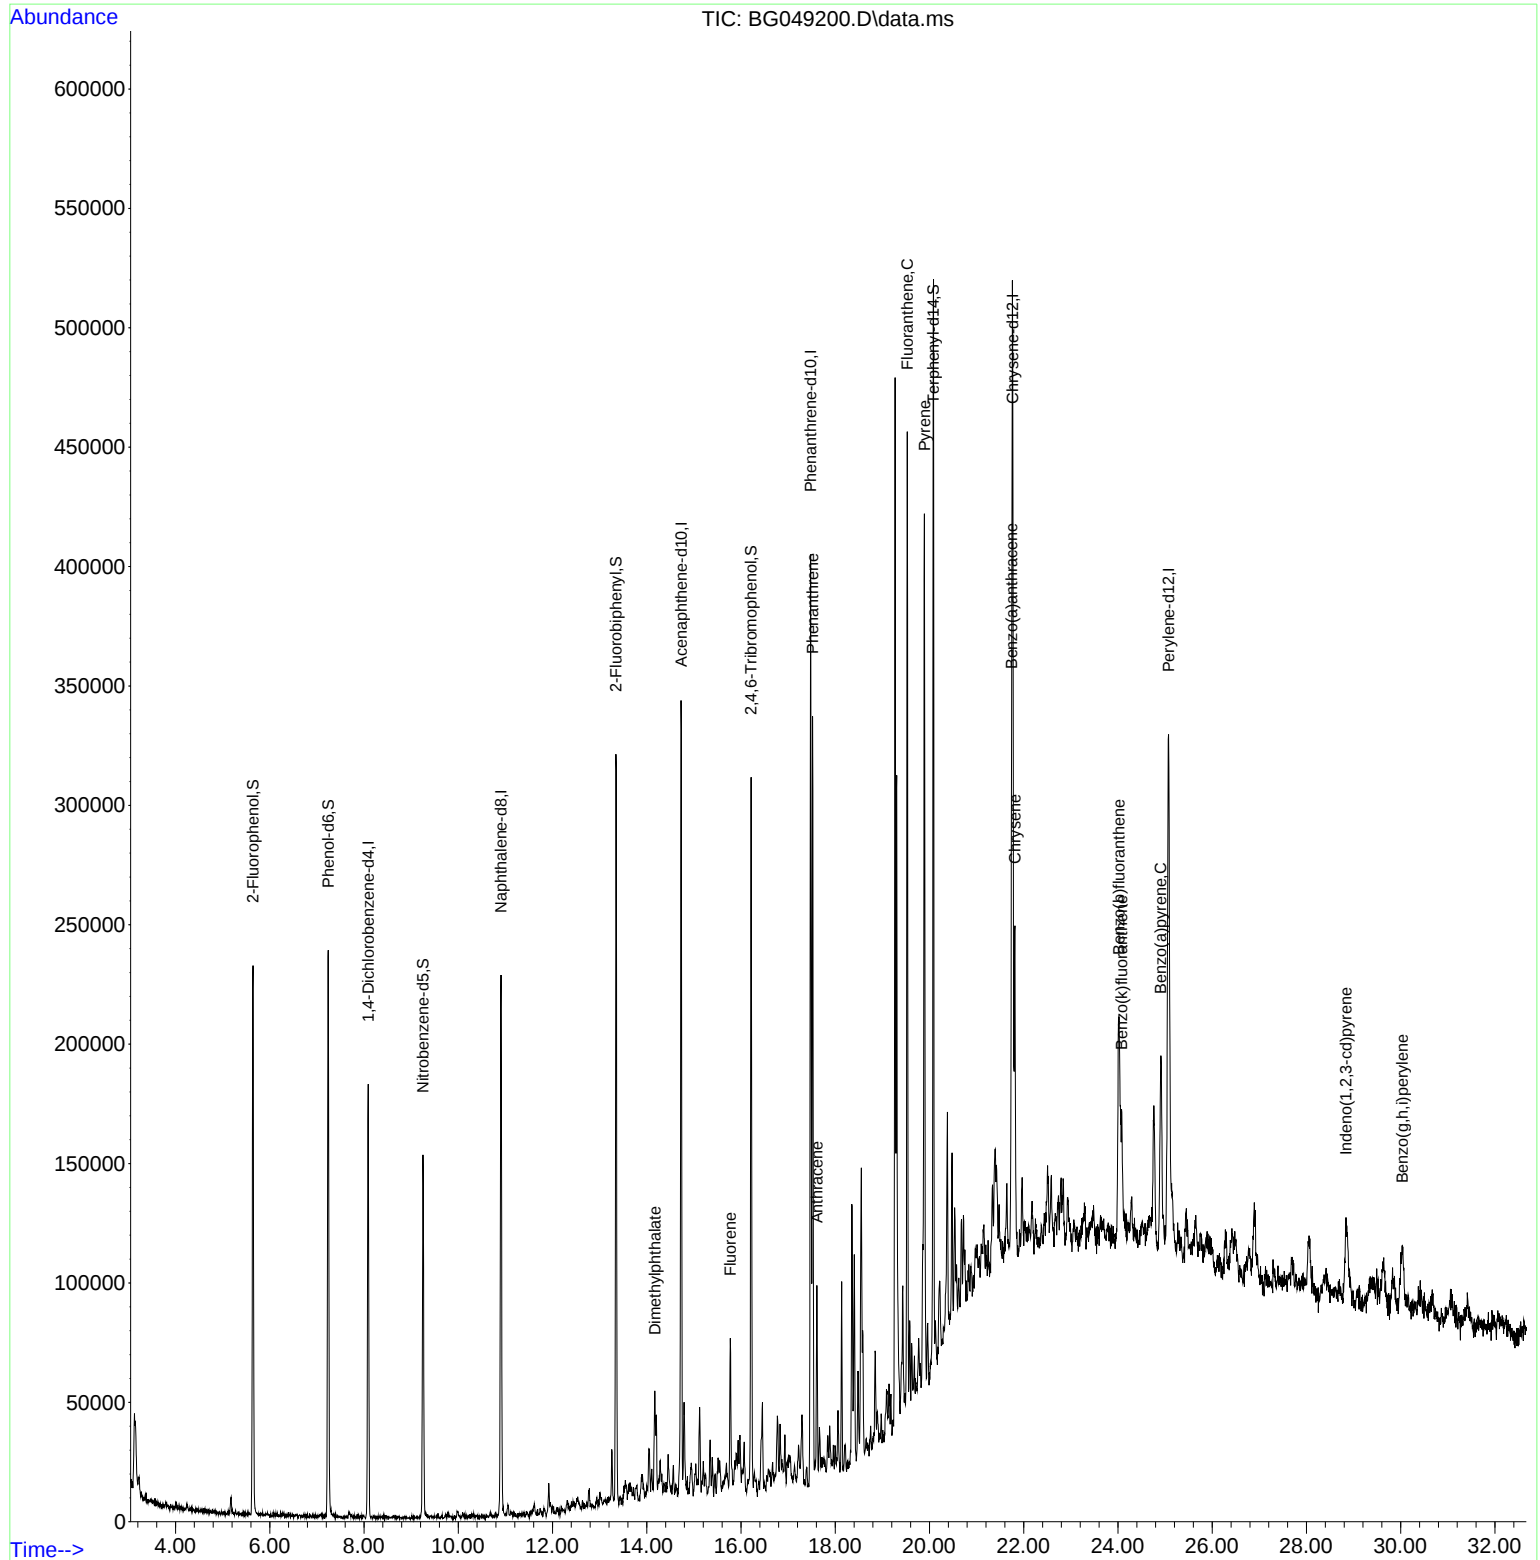



#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.088 min Scan# 859
Delta R.T. -0.003 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21




Instrument :
BNA_G
ClientSampled :
TR-05-070221




Tgt Ion:152 Resp: 48495
Ion Ratio Lower Upper
152 100
150 155.0 119.4 179.0
115 70.2 60.2 90.4

Manual Integrations
APPROVED



mohammad
7/8/2021 12:40:22 PM

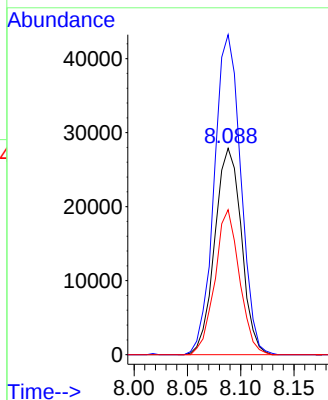


#5
2-Fluorophenol
Concen: 31.595 ng
RT: 5.644 min Scan# 443
Delta R.T. 0.009 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21

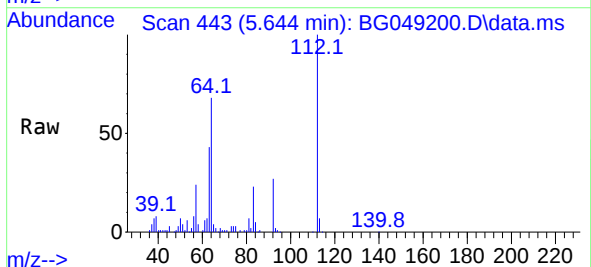


Tgt Ion:112 Resp: 97823
Ion Ratio Lower Upper
112 100
64 68.5 46.7 70.1
63 42.6 35.3 52.9


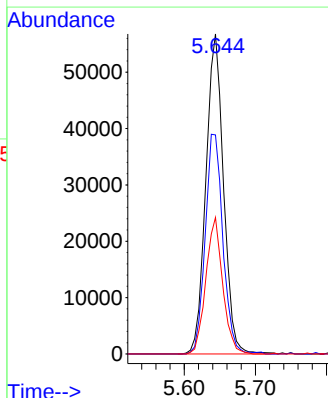
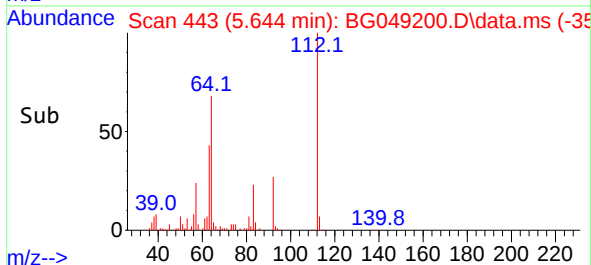





#7
Phenol-d6
Concen: 29.597 ng
RT: 7.242 min Scan# 715
Delta R.T. 0.003 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21





Tgt Ion: 99 Resp: 130649
Ion Ratio Lower Upper
99 100
42 22.5 20.5 30.7
71 44.9 41.5 62.3

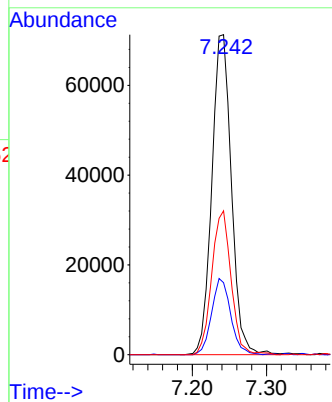

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.908 min Scan# 1339
Delta R.T. 0.003 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21

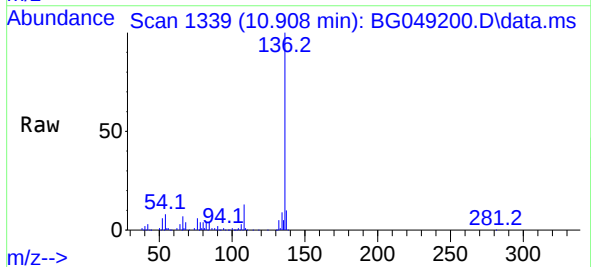


Tgt Ion: 136 Resp: 185178
Ion Ratio Lower Upper
136 100
137 9.5 8.2 12.2
54 8.4 5.5 8.3#
68 4.3 2.3 3.5#

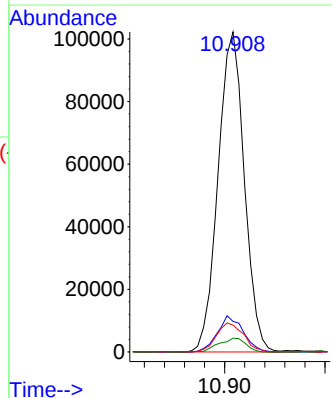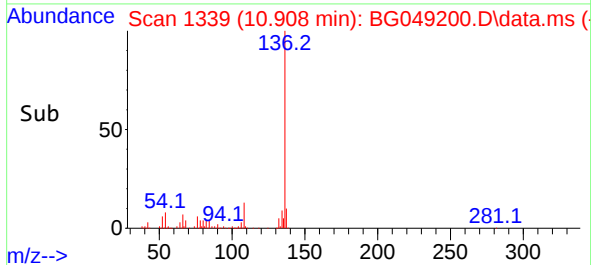

Instrument :
BNA_G
ClientSampled :
TR-05-070221

Manual Integrations
APPROVED

mohammad
7/8/2021 12:40:22 PM

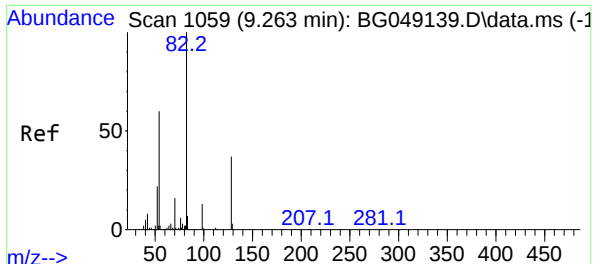





#23
Nitrobenzene-d5
Concen: 20.642 ng
RT: 9.251 min Scan# 1057
Delta R.T. -0.002 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21

Tgt Ion:	82	Resp:	90159
Ion Ratio	Lower	Upper	
82	100		
128	37.1	29.8	44.6
54	59.2	45.8	68.8

Instrument :
BNA_G
ClientSampleId :
TR-05-070221




Manual Integrations
APPROVED


mohammad
7/8/2021 12:40:22 PM

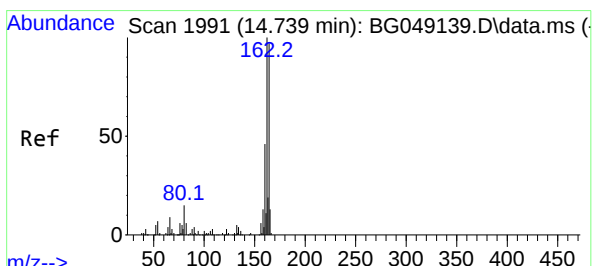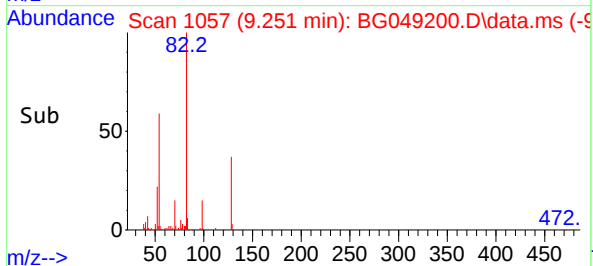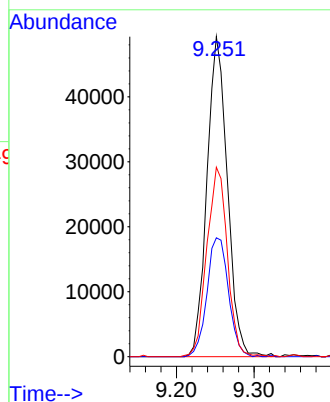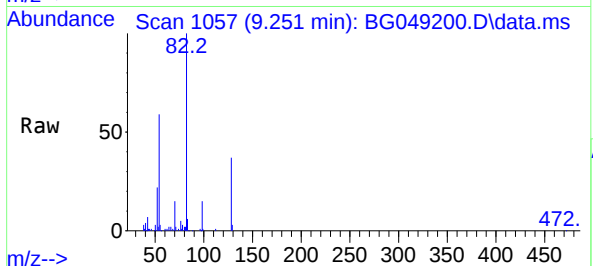

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.733 min Scan# 1990
Delta R.T. 0.003 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21


Tgt Ion:	164	Resp:	121673
Ion Ratio	Lower	Upper	
164	100		
162	95.6	81.4	122.0
160	43.8	34.9	52.3

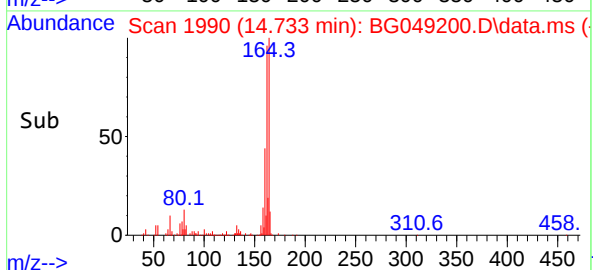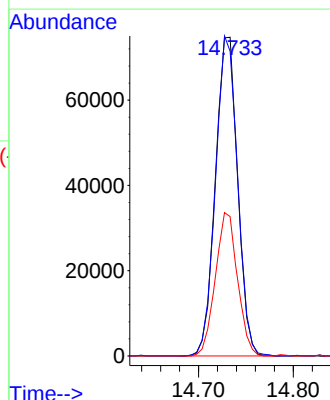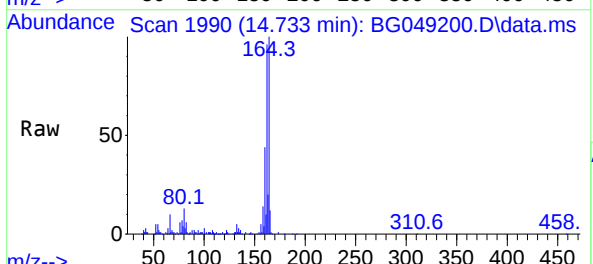



#42
2,4,6-Tribromophenol
Concen: 27.007 ng
RT: 16.214 min Scan# 2242
Delta R.T. -0.002 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21




Instrument :
BNA_G
ClientSampled :
TR-05-070221




Tgt Ion:330 Resp: 56965
Ion Ratio Lower Upper
330 100
332 95.7 77.3 115.9
141 36.2 35.6 53.4

Manual Integrations
APPROVED



mohammad
7/8/2021 12:40:22 PM

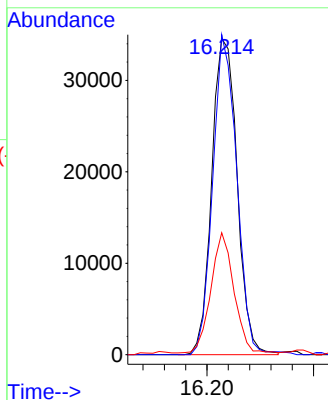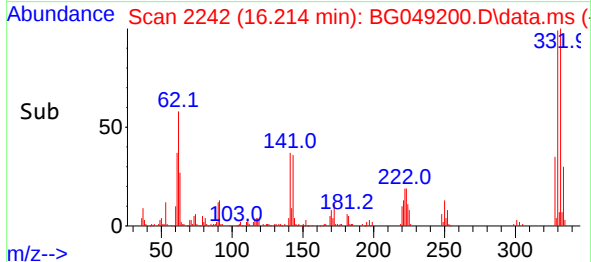


#45
2-Fluorobiphenyl
Concen: 18.727 ng
RT: 13.347 min Scan# 1754
Delta R.T. -0.002 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21

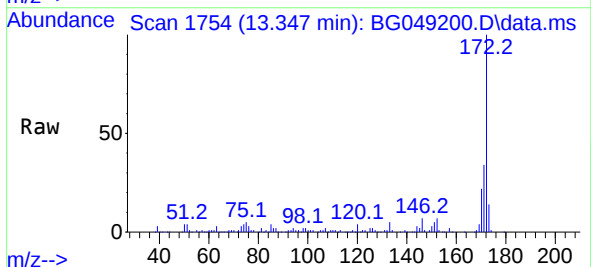


Tgt Ion:172 Resp: 168886
Ion Ratio Lower Upper
172 100
171 33.5 28.6 43.0
170 22.3 18.6 27.8


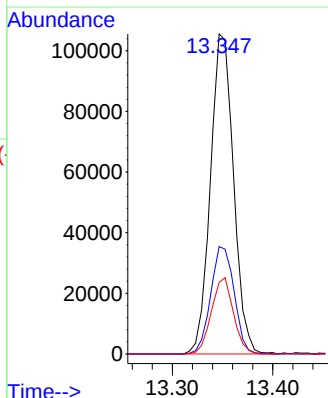
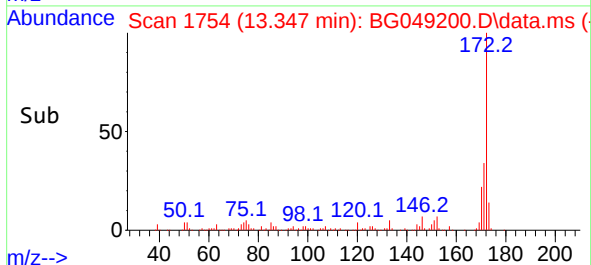





#50
Dimethylphthalate
Concen: 2.410 ng
RT: 14.175 min Scan# 1895
Delta R.T. -0.002 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21





Tgt Ion:163 Resp: 23531
Ion Ratio Lower Upper
163 100
194 4.4 3.0 4.6
164 12.1 8.6 12.8

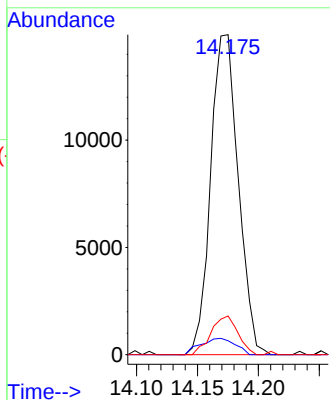

#58
Fluorene
Concen: 2.693 ng
RT: 15.773 min Scan# 2167
Delta R.T. -0.002 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21




Tgt Ion:166 Resp: 26650
Ion Ratio Lower Upper
166 100
165 93.1 77.7 116.5
167 12.9 10.8 16.2

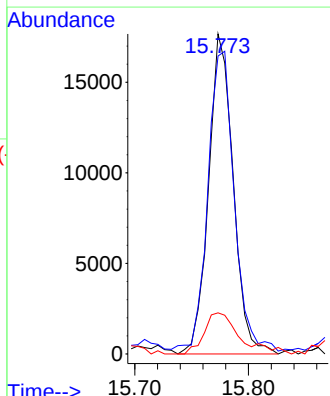

Instrument :
BNA_G
ClientSampleId :
TR-05-070221


Manual Integrations
APPROVED

mohammad
7/8/2021 12:40:22 PM



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.477 min Scan# 2457
Delta R.T. -0.002 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21




Instrument :
BNA_G
ClientSampleId :
TR-05-070221



Tgt Ion:188 Resp: 242221
Ion Ratio Lower Upper
188 100
94 5.9 5.4 8.0
80 6.7 3.7 5.5#




Manual Integrations
APPROVED


mohammad
7/8/2021 12:40:22 PM

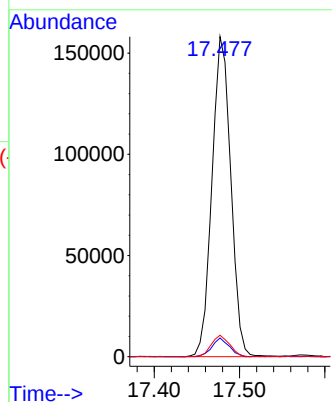

#71
Phenanthrene
Concen: 14.202 ng
RT: 17.518 min Scan# 2464
Delta R.T. -0.002 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21


Tgt Ion:178 Resp: 198093
Ion Ratio Lower Upper
178 100
176 19.1 16.0 24.0
179 16.0 14.2 21.4

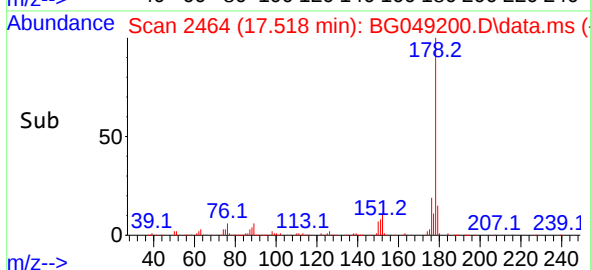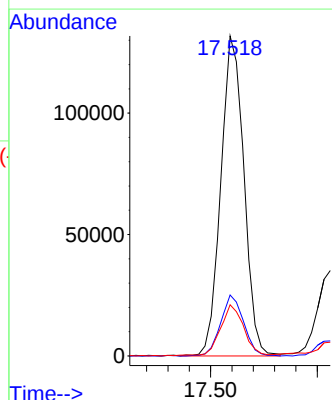



#72
 Anthracene
 Concen: 3.809 ng
 RT: 17.612 min Scan# 2480
 Delta R.T. 0.003 min
 Lab File: BG049200.D
 Acq: 7 Jul 2021 15:21




Instrument :
 BNA_G
 ClientSampleID :
 TR-05-070221




Tgt Ion:178 Resp: 52966
 Ion Ratio Lower Upper
 178 100
 176 17.7 14.6 21.8
 179 16.1 13.4 20.0

Manual Integrations
 APPROVED



mohammad
 7/8/2021 12:40:22 PM

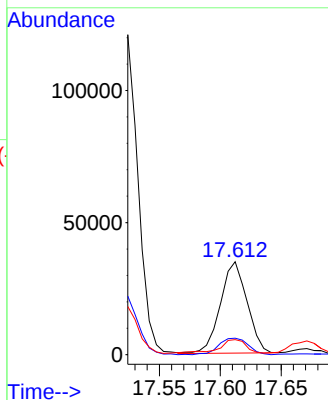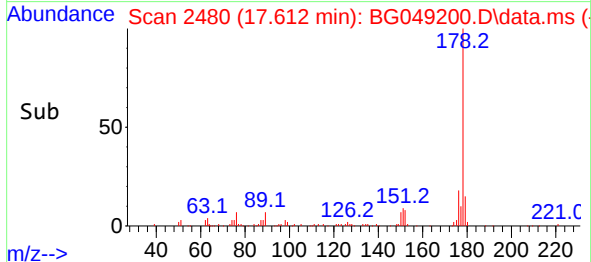


#75
 Fluoranthene
 Concen: 14.057 ng
 RT: 19.528 min Scan# 2806
 Delta R.T. -0.002 min
 Lab File: BG049200.D
 Acq: 7 Jul 2021 15:21




Tgt Ion:202 Resp: 245461
 Ion Ratio Lower Upper
 202 100
 101 5.9 0.0 24.7
 203 19.0 0.0 38.5

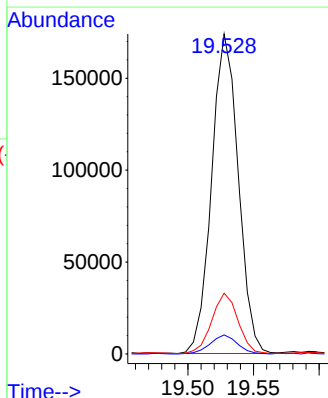



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.760 min Scan# 3186
Delta R.T. -0.002 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21




Instrument :
BNA_G
ClientSampleId :
TR-05-070221




Tgt Ion:240 Resp: 237606
Ion Ratio Lower Upper
240 100
120 4.9 4.2 6.2
236 24.8 21.8 32.6

Manual Integrations
APPROVED



mohammad
7/8/2021 12:40:22 PM

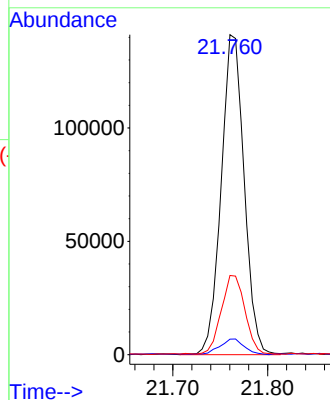


#78
Pyrene
Concen: 13.831 ng
RT: 19.892 min Scan# 2868
Delta R.T. 0.003 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21




Tgt Ion:202 Resp: 244082
Ion Ratio Lower Upper
202 100
200 21.7 15.8 23.8
203 17.1 14.6 21.8


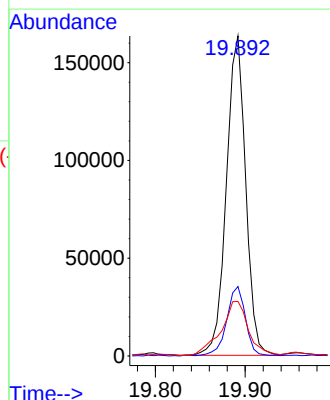






#79
Terphenyl-d14
Concen: 15.571 ng
RT: 20.086 min Scan# 2901
Delta R.T. 0.003 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21





Tgt Ion:244 Resp: 218337
Ion Ratio Lower Upper
244 100
212 8.4 6.9 10.3
122 6.6 5.0 7.6

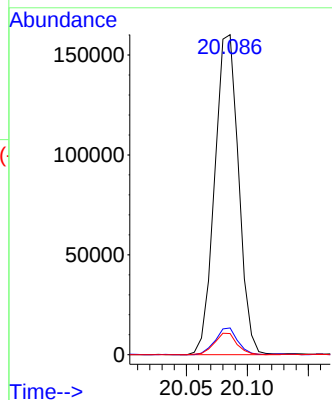

#81
Benzo(a)anthracene
Concen: 6.325 ng
RT: 21.743 min Scan# 3183
Delta R.T. -0.002 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21




Tgt Ion:228 Resp: 112097
Ion Ratio Lower Upper
228 100
226 30.0 22.7 34.1
229 22.3 16.0 24.0

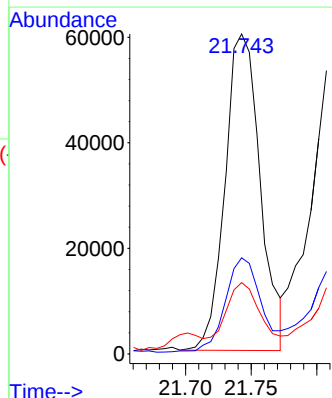

Instrument :
BNA_G
ClientSampleId :
TR-05-070221


Manual Integrations
APPROVED

mohammad
7/8/2021 12:40:22 PM



#83
Chrysene
Concen: 6.339 ng
RT: 21.813 min Scan# 3195
Delta R.T. 0.003 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21




Instrument :
BNA_G
ClientSampled :
TR-05-070221

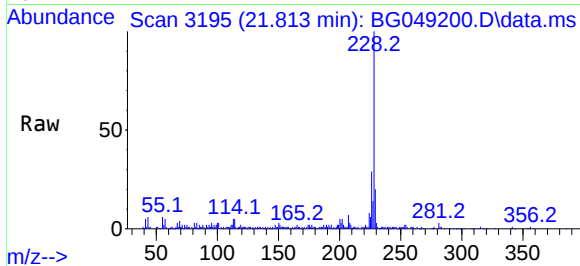


Tgt Ion:228 Resp: 106729
Ion Ratio Lower Upper
228 100
226 29.2 23.1 34.7
229 20.4 15.3 22.9

Manual Integrations
APPROVED



mohammad
7/8/2021 12:40:22 PM

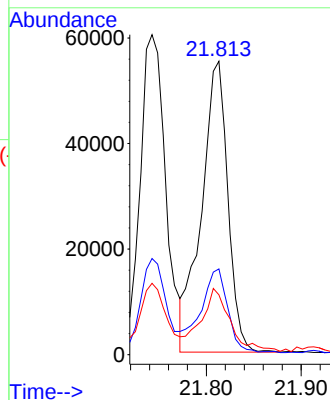


#86
Perylene-d12
Concen: 20.000 ng
RT: 25.074 min Scan# 3750
Delta R.T. 0.009 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21

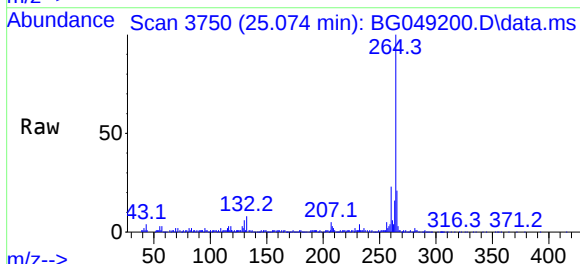


Tgt Ion:264 Resp: 254671
Ion Ratio Lower Upper
264 100
260 23.4 19.4 29.2
265 21.1 16.9 25.3


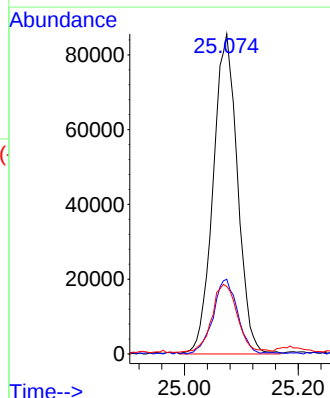



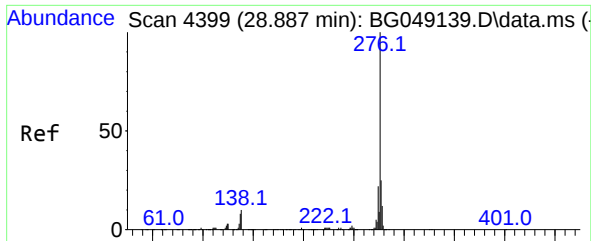


#87
Indeno(1,2,3-cd)pyrene
Concen: 3.124 ng
RT: 28.840 min Scan# 4391
Delta R.T. -0.020 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21

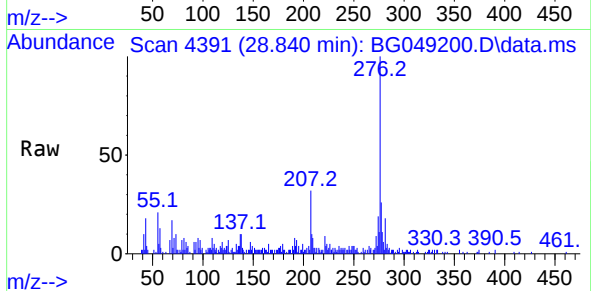



Tgt Ion:276 Resp: 63476
Ion Ratio Lower Upper
276 100
138 5.1 5.1 7.7
277 24.6 19.8 29.6

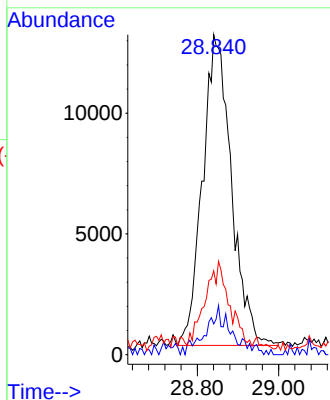

#88
Benzo(b)fluoranthene
Concen: 6.940 ng
RT: 24.022 min Scan# 3571
Delta R.T. 0.003 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21

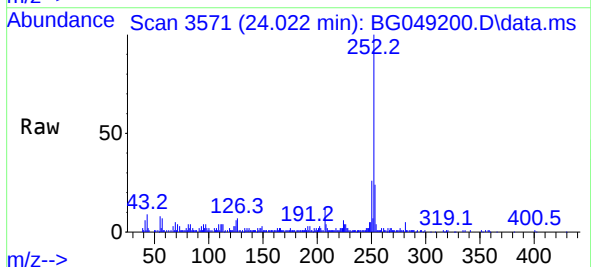


Tgt Ion:252 Resp: 127545
Ion Ratio Lower Upper
252 100
253 24.4 16.2 24.4#
125 6.3 3.0 4.4#

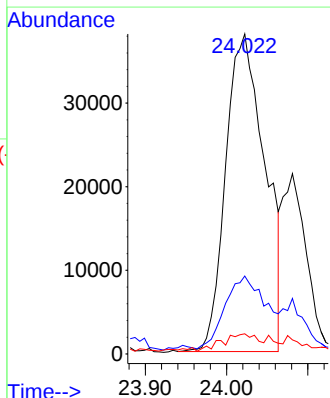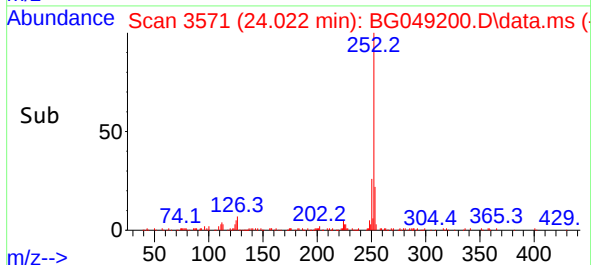

Instrument :
BNA_G
ClientSampleId :
TR-05-070221

Manual Integrations
APPROVED

mohammad
7/8/2021 12:40:22 PM







#89
Benzo(k)fluoranthene
Concen: 2.523 ng m
RT: 24.081 min Scan# 3581
Delta R.T. -0.008 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21

Tgt Ion:252 Resp: 44239
Ion Ratio Lower Upper
252 100
253 30.8 18.0 27.0#
125 7.8 3.1 4.7#

Instrument :
BNA_G
ClientSampleId :
TR-05-070221




Manual Integrations
APPROVED


mohammad
7/8/2021 12:40:22 PM

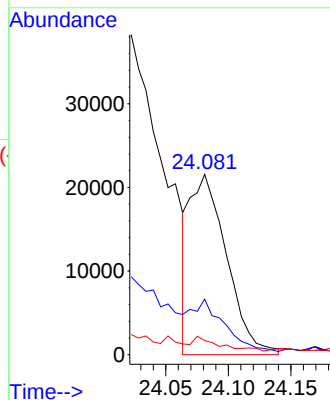

#90
Benzo(a)pyrene
Concen: 5.829 ng
RT: 24.910 min Scan# 3722
Delta R.T. -0.002 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21

Tgt Ion:252 Resp: 98825
Ion Ratio Lower Upper
252 100
253 23.5 16.6 25.0
125 6.7 3.5 5.3#

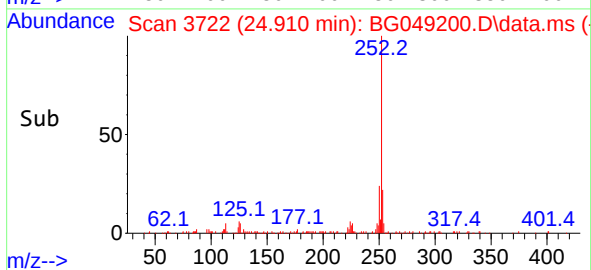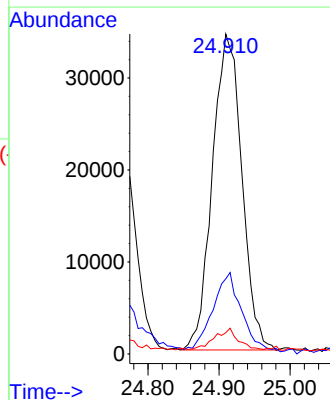



#92
Benzo(g,h,i)perylene
Concen: 3.692 ng
RT: 30.033 min Scan# 4594
Delta R.T. -0.002 min
Lab File: BG049200.D
Acq: 7 Jul 2021 15:21

Tgt Ion: 276 Resp: 62428
Ion Ratio Lower Upper
276 100
277 21.3 18.4 27.6
138 9.0 7.0 10.6

Instrument :
BNA_G
ClientSampleId :
TR-05-070221

Manual Integrations
APPROVED

mohammad
7/8/2021 12:40:22 PM

