


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070721\
 Data File : BG049194.D
 Acq On : 7 Jul 2021 11:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 06 10:59:02 2021

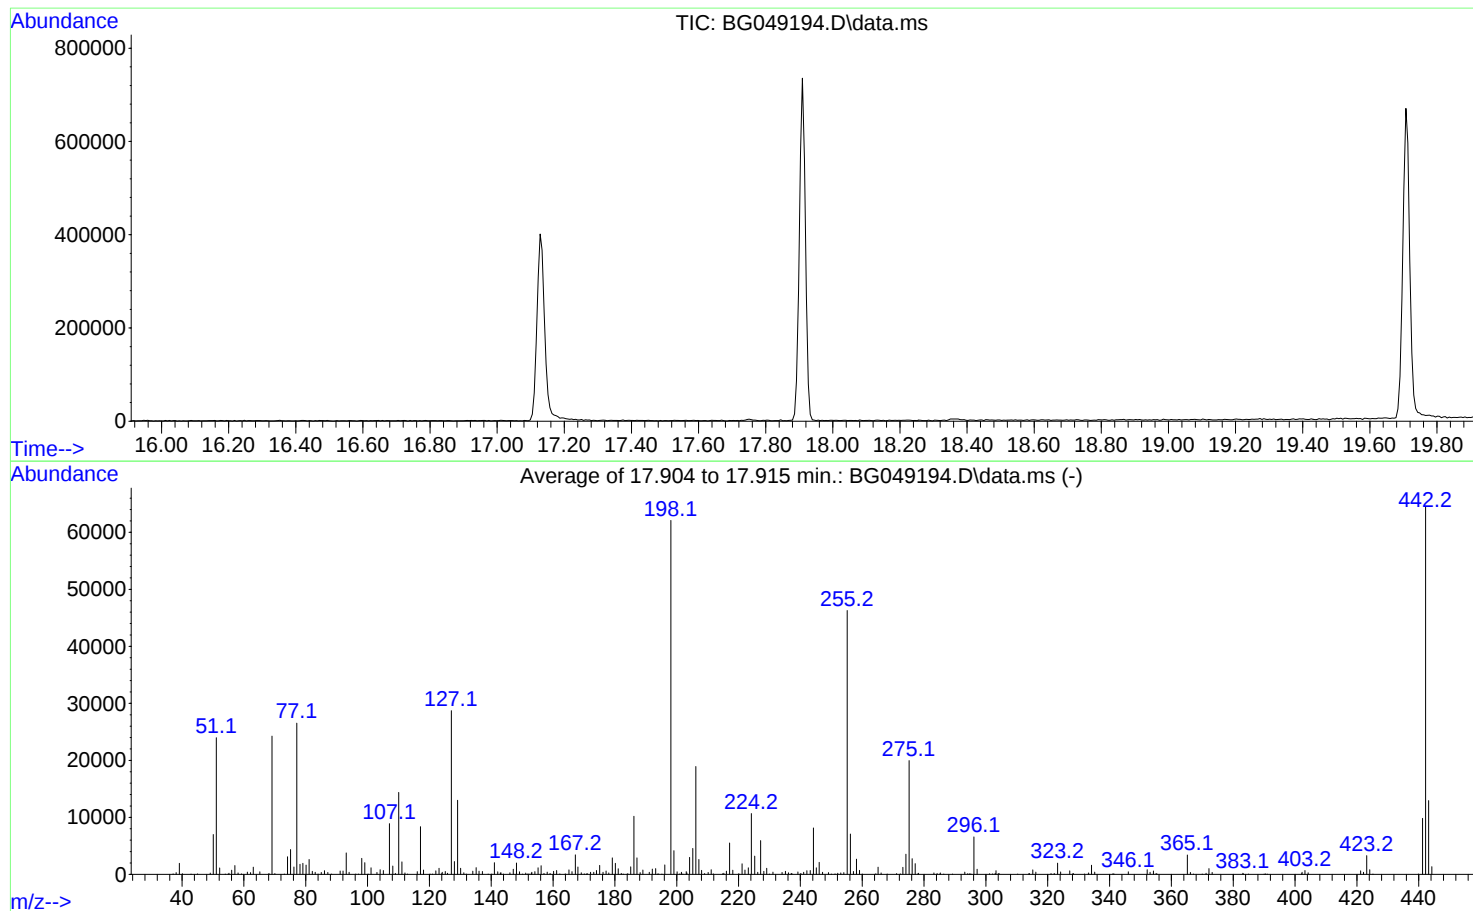




AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2522

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	23981	PASS
68	69	0.00	2	0.7	178	PASS
69	198	0.00	100	39.0	24240	PASS
70	69	0.00	2	0.6	135	PASS
127	198	10	80	46.3	28712	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62080	PASS
199	198	5	9	6.7	4149	PASS
275	198	10	60	32.2	19971	PASS
365	198	1	100	5.5	3387	PASS
441	198	0.01	100	15.8	9829	PASS
442	442	100	100	100.0	64533	PASS
443	442	15	24	20.1	12950	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070721\
Data File : BG049194.D
Acq On : 7 Jul 2021 11:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 07 11:58:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 06 10:59:02 2021
Response via : Initial Calibration

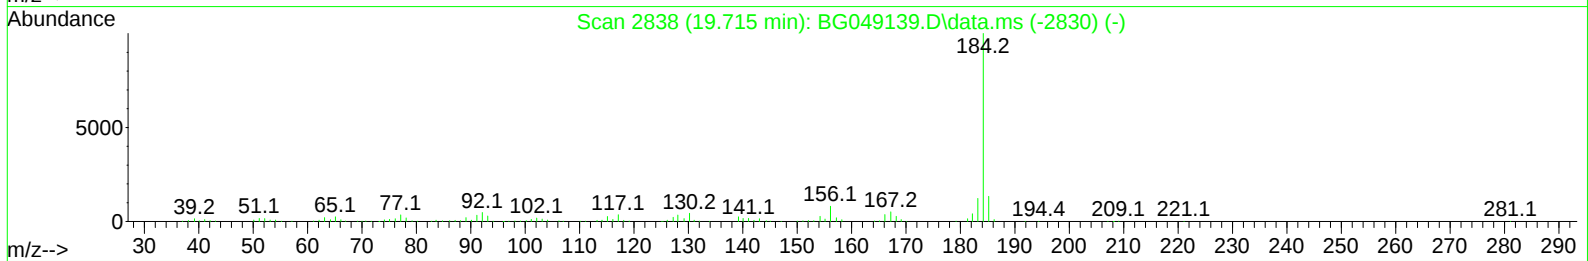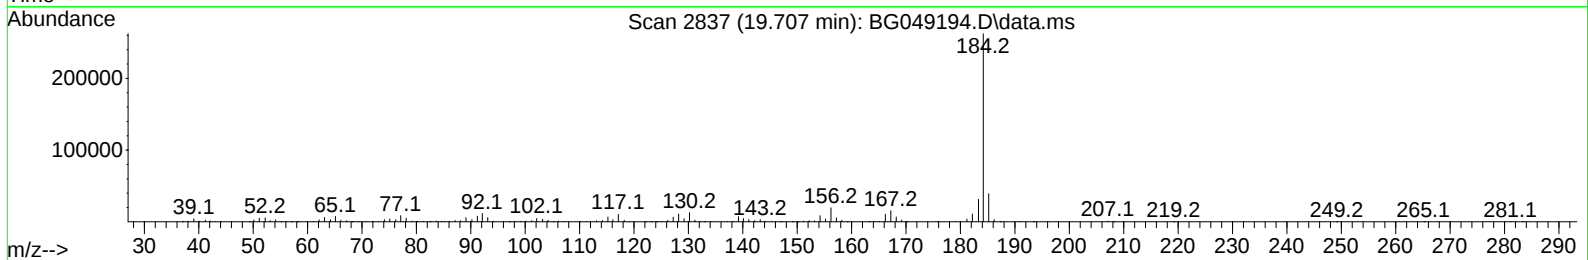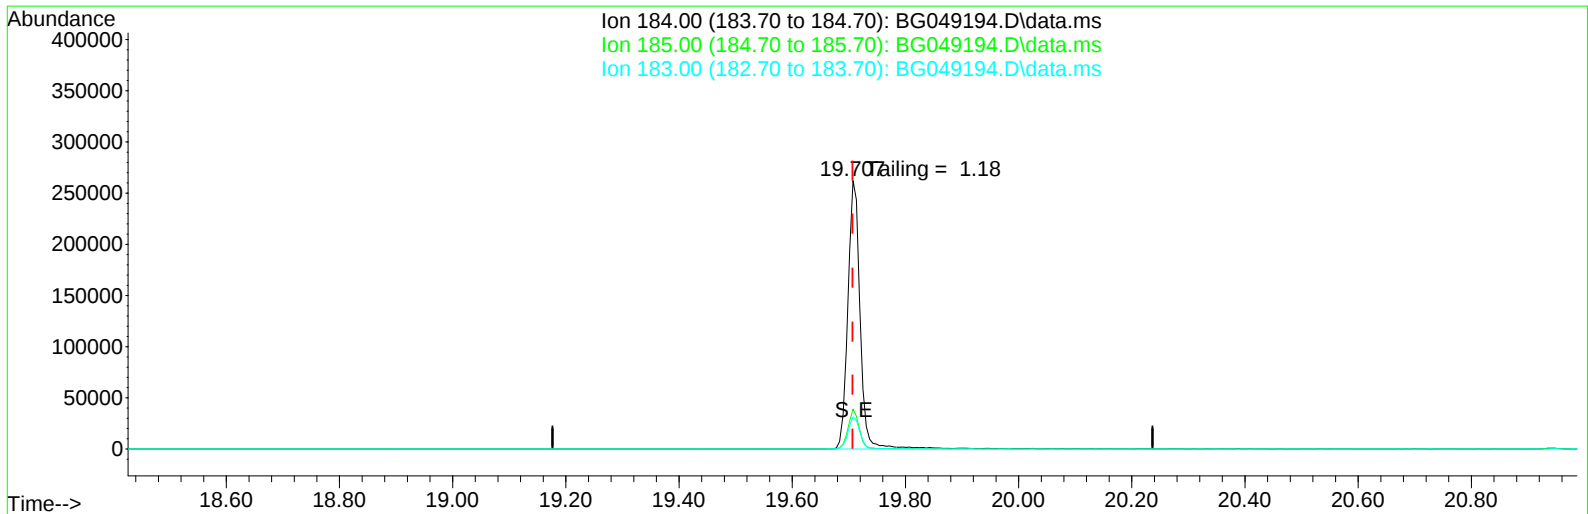

TIC: BG049194.D\data.ms

(77) Benzidine

19.707min (+ 0.001) 328478.20 ng




response 388059

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.93
183.00	11.70	11.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070721\
Data File : BG049194.D
Acq On : 7 Jul 2021 11:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 07 11:58:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 06 10:59:02 2021
Response via : Initial Calibration

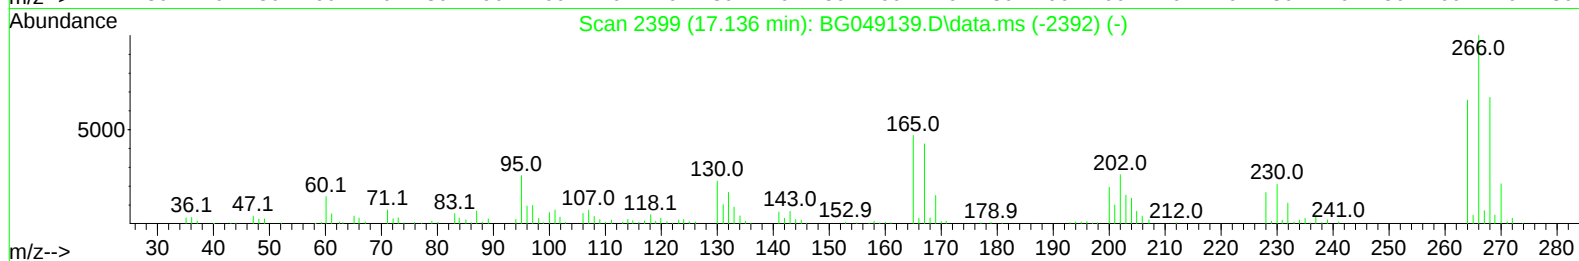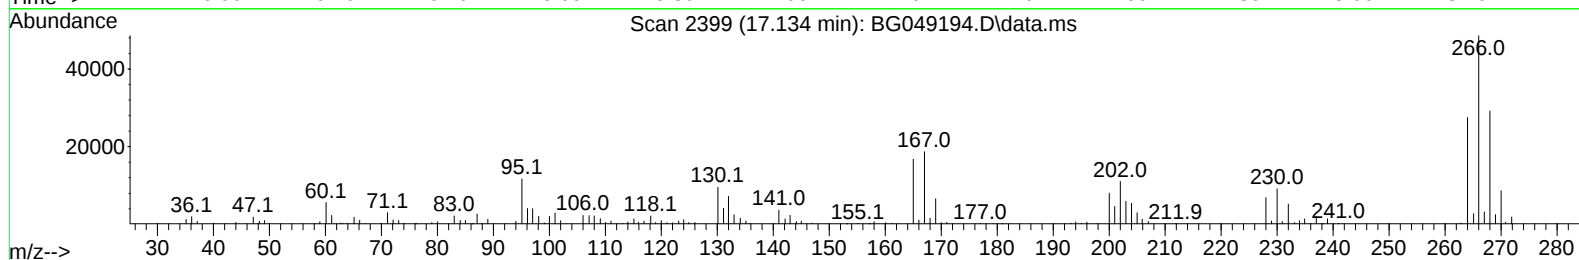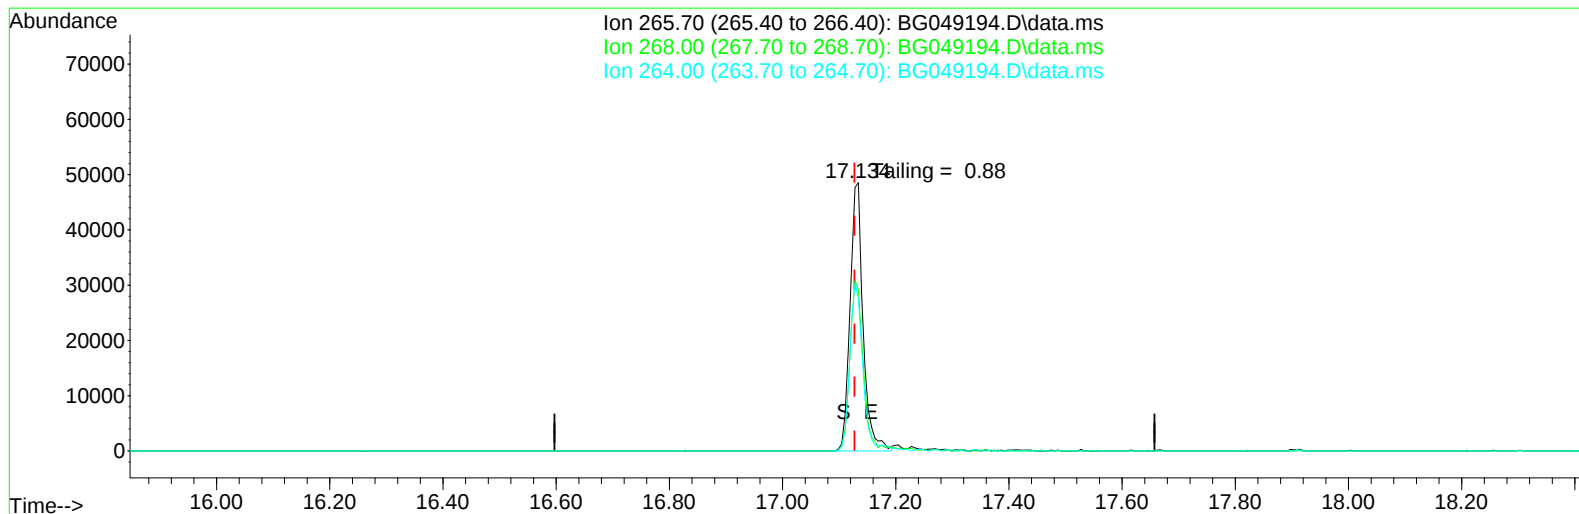

TIC: BG049194.D\data.ms

(70) Pentachlorophenol (C)

17.134min (+ 0.007) 27119.77 ng

response 77460

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	60.09
264.00	61.30	56.65
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/7/2021	BNA_G	BG049194.D
Compound Name	Response	Retention Time
DDT	210258	20.94
DDD	4230	20.5
DDE	948	20.5
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5178	215436	2.40