
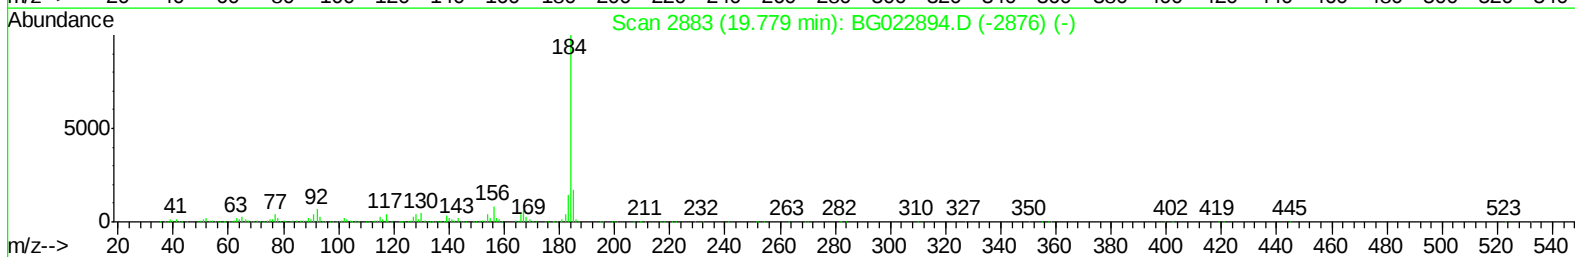
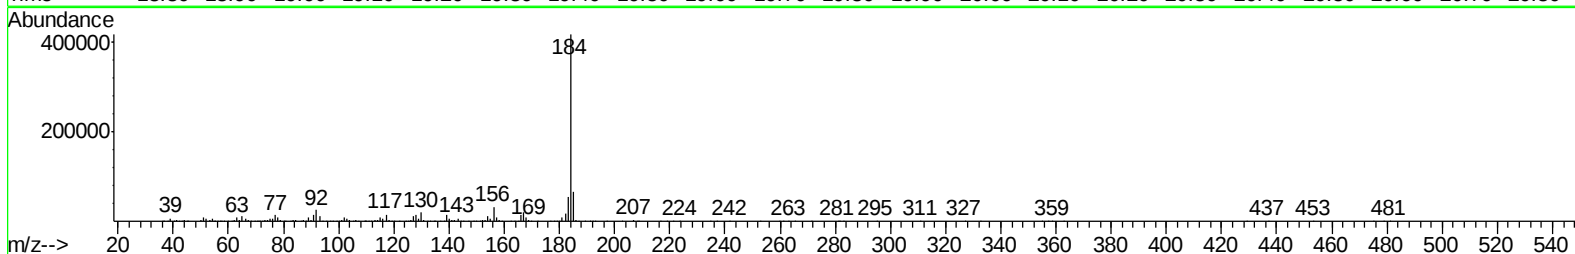


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070816\
Data File : BG022889.D
Acq On : 7 Jul 2016 9:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 07:24:08 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 16:51:07 2016
Response via : Initial Calibration

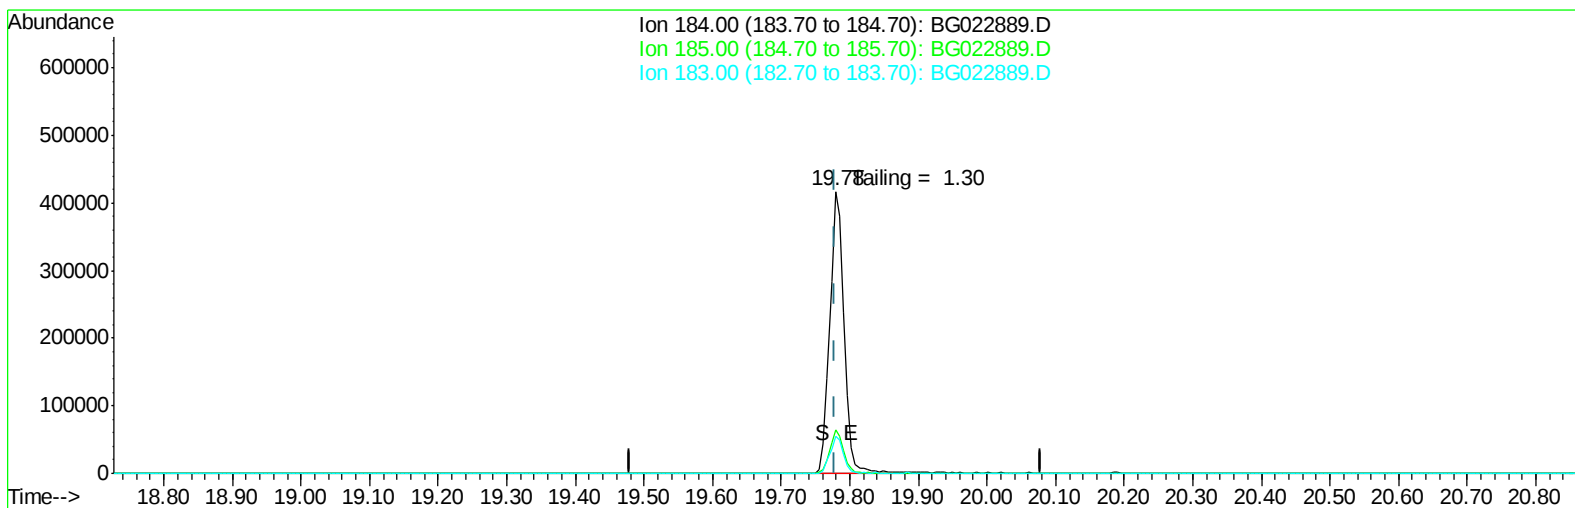

TIC: BG022889.D

(76) Benzidine




19.779min (-0.001) 376339.34ng

response 604191

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.56
183.00	13.40	13.07
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070816\
Data File : BG022889.D
Acq On : 7 Jul 2016 9:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 07:24:08 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 16:51:07 2016
Response via : Initial Calibration

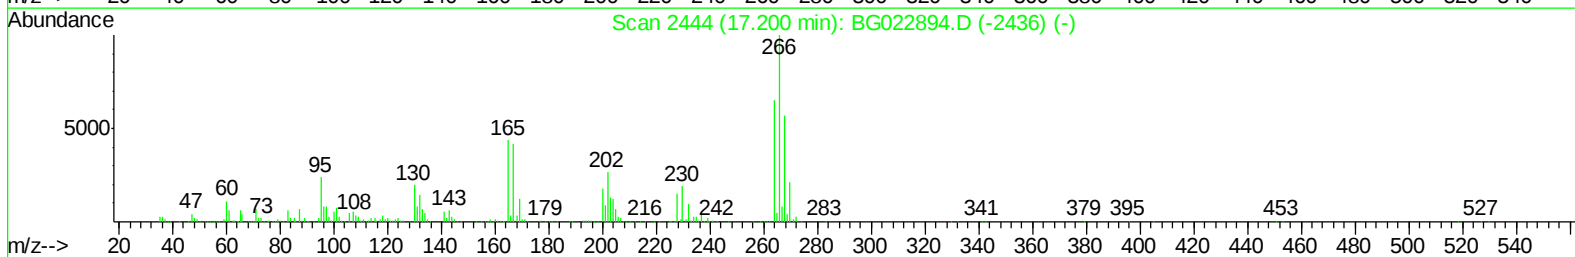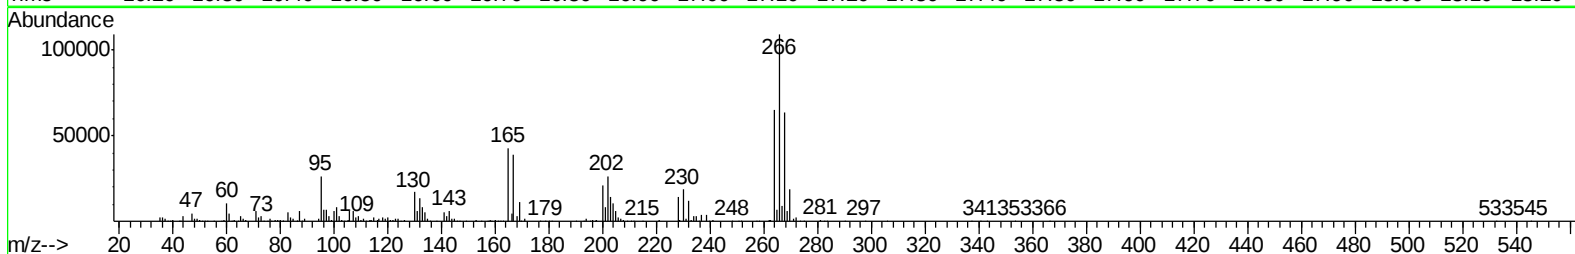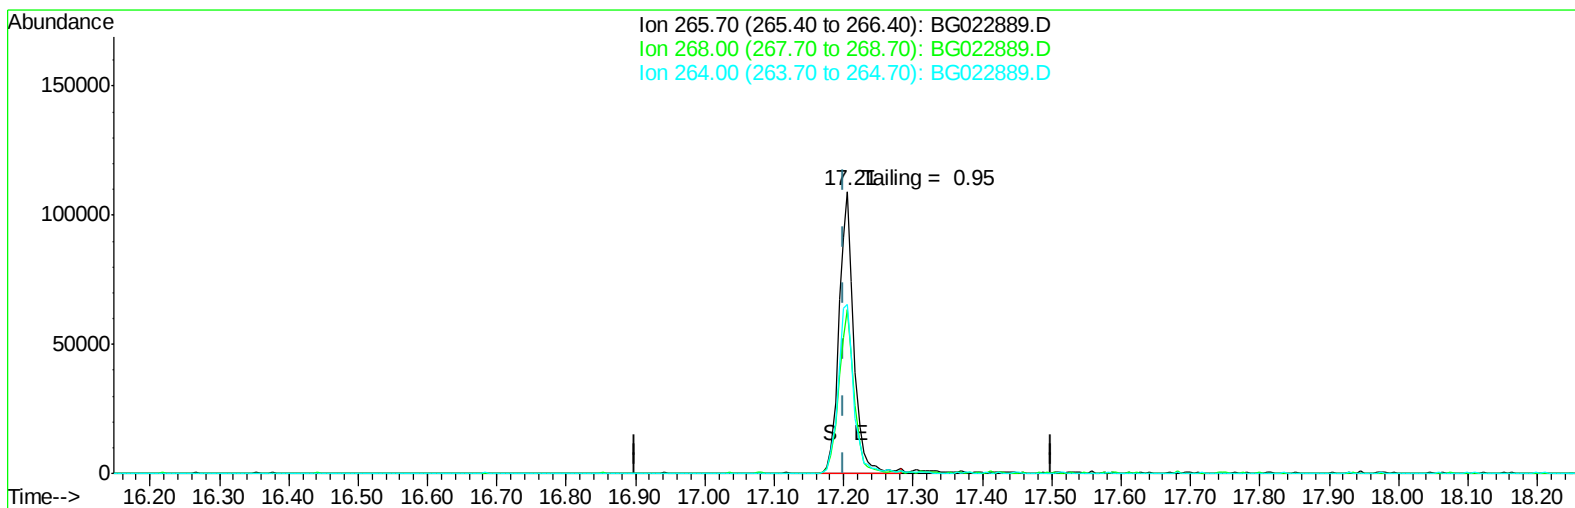

TIC: BG022889.D

(69) Pentachlorophenol (C)

17.205min (+0.005) 149870.79ng

response 162009

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	58.13
264.00	63.20	59.90
0.00	0.00	0.00