
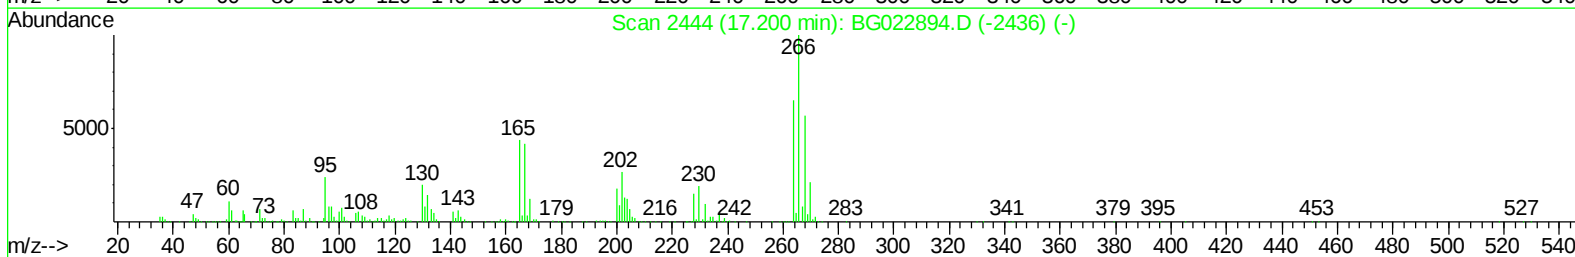
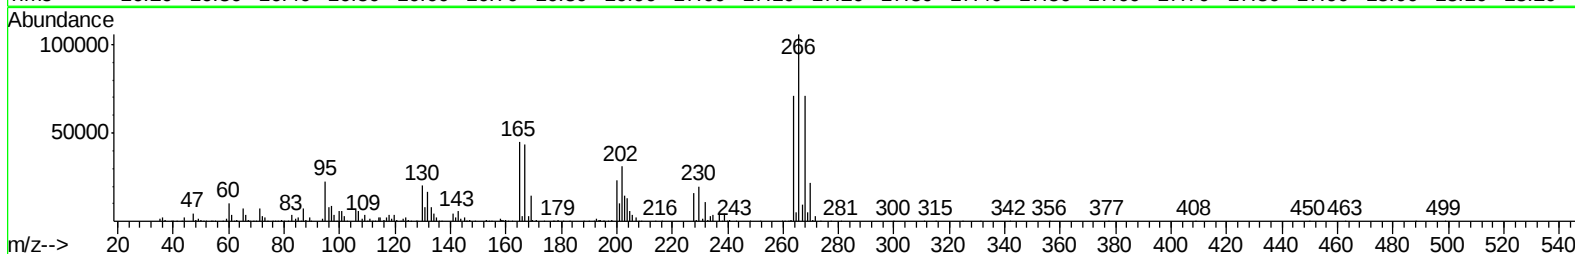


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070816\
Data File : BG022899.D
Acq On : 7 Jul 2016 17:21
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 07:25:01 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 16:51:07 2016
Response via : Initial Calibration

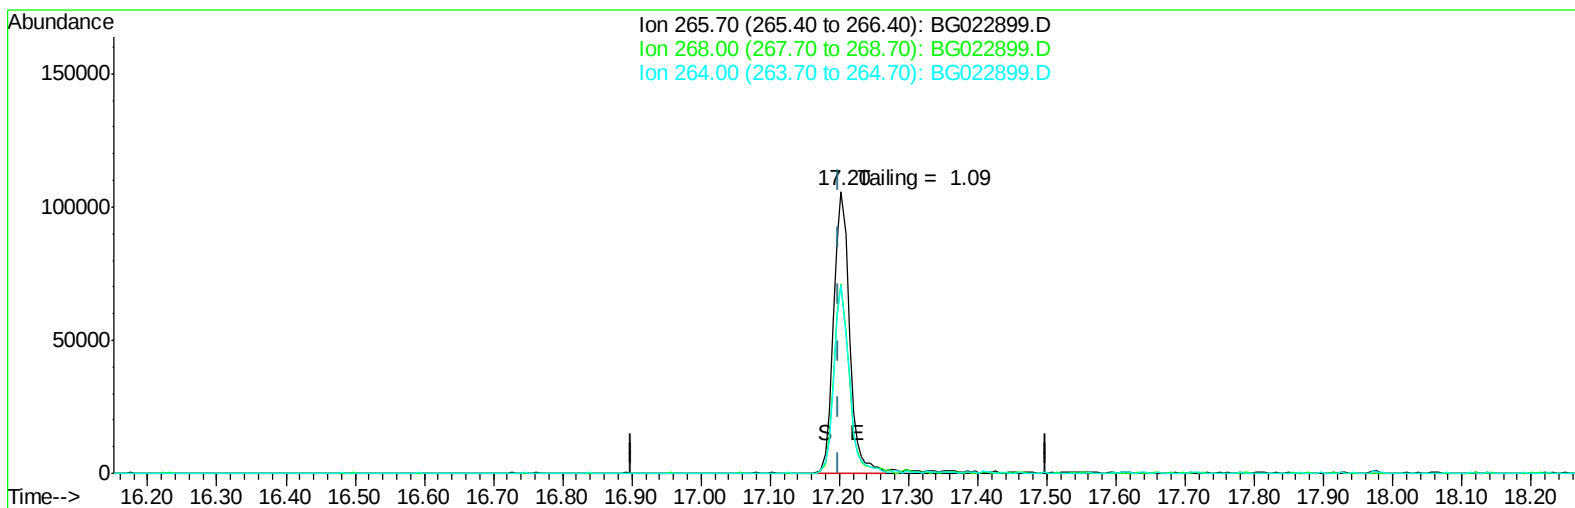

TIC: BG022899.D

(69) Pentachlorophenol (C)




17.203min (+0.003) 187393.83ng

response 168237

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	67.41
264.00	63.20	66.87
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070816\
Data File : BG022899.D
Acq On : 7 Jul 2016 17:21
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 07:25:01 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 16:51:07 2016
Response via : Initial Calibration

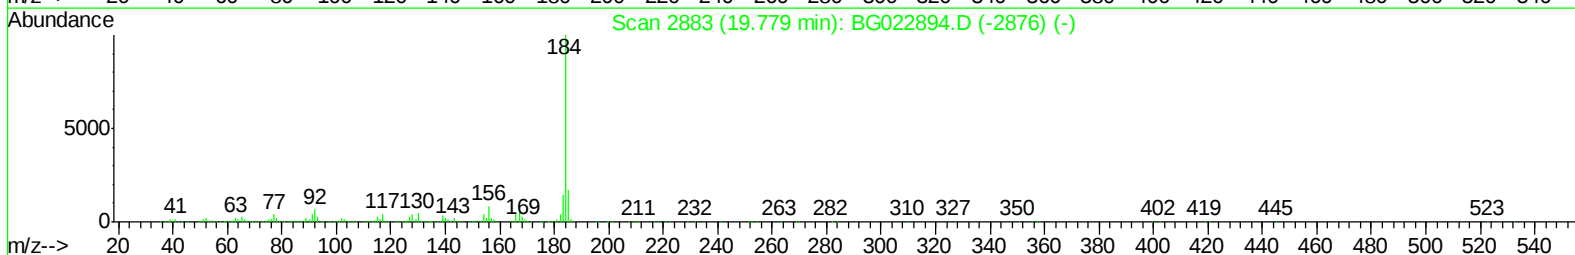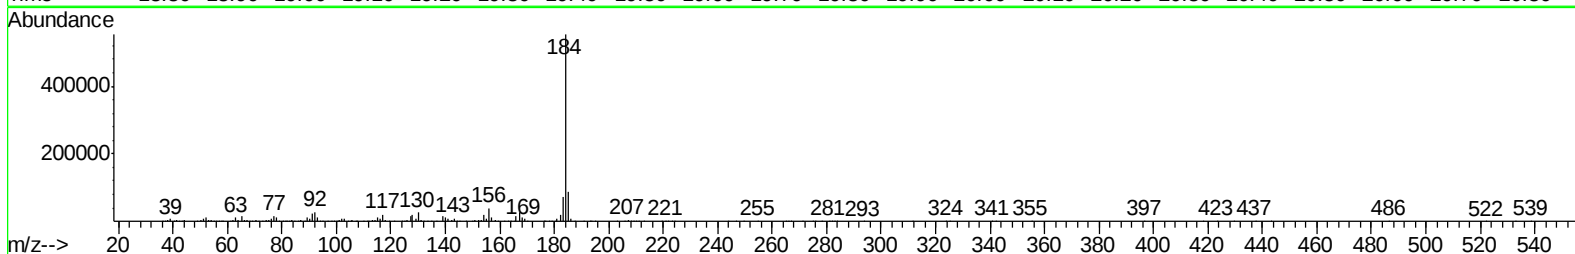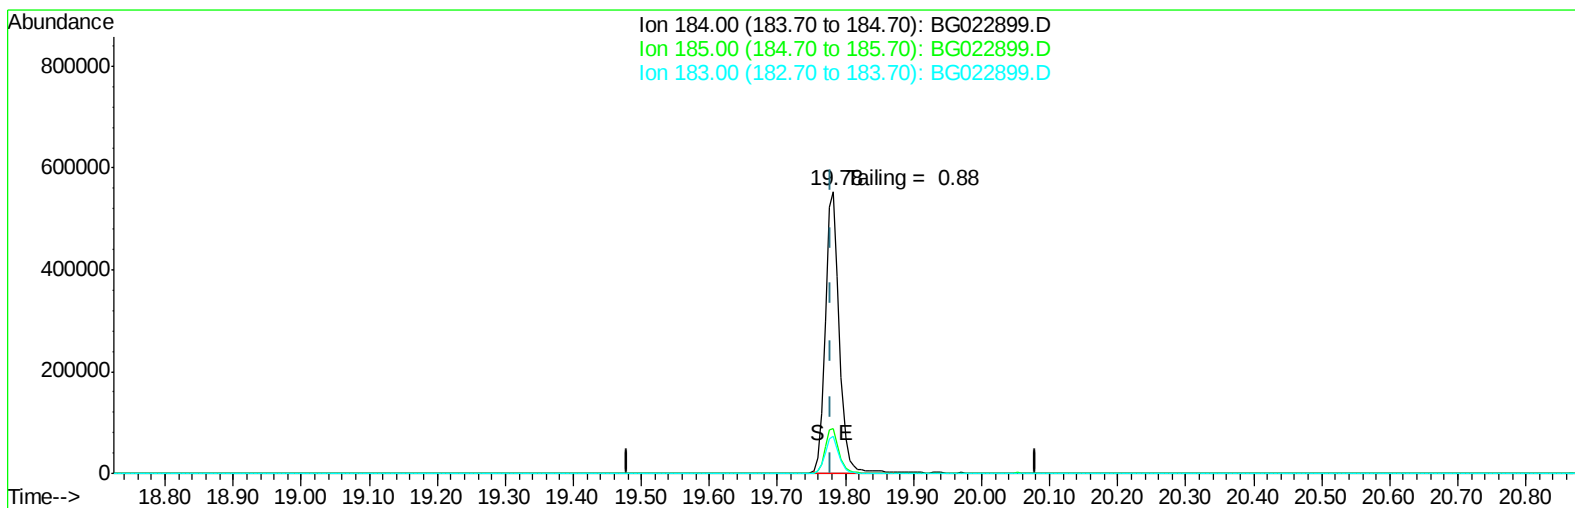

TIC: BG022899.D

(76) Benzidine

19.782min (+0.003) 153901.37ng

response 798597

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	16.02
183.00	13.40	13.36
0.00	0.00	0.00