
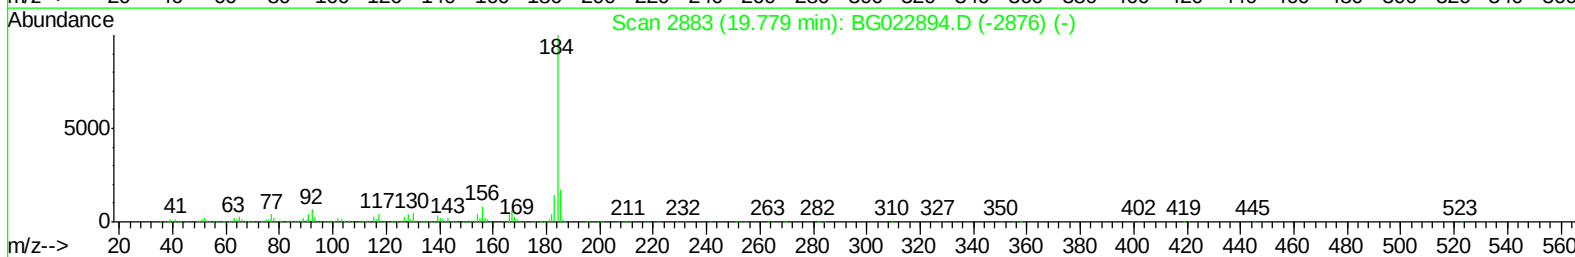
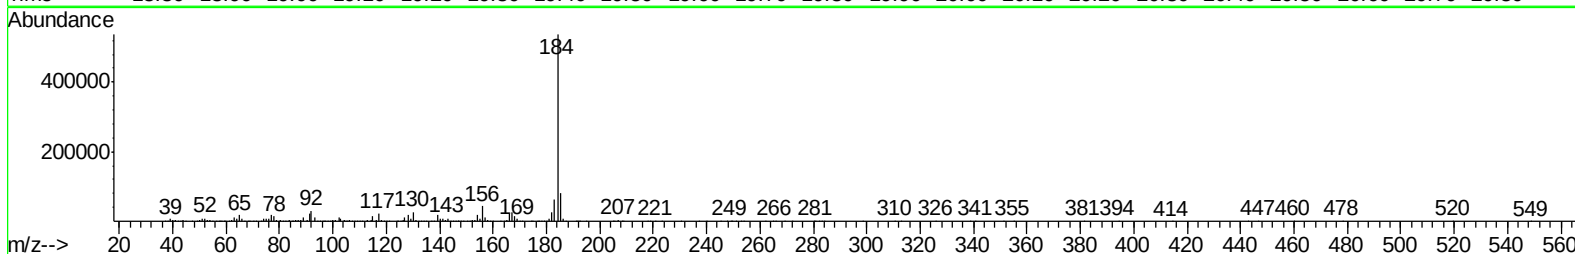


Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG070816\  
Data File : BG022917.D  
Acq On : 8 Jul 2016 5:23  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 07:26:02 2016  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG070816.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 07 16:51:07 2016  
Response via : Initial Calibration

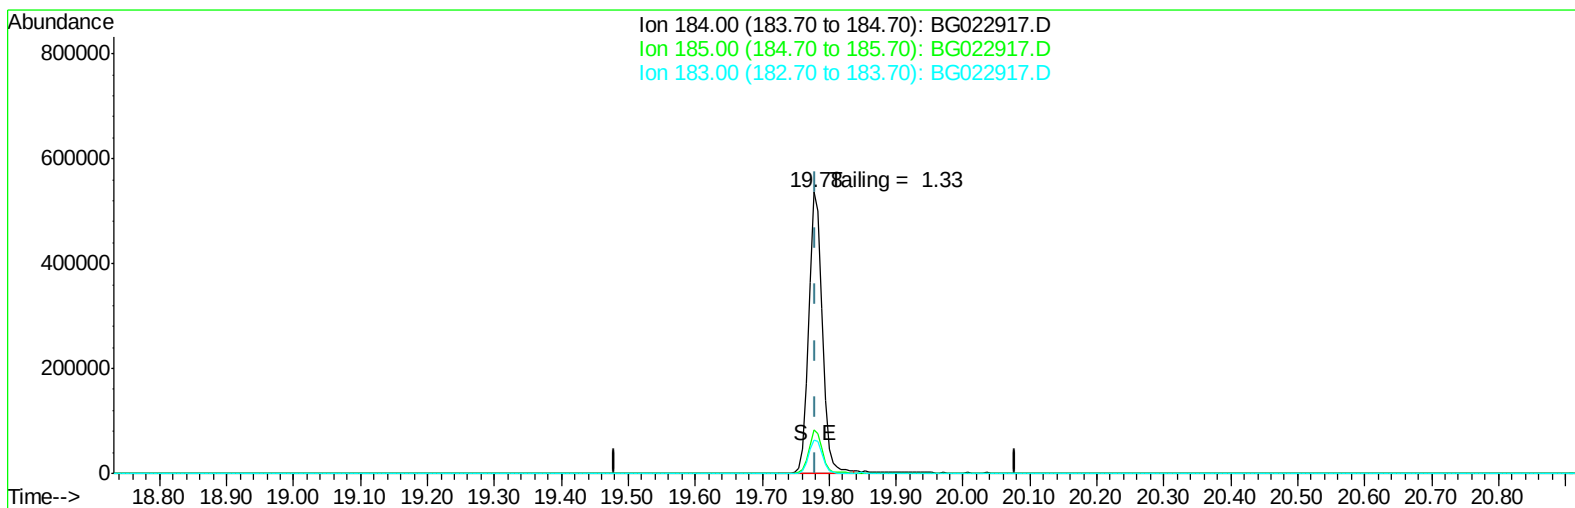

TIC: BG022917.D

(76) Benzidine




19.777min (-0.002) 113209.47ng

response 785425

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.80 | 15.25 |
| 183.00 | 13.40 | 11.82 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG070816\  
Data File : BG022917.D  
Acq On : 8 Jul 2016 5:23  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 07:26:02 2016  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG070816.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 07 16:51:07 2016  
Response via : Initial Calibration

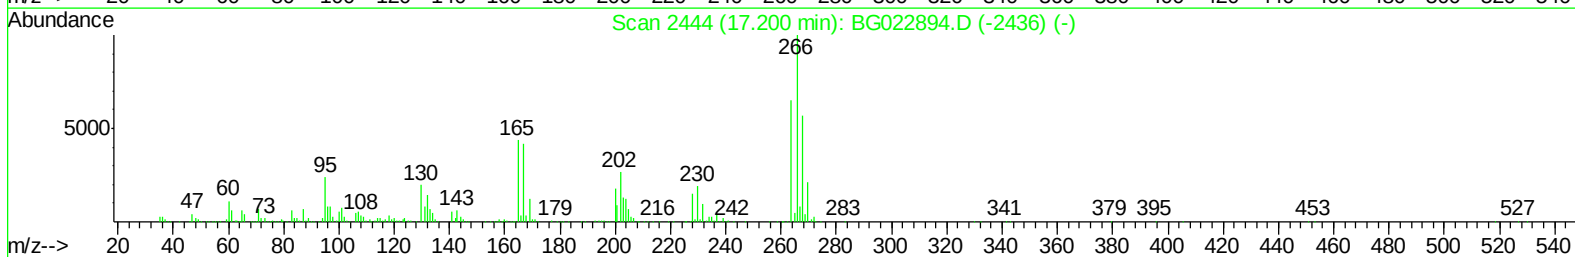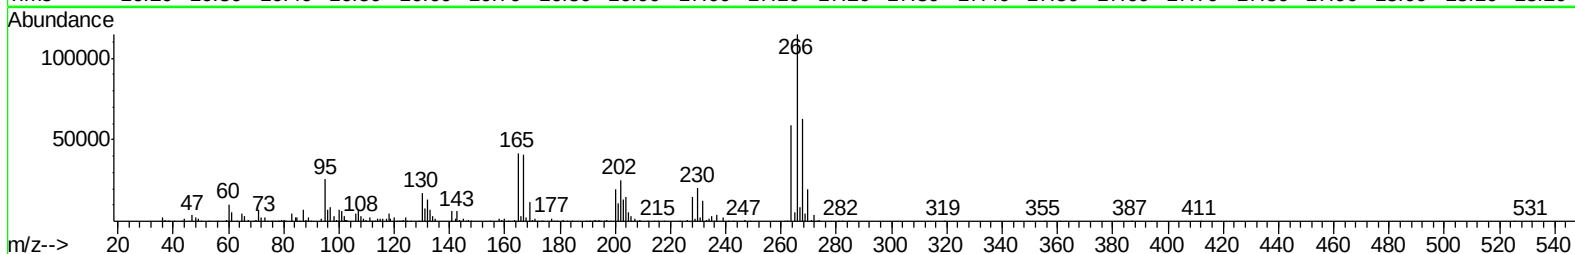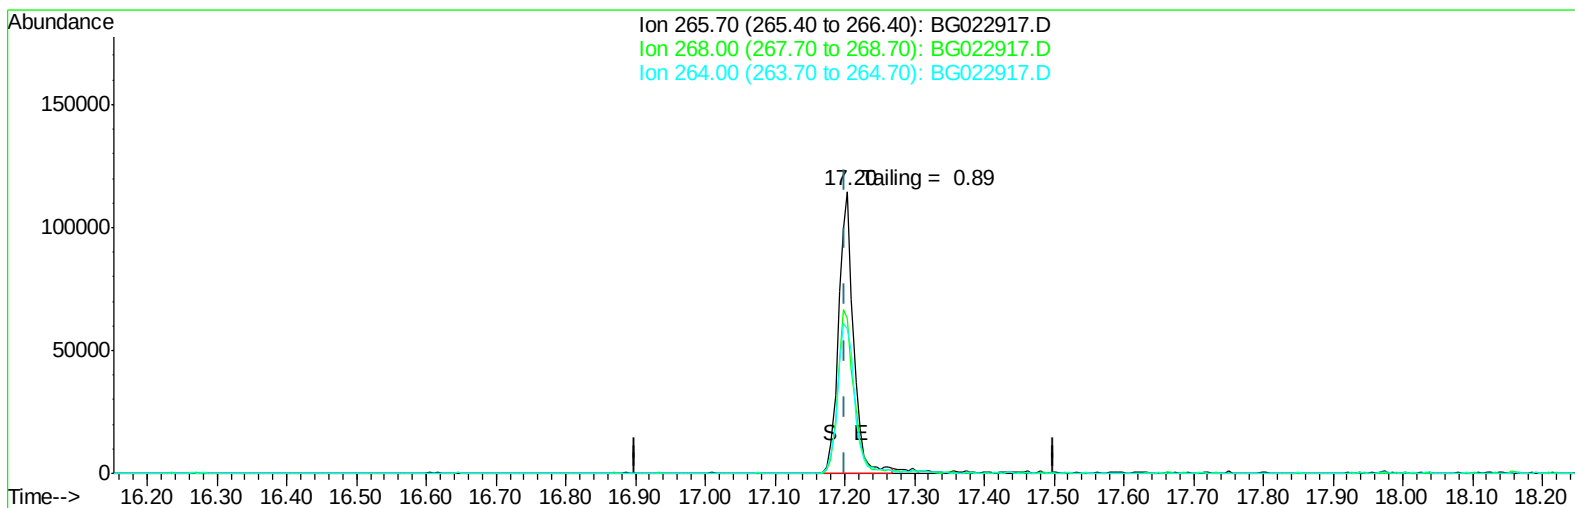

TIC: BG022917.D

(69) Pentachlorophenol (C)

17.204min (+0.004) 297636.30ng

response 169051

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.90 | 54.94 |
| 264.00 | 63.20 | 51.19 |
| 0.00   | 0.00  | 0.00  |