


Data Path : Z:\HPCHEM1\BNA G\DATA\BG070816\
 Data File : BG022889.D
 Acq On : 7 Jul 2016 9:27
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 07 16:51:07 2016

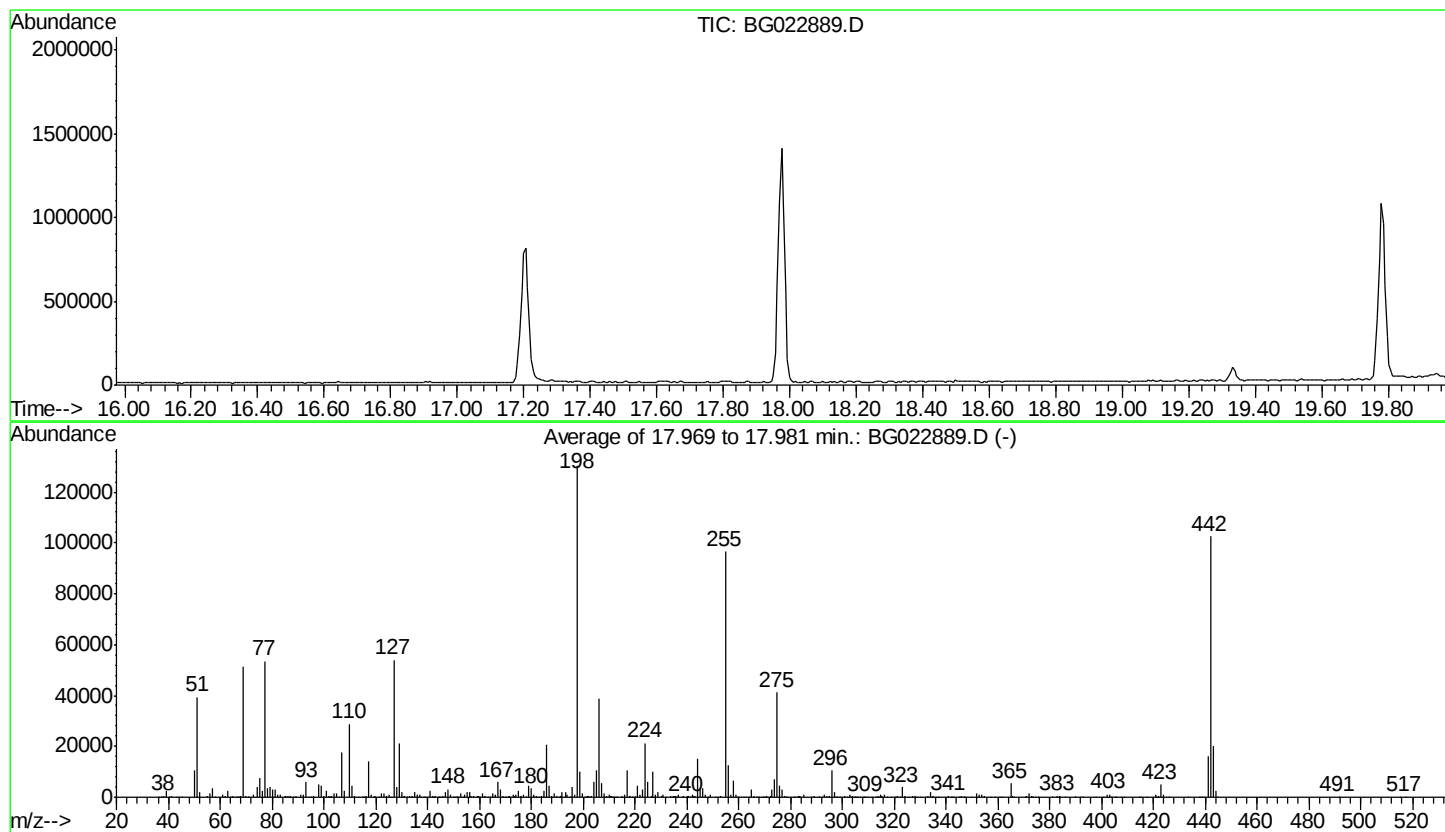

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.3	39466	PASS
68	69	0.00	2	0.8	411	PASS
69	198	0.00	100	39.4	51336	PASS
70	69	0.00	2	0.5	279	PASS
127	198	10	80	41.4	53941	PASS
197	198	0.00	2	0.8	1001	PASS
198	198	100	100	100.0	130354	PASS
199	198	5	9	7.9	10238	PASS
275	198	10	60	31.6	41210	PASS
365	198	1	100	4.1	5345	PASS
441	442	0.01	24	15.6	15971	PASS
442	198	50	100	78.7	102544	PASS
443	442	15	24	19.8	20338	PASS