


Data Path : Z:\HPCHEM1\BNA G\DATA\BG070816\
 Data File : BG022917.D
 Acq On : 8 Jul 2016 5:23
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 07 16:51:07 2016

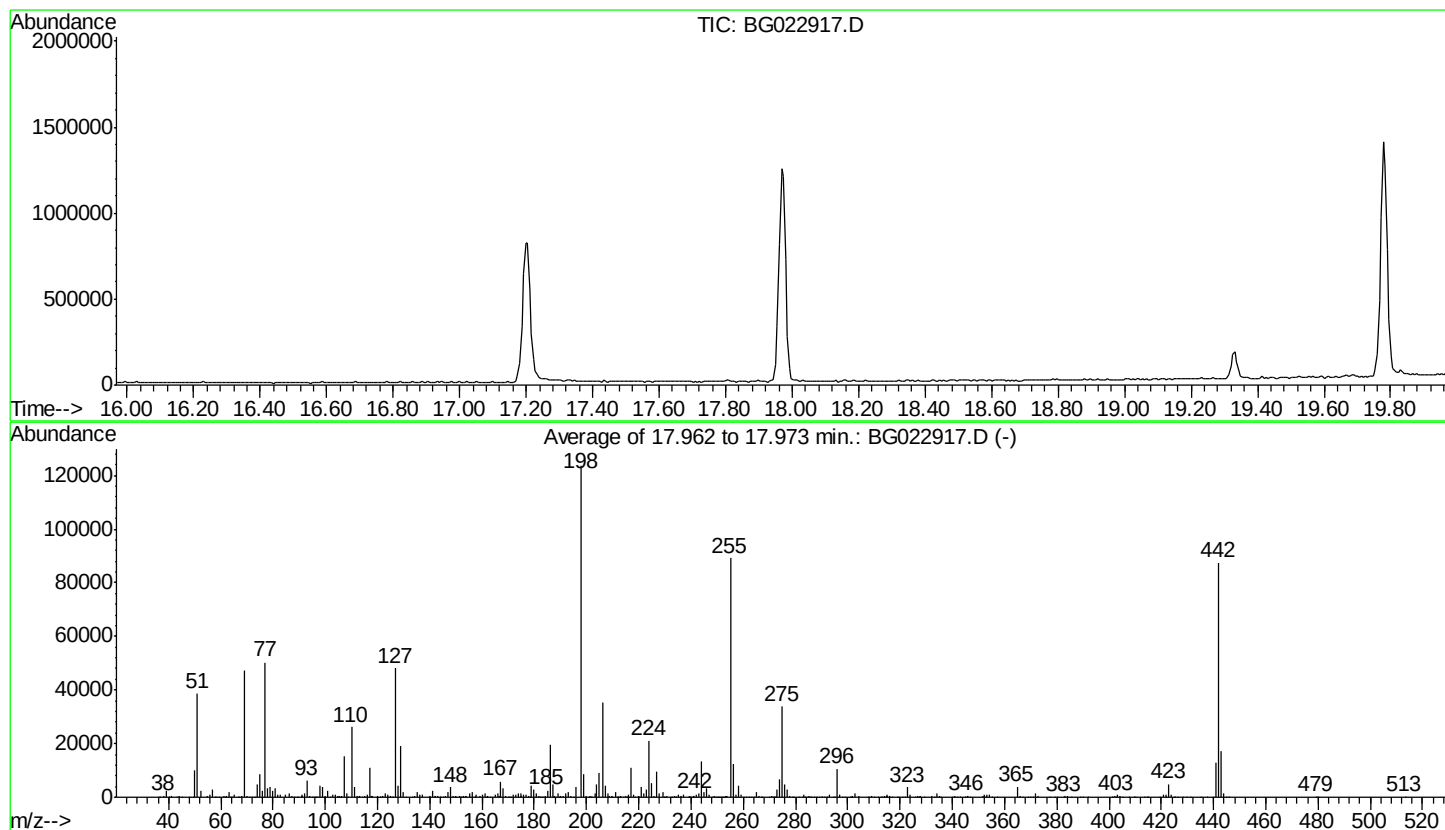

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	38504	PASS
68	69	0.00	2	1.1	539	PASS
69	198	0.00	100	38.3	47304	PASS
70	69	0.00	2	0.8	365	PASS
127	198	10	80	38.9	48130	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	123656	PASS
199	198	5	9	6.9	8541	PASS
275	198	10	60	27.4	33840	PASS
365	198	1	100	3.2	3906	PASS
441	442	0.01	24	15.0	13099	PASS
442	198	50	100	70.8	87498	PASS
443	442	15	24	19.5	17033	PASS