
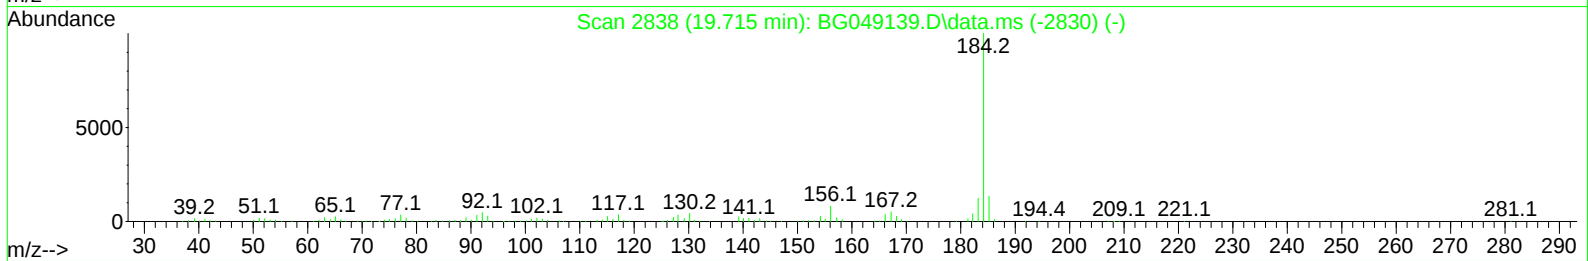
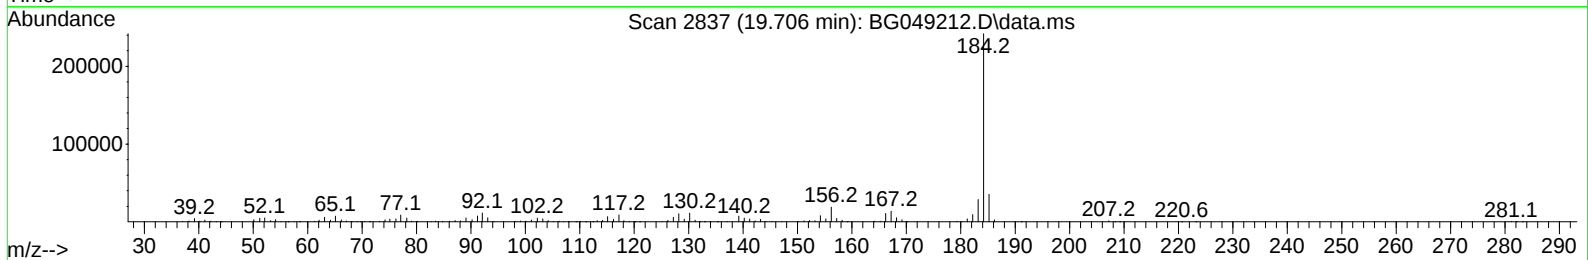


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070821\
Data File : BG049212.D
Acq On : 8 Jul 2021 9:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 11:55:04 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 06 10:59:02 2021
Response via : Initial Calibration

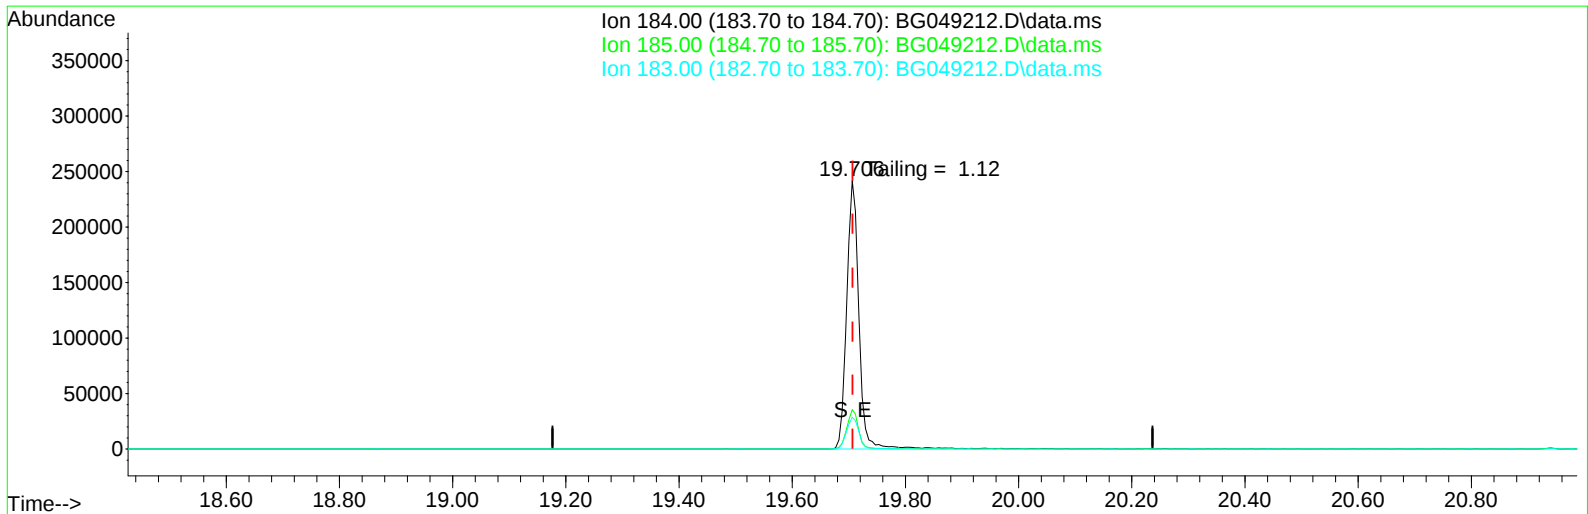

TIC: BG049212.D\data.ms

(77) Benzidine




19.706min (-0.000) 0.00 ng

response 355352

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.68
183.00	11.70	11.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070821\
Data File : BG049212.D
Acq On : 8 Jul 2021 9:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 11:55:04 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 06 10:59:02 2021
Response via : Initial Calibration

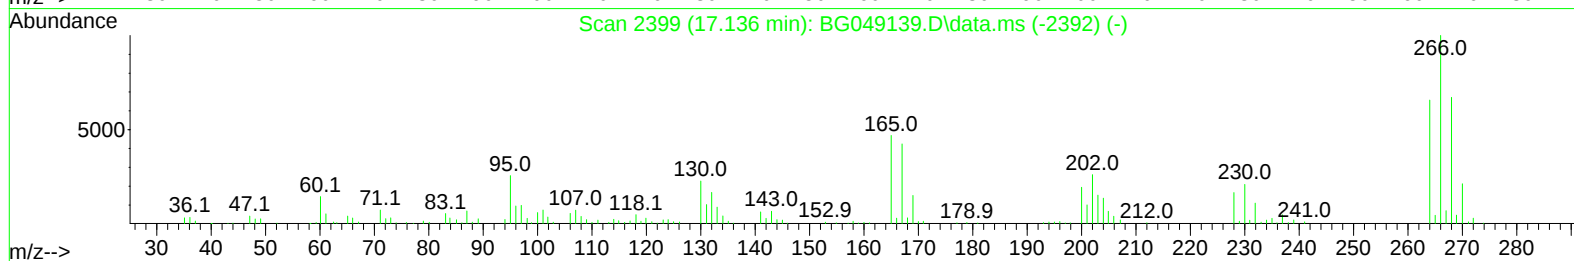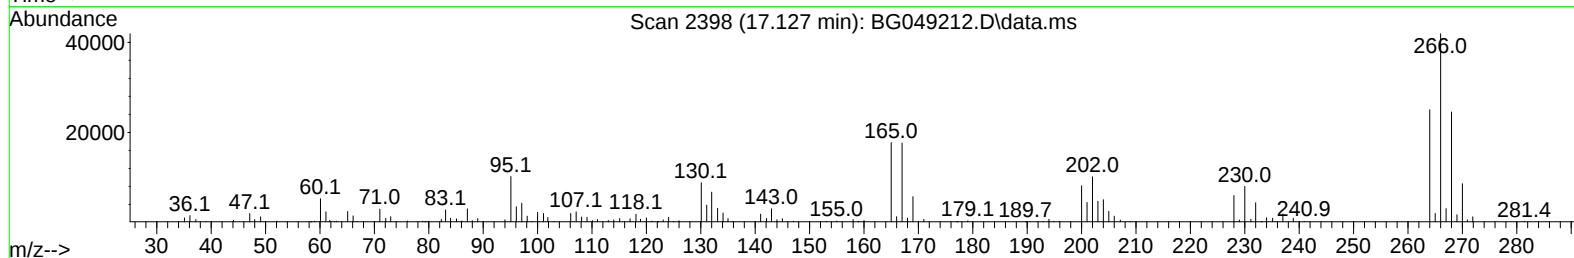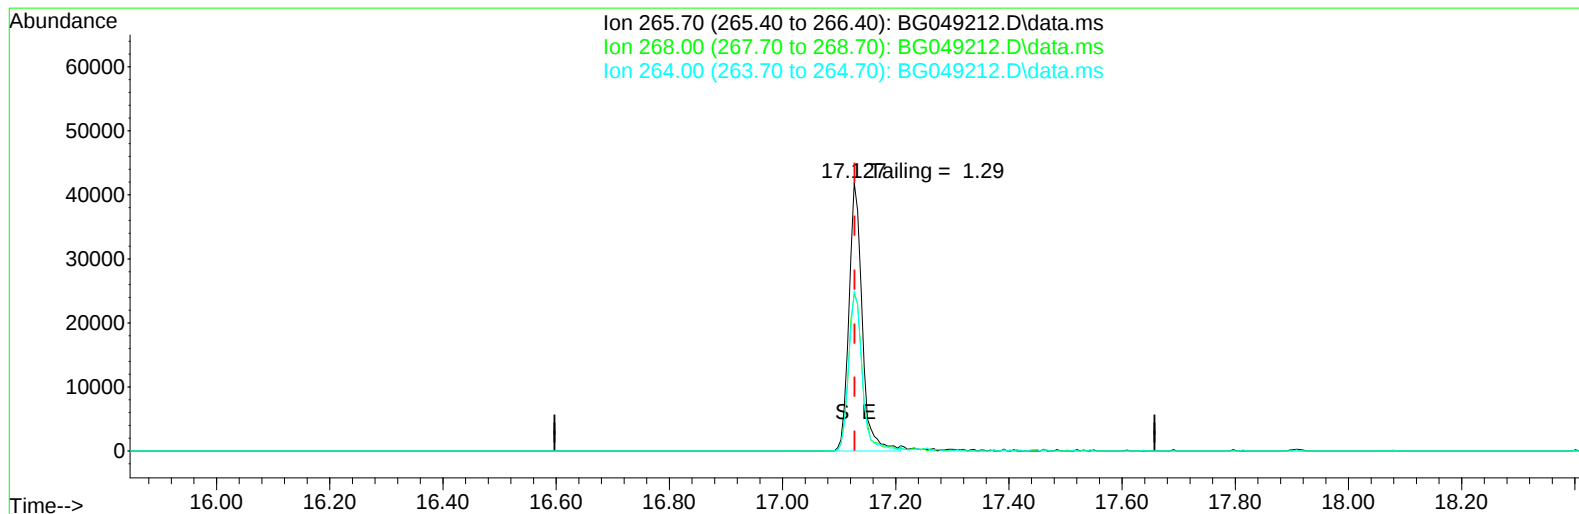

TIC: BG049212.D\data.ms

(70) Pentachlorophenol (C)

17.127min (-0.000) 28914.57 ng

response 67525

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	58.50
264.00	61.30	59.69
0.00	0.00	0.00