

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070822\
 Data File : BG054246.D
 Acq On : 8 Jul 2022 14:34
 Operator : CG/JU
 Sample : N3622-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 20220496A-SIM-C2A-COMPOSITE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG054246.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.632	375	382	391	rBV	224579	380997	23.61%	6.123%
2	7.230	645	654	668	rBV	232902	422723	26.19%	6.794%
3	8.065	788	796	805	rBV	47852	85787	5.32%	1.379%
4	9.222	984	993	1004	rBV	140971	263848	16.35%	4.241%
5	10.873	1265	1274	1281	rBV	68158	124879	7.74%	2.007%
6	13.311	1682	1689	1697	rBV	460849	725193	44.93%	11.655%
7	14.686	1917	1923	1931	rBV	135515	223047	13.82%	3.585%
8	16.179	2170	2177	2186	rBV2	530242	859865	53.27%	13.820%
9	17.436	2384	2391	2405	rVV	222282	363934	22.55%	5.849%
10	18.317	2537	2541	2550	rBV6	14301	28756	1.78%	0.462%
11	19.486	2734	2740	2745	rBV	14793	26218	1.62%	0.421%
12	19.845	2797	2801	2810	rVB2	23079	40345	2.50%	0.648%
13	20.039	2828	2834	2843	rVB	1171454	1614034	100.00%	25.941%
14	20.338	2878	2885	2890	rVB6	9034	18569	1.15%	0.298%
15	21.337	3050	3055	3060	rBV3	24695	41102	2.55%	0.661%
16	21.590	3095	3098	3104	rVB6	11929	17298	1.07%	0.278%
17	21.707	3111	3118	3130	rVB	281561	500298	31.00%	8.041%
18	24.962	3662	3672	3685	rVB2	159839	485079	30.05%	7.796%




Sum of corrected areas: 6221972

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070822\
Data File : BG054246.D
Acq On : 8 Jul 2022 14:34
Operator : CG/JU
Sample : N3622-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20220496A-SIM-C2A-COMPOSITE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

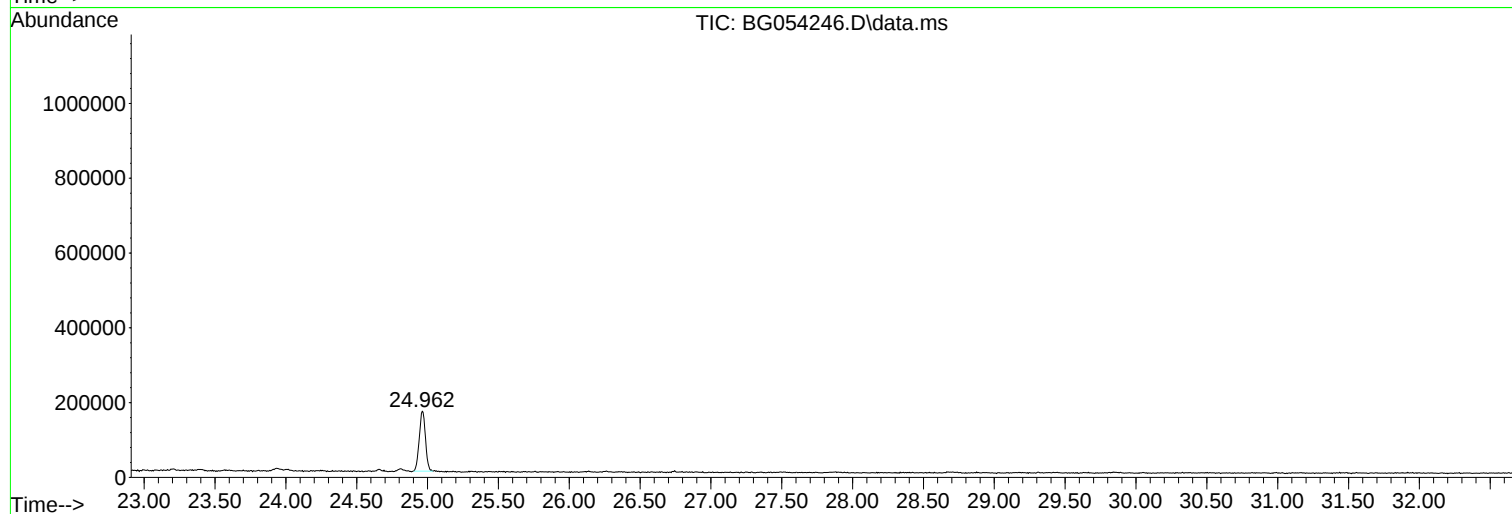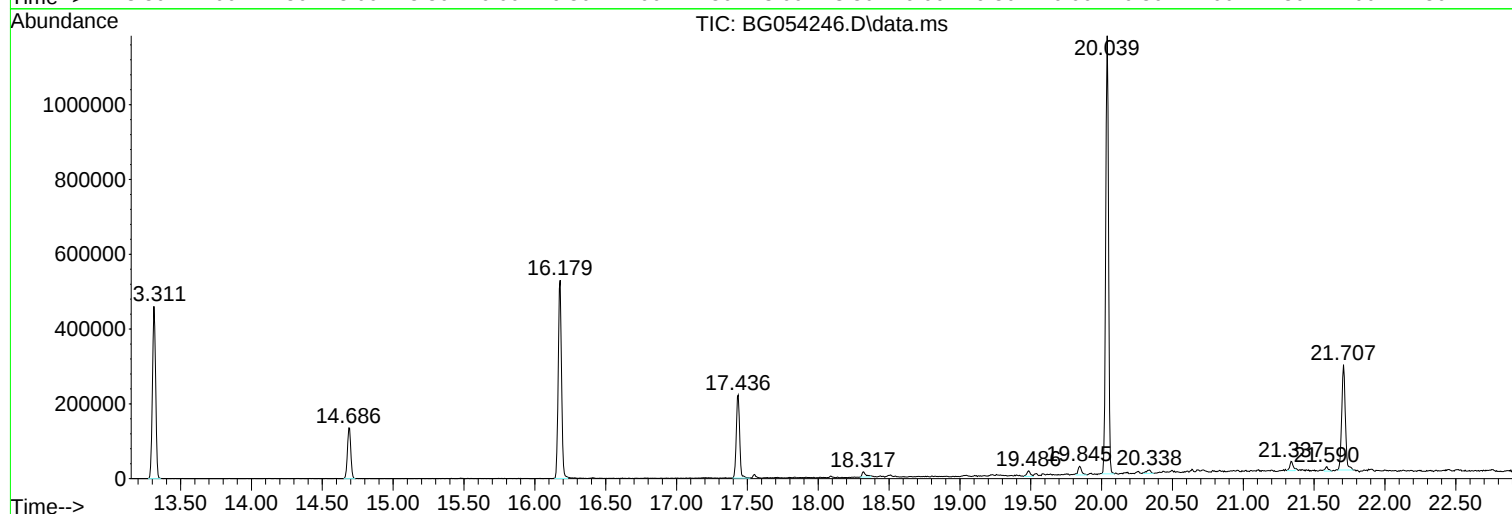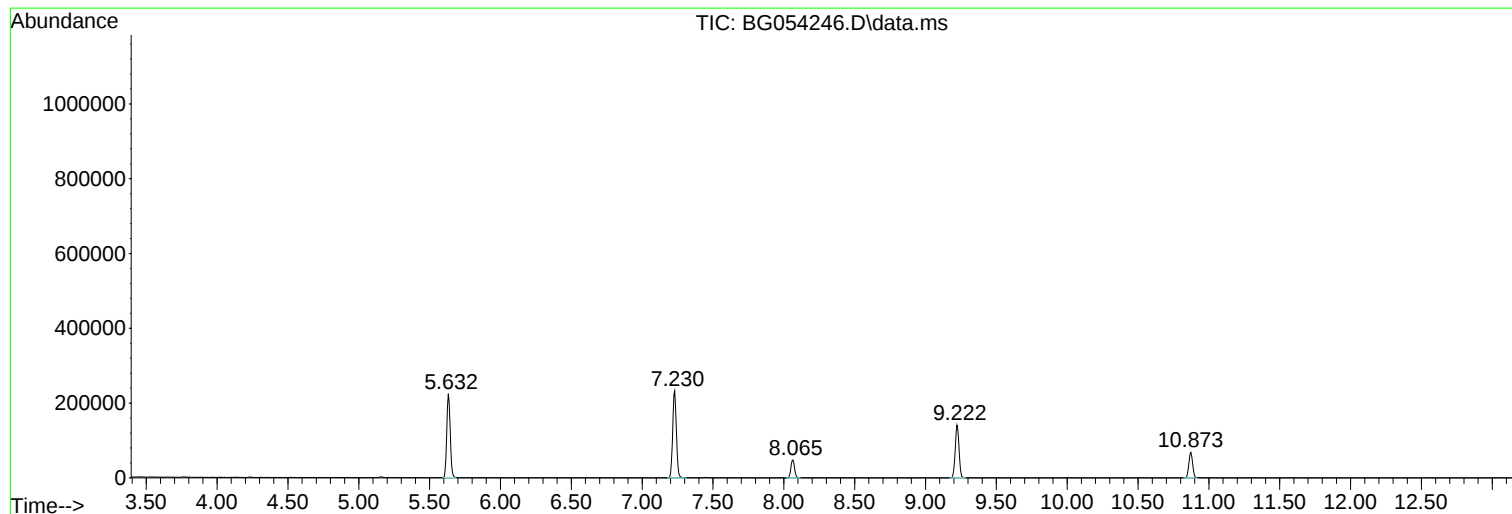

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070822\
Data File : BG054246.D
Acq On : 8 Jul 2022 14:34
Operator : CG/JU
Sample : N3622-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20220496A-SIM-C2A-COMPOSITE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070822\
Data File : BG054246.D
Acq On : 8 Jul 2022 14:34
Operator : CG/JU
Sample : N3622-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20220496A-SIM-C2A-COMPOSITE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------