
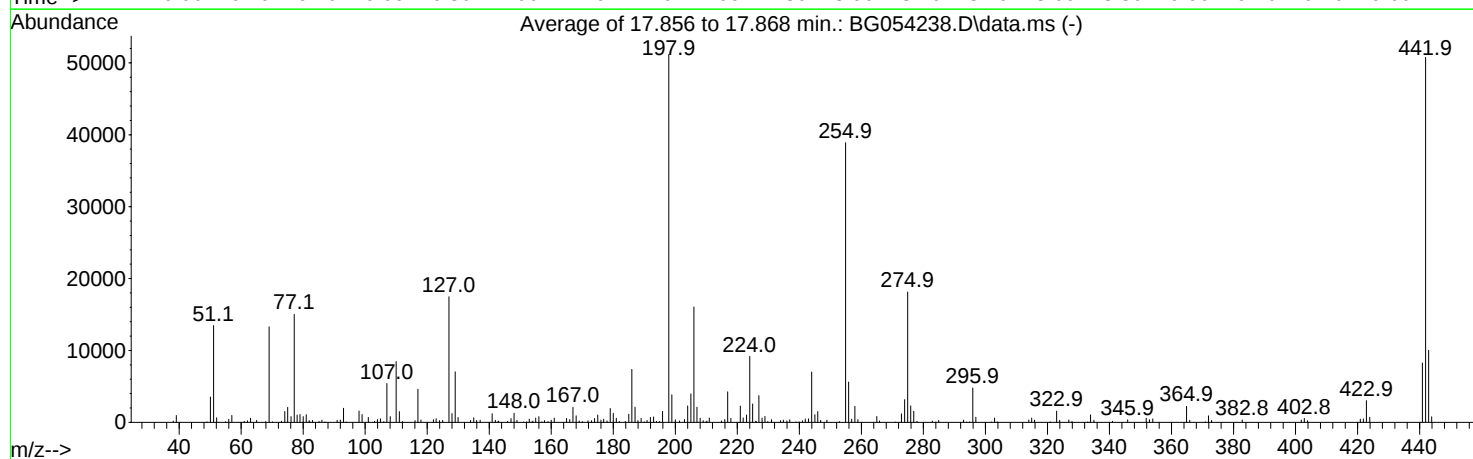


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070822\
 Data File : BG054238.D
 Acq On : 8 Jul 2022 8:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 08 13:46:14 2022

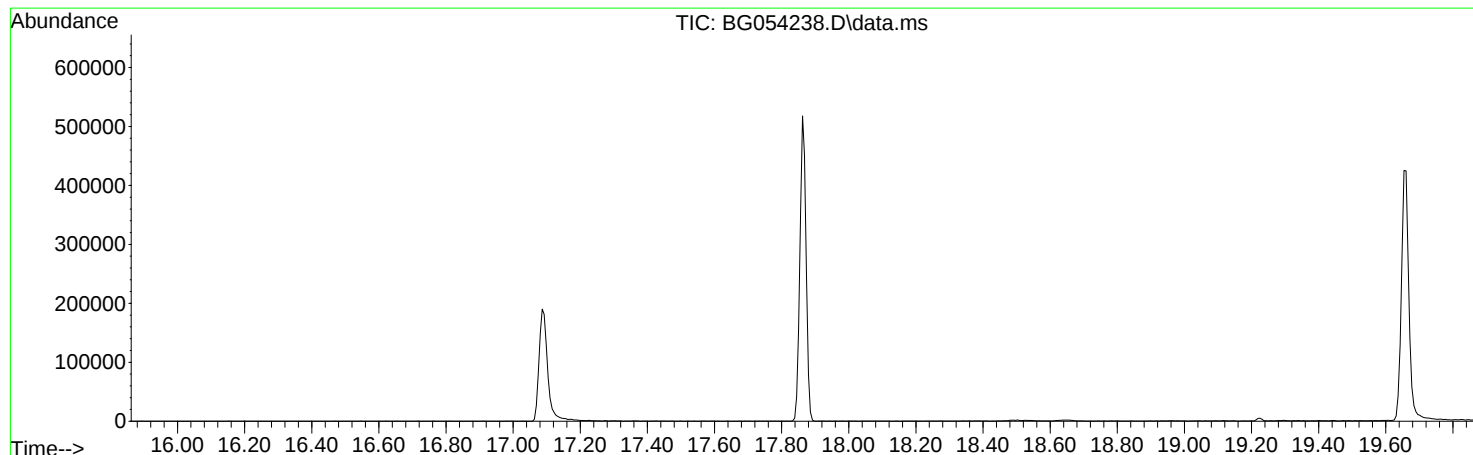

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.3	13463	PASS
68	69	0.00	2	0.6	81	PASS
69	198	0.00	100	26.0	13289	PASS
70	69	0.00	2	0.4	58	PASS
127	198	10	80	34.1	17472	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51165	PASS
199	198	5	9	7.5	3824	PASS
275	198	10	60	35.4	18137	PASS
365	198	1	100	4.4	2236	PASS
441	198	0.01	100	16.1	8254	PASS
442	442	50	100	100.0	50763	PASS
443	442	15	24	19.7	10009	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/8/2022	BNA_G	<u>BG054238.D</u>
Compound Name	Response	Retention Time
DDT	201757	20.89
DDD	3370	20.45
DDE	1333	19.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4703	206460	2.28

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070822\
Data File : BG054238.D
Acq On : 8 Jul 2022 8:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 08 13:49:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 13:46:14 2022
Response via : Initial Calibration

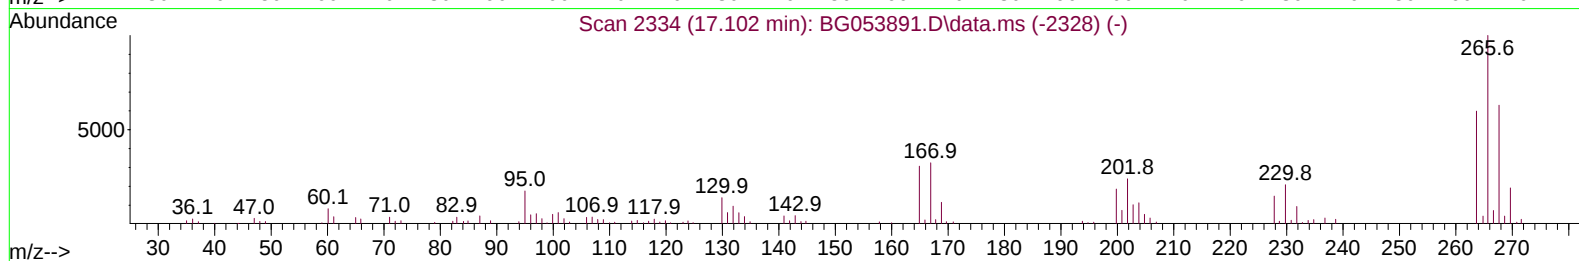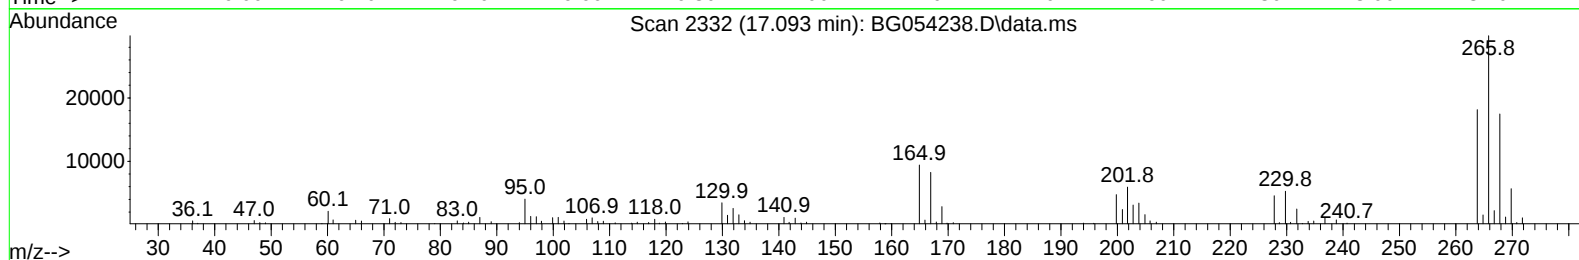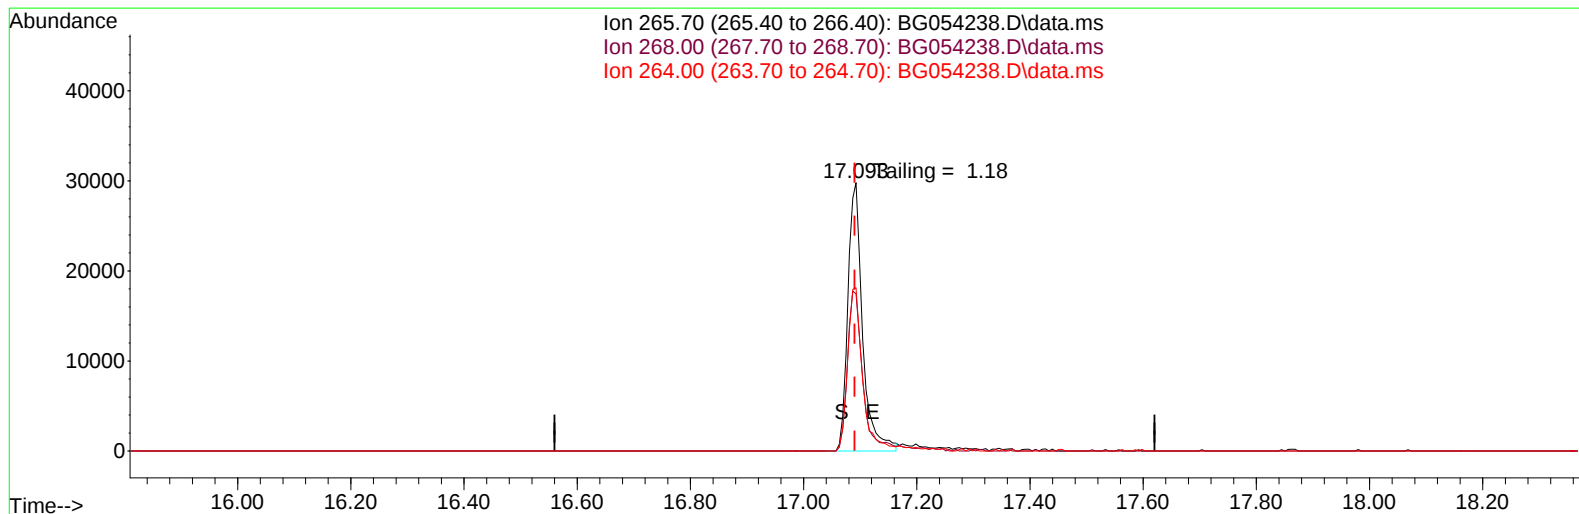

TIC: BG054238.D\data.ms

(70) Pentachlorophenol (C)

17.093min (+ 0.003) 25152.77 ng




response 54918

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	58.59
264.00	66.20	60.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070822\
Data File : BG054238.D
Acq On : 8 Jul 2022 8:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 08 13:49:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 13:46:14 2022
Response via : Initial Calibration

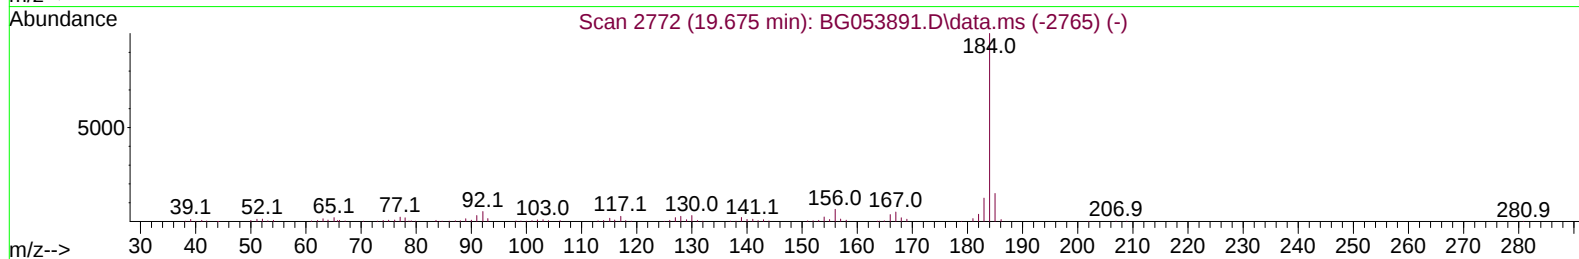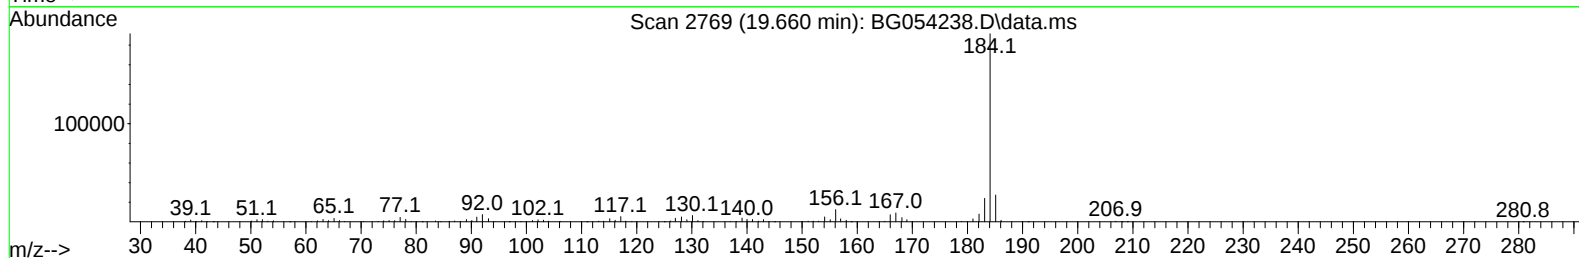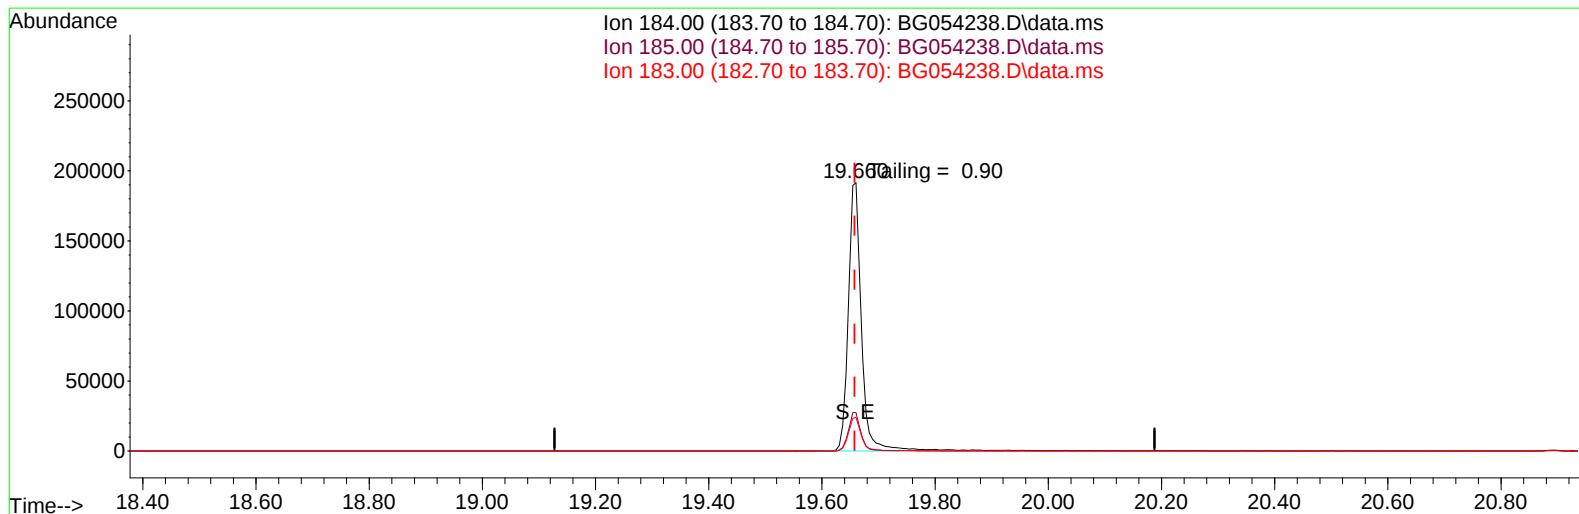

TIC: BG054238.D\data.ms

(77) Benzidine

19.660min (+ 0.003) 0.00 ng

response 307507

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.31
183.00	11.10	12.53
0.00	0.00	0.00