

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
 Data File : BG061936.D
 Acq On : 8 Jul 2024 10:44
 Operator : MA/JU
 Sample : PB161727BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK727

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061936.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.376	13	15	18	rVB3	2558	2414	0.16%	0.015%
2	3.482	29	33	38	rVB3	11513	17800	1.21%	0.113%
3	3.588	47	51	52	rBV4	2048	2483	0.17%	0.016%
4	3.599	52	53	56	rBV2	2575	2210	0.15%	0.014%
5	3.899	100	104	115	rBV	157819	250506	17.01%	1.596%
6	4.381	184	186	190	rVB3	1927	2779	0.19%	0.018%
7	4.533	211	212	215	rBV	2122	2352	0.16%	0.015%
8	4.663	232	234	236	rBV2	3269	2740	0.19%	0.017%
9	4.716	239	243	244	rBV2	1985	2138	0.15%	0.014%
10	4.904	271	275	277	rBV2	2088	2075	0.14%	0.013%
11	5.180	320	322	326	rBV2	2608	2225	0.15%	0.014%
12	5.338	346	349	350	rBV	2595	2834	0.19%	0.018%
13	6.596	559	563	568	rVB2	2617	3216	0.22%	0.020%
14	7.248	667	674	682	rBV	230200	405860	27.55%	2.586%
15	7.412	693	702	709	rBV	138483	241266	16.38%	1.538%
16	7.624	731	738	748	rVB2	212936	358875	24.36%	2.287%
17	7.941	788	792	795	rBV	1765	2459	0.17%	0.016%
18	7.982	795	799	801	rBV	2228	2896	0.20%	0.018%
19	8.094	809	818	826	rBV	163527	268436	18.22%	1.711%
20	8.188	831	834	838	rBV	2022	2525	0.17%	0.016%
21	8.329	857	858	863	rVB	1959	2680	0.18%	0.017%
22	8.364	863	864	868	rBV	1935	2448	0.17%	0.016%
23	8.793	930	937	945	rBV2	293089	501630	34.05%	3.197%
24	9.263	1009	1017	1024	rVB	223974	406483	27.59%	2.590%
25	9.980	1133	1139	1146	rBV2	215169	373794	25.38%	2.382%
26	10.209	1175	1178	1181	rBV2	2934	3635	0.25%	0.023%
27	10.521	1223	1231	1239	rBV	309448	536090	36.39%	3.416%
28	10.609	1243	1246	1249	rBV	1986	2528	0.17%	0.016%
29	10.808	1278	1280	1281	rBV	2385	2199	0.15%	0.014%
30	10.908	1285	1297	1304	rVV	254733	447640	30.39%	2.853%
31	11.038	1310	1319	1327	rBV2	260689	448421	30.44%	2.858%
32	11.173	1339	1342	1346	rBV	1858	2302	0.16%	0.015%
33	11.484	1392	1395	1397	rBV	1633	2205	0.15%	0.014%
34	11.660	1421	1425	1429	rBV2	2823	4048	0.27%	0.026%
35	11.696	1429	1431	1434	rBV2	2050	2790	0.19%	0.018%
36	12.013	1483	1485	1487	rVB	3571	2133	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
 Data File : BG061936.D
 Acq On : 8 Jul 2024 10:44
 Operator : MA/JU
 Sample : PB161727BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK727

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

37	12.236	1522	1523	1526	rVB	3184	2514	0.17%	0.016%
38	12.266	1526	1528	1531	rBV	1635	2501	0.17%	0.016%
39	12.365	1542	1545	1547	rBV	1629	2319	0.16%	0.015%
40	12.477	1561	1564	1568	rBV3	5220	7916	0.54%	0.050%

41	12.718	1604	1605	1609	rVB	2398	2415	0.16%	0.015%
42	12.759	1609	1612	1613	rBV	2809	2612	0.18%	0.017%
43	12.812	1618	1621	1623	rBV	1755	2216	0.15%	0.014%
44	13.112	1671	1672	1677	rVB	2781	2238	0.15%	0.014%
45	14.116	1835	1843	1849	rBV	587977	830036	56.35%	5.290%

46	14.416	1886	1894	1903	rBV2	562386	927616	62.97%	5.911%
47	14.716	1939	1945	1951	rVB	433307	655205	44.48%	4.175%
48	14.763	1951	1953	1956	rVB	3696	2963	0.20%	0.019%
49	14.792	1956	1958	1960	rBV	2770	2531	0.17%	0.016%
50	14.904	1971	1977	1985	rBV	291186	473153	32.12%	3.015%

51	15.039	1998	2000	2002	rBV2	2191	2144	0.15%	0.014%
52	15.056	2002	2003	2007	rVB2	2808	2783	0.19%	0.018%
53	15.121	2012	2014	2017	rVB	2712	2325	0.16%	0.015%
54	15.227	2031	2032	2035	rVB	3091	2364	0.16%	0.015%
55	15.250	2035	2036	2039	rBV2	3131	3164	0.21%	0.020%

56	15.303	2042	2045	2046	rBV2	2143	2187	0.15%	0.014%
57	15.544	2082	2086	2088	rBV	2429	2933	0.20%	0.019%
58	15.703	2107	2113	2122	rBV	746826	1141514	77.49%	7.275%
59	15.814	2126	2132	2142	rVB2	300482	430761	29.24%	2.745%
60	15.967	2157	2158	2161	rBV	2079	2244	0.15%	0.014%

61	16.061	2171	2174	2177	rBV	2187	2455	0.17%	0.016%
62	16.108	2177	2182	2184	rBV	2994	4476	0.30%	0.029%
63	16.149	2187	2189	2192	rVB2	3472	2424	0.16%	0.015%
64	16.202	2196	2198	2202	rBV	3883	5108	0.35%	0.033%
65	16.631	2269	2271	2274	rBV	3147	3827	0.26%	0.024%

66	16.666	2274	2277	2279	rVB	3184	3451	0.23%	0.022%
67	16.702	2281	2283	2286	rVV	2443	2479	0.17%	0.016%
68	16.772	2291	2295	2296	rBV	2598	2774	0.19%	0.018%
69	17.031	2337	2339	2341	rVB2	4245	2441	0.17%	0.016%
70	17.177	2362	2364	2366	rVB	2802	2478	0.17%	0.016%

71	17.195	2366	2367	2371	rBV	3264	2641	0.18%	0.017%
72	17.236	2371	2374	2378	rBV2	2669	4362	0.30%	0.028%
73	17.460	2405	2412	2420	rVB	535342	823515	55.91%	5.248%
74	17.554	2420	2428	2437	rBV2	831712	1270088	86.22%	8.094%
75	17.724	2455	2457	2461	rBV4	3098	2883	0.20%	0.018%

76	17.859	2478	2480	2483	rBV2	2833	3002	0.20%	0.019%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
 Data File : BG061936.D
 Acq On : 8 Jul 2024 10:44
 Operator : MA/JU
 Sample : PB161727BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK727

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

77	17.941	2490	2494	2495	rBV2	2509	2776	0.19%	0.018%
78	18.006	2502	2505	2507	rBV	4600	5277	0.36%	0.034%
79	18.100	2520	2521	2523	rBV2	3620	3156	0.21%	0.020%
80	18.170	2529	2533	2536	rVB3	3354	5083	0.35%	0.032%
81	18.200	2536	2538	2539	rBV	5098	3202	0.22%	0.020%
82	18.311	2555	2557	2560	rBV	3861	4832	0.33%	0.031%
83	18.382	2568	2569	2572	rVB3	3402	2811	0.19%	0.018%
84	18.546	2594	2597	2598	rBV3	2586	2278	0.15%	0.015%
85	18.611	2606	2608	2610	rBV	3068	2821	0.19%	0.018%
86	18.870	2648	2652	2655	rBV2	3532	5257	0.36%	0.034%
87	18.940	2662	2664	2666	rBV2	2470	2391	0.16%	0.015%
88	18.987	2670	2672	2675	rVB2	3994	2885	0.20%	0.018%
89	19.034	2678	2680	2682	rBV2	2406	2603	0.18%	0.017%
90	19.187	2704	2706	2707	rVB2	3485	2375	0.16%	0.015%
91	19.205	2707	2709	2711	rBV2	6908	6640	0.45%	0.042%
92	19.322	2727	2729	2733	rBV3	3691	4787	0.32%	0.031%
93	19.398	2738	2742	2746	rVB5	14253	21430	1.45%	0.137%
94	19.463	2748	2753	2757	rBV3	15281	23983	1.63%	0.153%
95	19.545	2765	2767	2768	rBV2	3648	2765	0.19%	0.018%
96	19.739	2798	2800	2803	rVB3	6363	4765	0.32%	0.030%
97	19.833	2810	2816	2823	rVB	963797	1376944	93.48%	8.775%
98	21.713	3130	3136	3144	rVB	487552	821270	55.75%	5.234%
99	24.739	3641	3651	3664	rVB2	514948	1473054	100.00%	9.387%
100	24.957	3680	3688	3700	rVB	329045	942382	63.97%	6.006%




Sum of corrected areas: 15691940

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061936.D
Acq On : 8 Jul 2024 10:44
Operator : MA/JU
Sample : PB161727BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK727

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

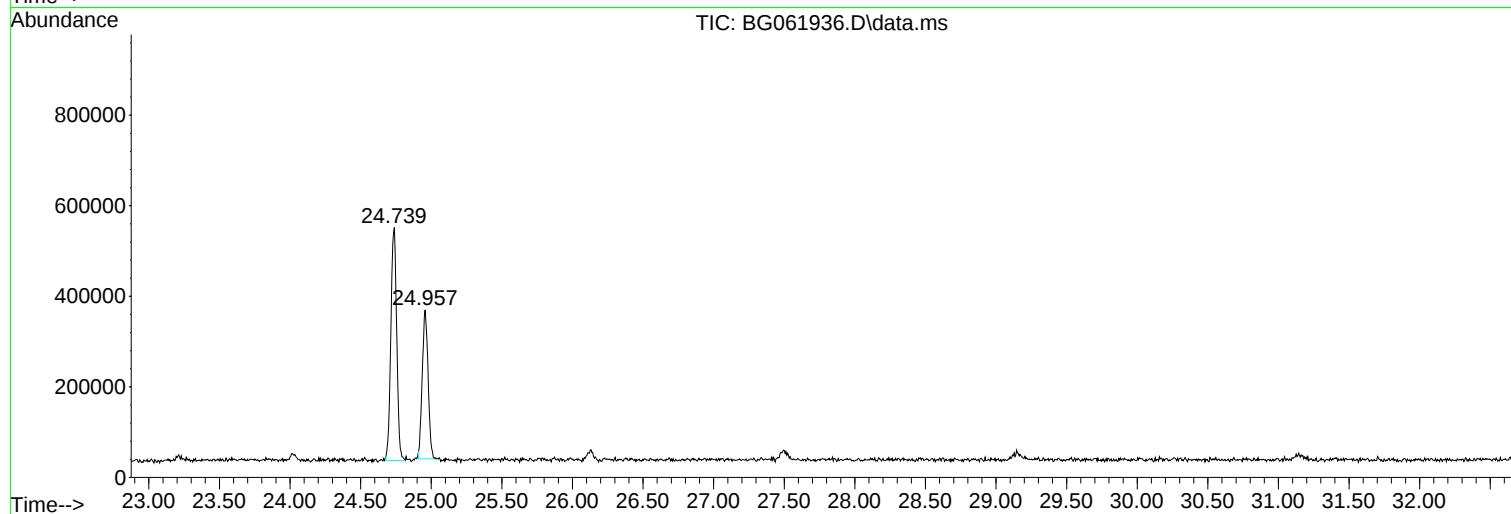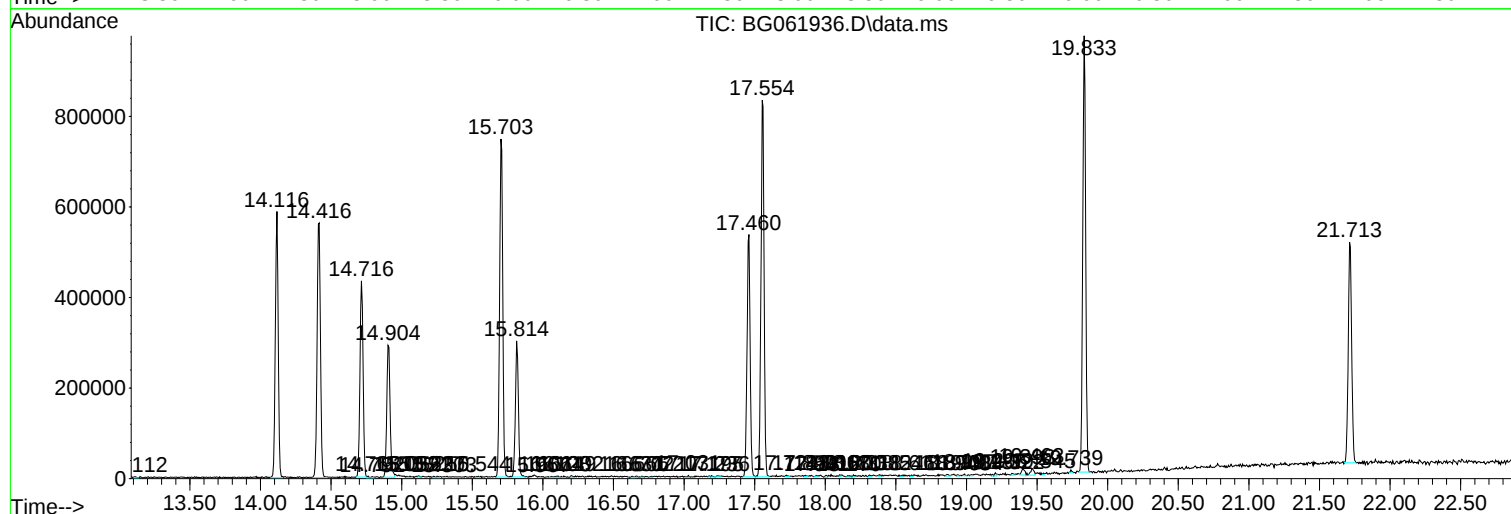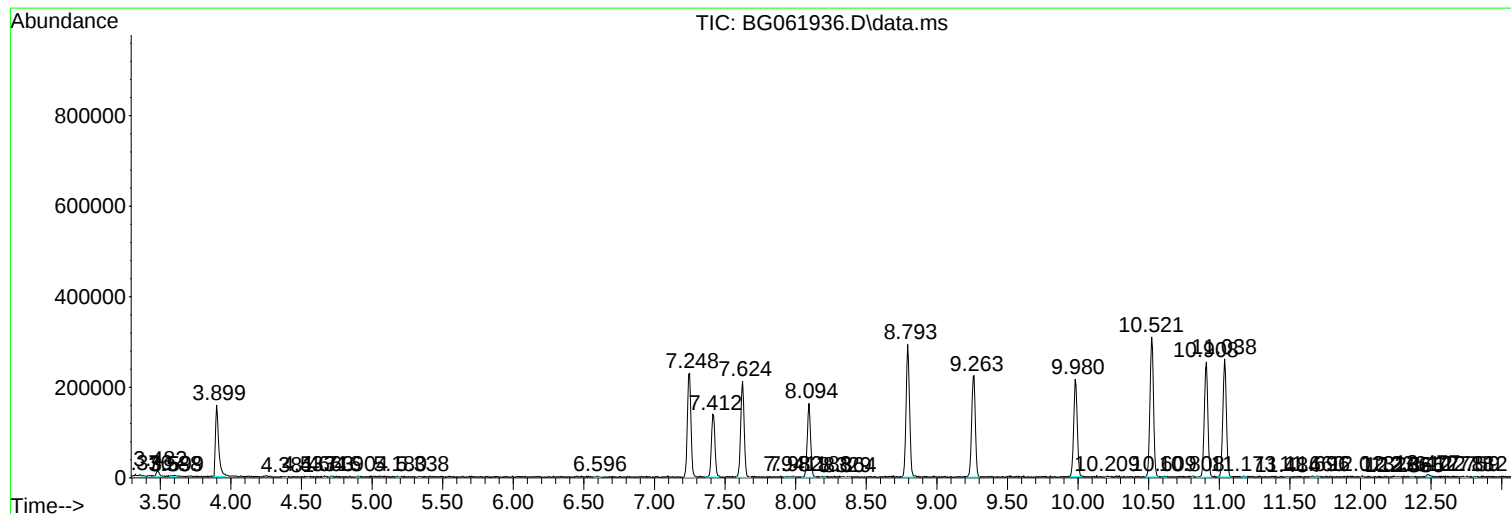

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061936.D
Acq On : 8 Jul 2024 10:44
Operator : MA/JU
Sample : PB161727BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK727

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061936.D
Acq On : 8 Jul 2024 10:44
Operator : MA/JU
Sample : PB161727BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK727

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc