

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
 Data File : BG061937.D
 Acq On : 8 Jul 2024 11:24
 Operator : MA/JU
 Sample : PB161733BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK733

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061937.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.440	22	26	27	rVB2	2348	2737	0.16%	0.015%
2	3.481	30	33	37	rBV2	11473	17005	1.01%	0.096%
3	3.692	68	69	71	rBV	3814	2457	0.15%	0.014%
4	3.734	75	76	80	rVB	2669	2590	0.15%	0.015%
5	3.857	94	97	100	rBV3	1490	2471	0.15%	0.014%
6	3.898	100	104	113	rVV	172942	277723	16.43%	1.565%
7	4.797	256	257	264	rVB2	2379	3414	0.20%	0.019%
8	5.050	298	300	304	rVB3	2507	3389	0.20%	0.019%
9	5.379	351	356	360	rBV3	1630	2973	0.18%	0.017%
10	5.520	377	380	382	rVB2	2969	2587	0.15%	0.015%
11	5.549	382	385	387	rVB	3012	2942	0.17%	0.017%
12	5.620	394	397	400	rVB	1901	2629	0.16%	0.015%
13	5.878	437	441	446	rBV2	1891	3065	0.18%	0.017%
14	6.378	524	526	529	rBV	2940	3019	0.18%	0.017%
15	6.495	544	546	550	rBV2	1696	2533	0.15%	0.014%
16	7.065	640	643	645	rVB	2213	2577	0.15%	0.015%
17	7.124	650	653	656	rBV2	2419	2506	0.15%	0.014%
18	7.247	666	674	683	rVB	251433	440170	26.04%	2.481%
19	7.418	696	703	710	rVB	156733	263879	15.61%	1.487%
20	7.623	732	738	747	rVB	229142	385682	22.82%	2.174%
21	7.694	747	750	751	rBV	3046	2760	0.16%	0.016%
22	7.788	764	766	770	rBV	2282	2628	0.16%	0.015%
23	7.911	784	787	789	rBV	3448	2891	0.17%	0.016%
24	8.093	811	818	827	rVB2	161212	273926	16.21%	1.544%
25	8.205	833	837	839	rBV2	1816	3454	0.20%	0.019%
26	8.346	857	861	863	rBV	2073	2759	0.16%	0.016%
27	8.687	913	919	921	rBV2	2142	3770	0.22%	0.021%
28	8.798	930	938	949	rVB	308614	546043	32.31%	3.078%
29	8.945	961	963	965	rBV	3294	2683	0.16%	0.015%
30	9.004	972	973	976	rBV	2669	2635	0.16%	0.015%
31	9.057	978	982	986	rBV	2125	3675	0.22%	0.021%
32	9.257	1006	1016	1027	rBV	253798	460113	27.22%	2.594%
33	9.515	1058	1060	1062	rVB	3947	2588	0.15%	0.015%
34	9.873	1118	1121	1124	rVB	2069	2739	0.16%	0.015%
35	9.979	1132	1139	1147	rBV2	232156	421490	24.94%	2.376%
36	10.173	1166	1172	1174	rBV	1642	2607	0.15%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
 Data File : BG061937.D
 Acq On : 8 Jul 2024 11:24
 Operator : MA/JU
 Sample : PB161733BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK733

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

37	10.520	1223	1231	1240	rBV	327249	593558	35.12%	3.346%
38	10.908	1289	1297	1306	rVB	256831	461940	27.33%	2.604%
39	11.037	1312	1319	1326	rBV2	278376	492610	29.14%	2.777%
40	11.801	1446	1449	1451	rBV	2503	3349	0.20%	0.019%
41	12.018	1483	1486	1488	rBV	1898	2699	0.16%	0.015%
42	12.171	1510	1512	1515	rVB	2493	2531	0.15%	0.014%
43	12.488	1561	1566	1569	rVB3	7610	10735	0.64%	0.061%
44	12.653	1592	1594	1597	rVB	2373	2573	0.15%	0.015%
45	12.688	1597	1600	1602	rBV	2529	3062	0.18%	0.017%
46	13.434	1726	1727	1731	rVB	2569	3062	0.18%	0.017%
47	13.516	1740	1741	1744	rVB	3686	2698	0.16%	0.015%
48	13.581	1751	1752	1756	rVB	2932	2680	0.16%	0.015%
49	13.787	1784	1787	1790	rBV	2368	3413	0.20%	0.019%
50	14.116	1836	1843	1851	rBV	666281	947349	56.05%	5.340%
51	14.415	1887	1894	1902	rVB	674547	1055039	62.42%	5.947%
52	14.633	1926	1931	1932	rBV	3017	3112	0.18%	0.018%
53	14.715	1938	1945	1952	rBV	443188	716128	42.37%	4.037%
54	14.909	1971	1978	1987	rBV	344456	553402	32.74%	3.119%
55	15.073	2002	2006	2009	rBV	2792	4283	0.25%	0.024%
56	15.114	2009	2013	2017	rVB	3964	6782	0.40%	0.038%
57	15.279	2038	2041	2043	rBV	2858	3691	0.22%	0.021%
58	15.391	2056	2060	2064	rBV	1929	2727	0.16%	0.015%
59	15.708	2107	2114	2121	rBV	861600	1324026	78.33%	7.463%
60	15.814	2124	2132	2139	rBV	340866	519569	30.74%	2.929%
61	15.925	2147	2151	2152	rBV	3559	4560	0.27%	0.026%
62	15.949	2152	2155	2156	rVB3	5051	4529	0.27%	0.026%
63	16.025	2165	2168	2169	rBV	3029	3029	0.18%	0.017%
64	16.225	2201	2202	2206	rVB2	3115	2590	0.15%	0.015%
65	16.483	2244	2246	2249	rBV3	4505	5388	0.32%	0.030%
66	17.047	2339	2342	2346	rBV	3030	3809	0.23%	0.021%
67	17.130	2348	2356	2361	rBV	4399	7315	0.43%	0.041%
68	17.171	2361	2363	2366	rVB	3248	2670	0.16%	0.015%
69	17.206	2366	2369	2370	rBV	2856	2662	0.16%	0.015%
70	17.247	2374	2376	2379	rVB2	3733	3402	0.20%	0.019%
71	17.400	2399	2402	2403	rBV	3616	3769	0.22%	0.021%
72	17.459	2406	2412	2419	rVV	598768	915207	54.15%	5.159%
73	17.559	2421	2429	2436	rVV	964044	1478409	87.47%	8.333%
74	17.694	2449	2452	2453	rBV	3219	3768	0.22%	0.021%
75	17.711	2453	2455	2458	rBV2	3607	2860	0.17%	0.016%
76	17.893	2484	2486	2490	rVB	2410	2728	0.16%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
 Data File : BG061937.D
 Acq On : 8 Jul 2024 11:24
 Operator : MA/JU
 Sample : PB161733BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK733

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

77	18.170	2531	2533	2537	rBV	3244	3201	0.19%	0.018%
78	18.275	2550	2551	2554	rVB	3627	2931	0.17%	0.017%
79	18.346	2561	2563	2565	rBV3	3737	2965	0.18%	0.017%
80	18.399	2568	2572	2575	rBV2	2740	3600	0.21%	0.020%
81	18.516	2589	2592	2594	rBV2	3219	3253	0.19%	0.018%
82	18.822	2642	2644	2646	rBV2	2838	2664	0.16%	0.015%
83	18.933	2661	2663	2665	rVB2	3771	3446	0.20%	0.019%
84	18.957	2665	2667	2669	rBV2	2823	2512	0.15%	0.014%
85	19.027	2677	2679	2681	rBV2	2424	2771	0.16%	0.016%
86	19.227	2711	2713	2716	rBV3	3196	3497	0.21%	0.020%
87	19.286	2721	2723	2725	rVB	4326	2885	0.17%	0.016%
88	19.362	2734	2736	2738	rVB3	4066	2953	0.17%	0.017%
89	19.403	2738	2743	2747	rBV5	18794	29241	1.73%	0.165%
90	19.474	2751	2755	2757	rVV3	11048	12716	0.75%	0.072%
91	19.580	2770	2773	2775	rBV3	3985	3954	0.23%	0.022%
92	19.738	2798	2800	2804	rBV3	7357	8476	0.50%	0.048%
93	19.832	2810	2816	2823	rBV	1111088	1611540	95.34%	9.084%
94	19.926	2830	2832	2833	rVB2	6150	3891	0.23%	0.022%
95	19.944	2833	2835	2836	rBV2	5124	4165	0.25%	0.023%
96	20.185	2874	2876	2879	rBV3	5810	6102	0.36%	0.034%
97	21.718	3130	3137	3143	rBV	581046	928324	54.92%	5.233%
98	24.738	3641	3651	3660	rVB	620244	1690272	100.00%	9.528%
99	24.962	3679	3689	3701	rVB2	364282	1068206	63.20%	6.021%
100	28.146	4229	4231	4232	rBV2	11507	6174	0.37%	0.035%



Sum of corrected areas: 17740561

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061937.D
Acq On : 8 Jul 2024 11:24
Operator : MA/JU
Sample : PB161733BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK733

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

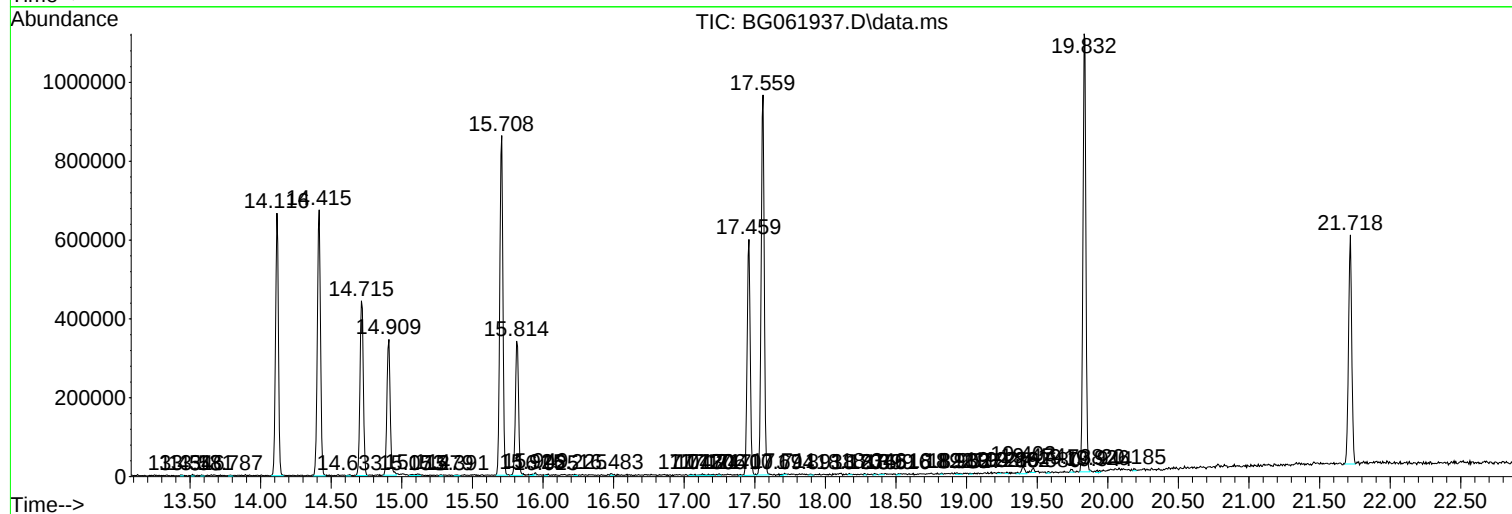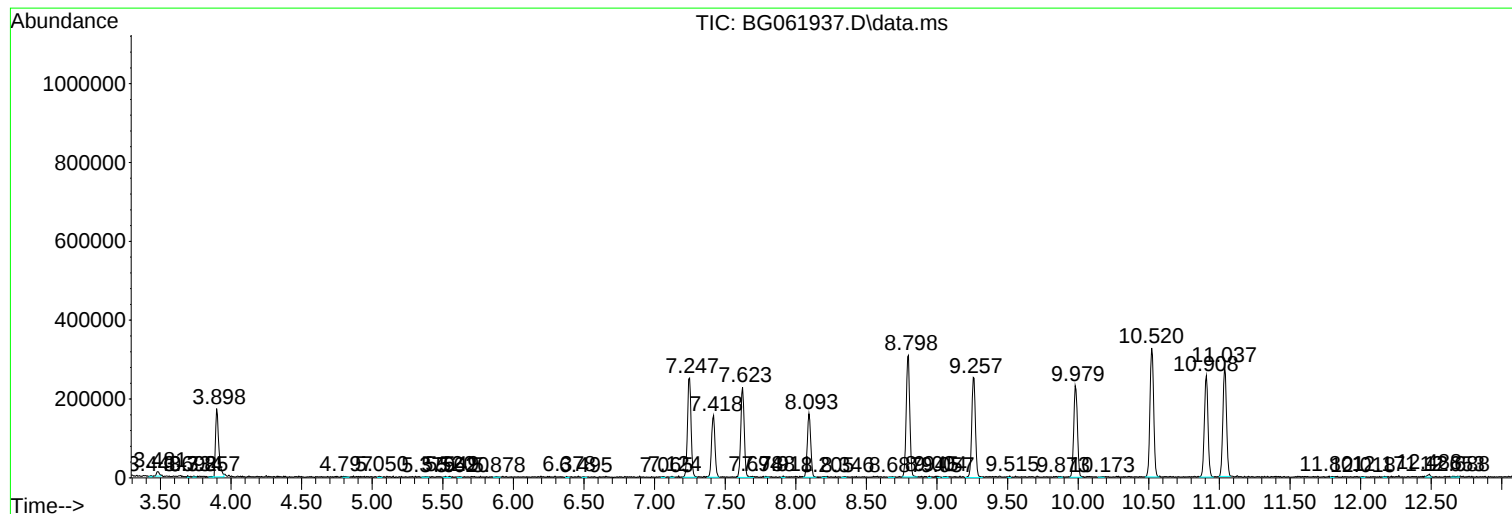

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061937.D
Acq On : 8 Jul 2024 11:24
Operator : MA/JU
Sample : PB161733BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK733

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061937.D
Acq On : 8 Jul 2024 11:24
Operator : MA/JU
Sample : PB161733BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK733

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc