

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
 Data File : BG061938.D
 Acq On : 8 Jul 2024 12:04
 Operator : MA/JU
 Sample : P3059-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E1GM3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061938.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.390	13	17	22	rVB6	3080	5118	0.24%	0.026%
2	3.484	29	33	39	rVB4	8639	14722	0.70%	0.075%
3	3.766	75	81	86	rBV4	3817	7324	0.35%	0.037%
4	3.825	89	91	93	rBV	3834	3243	0.15%	0.017%
5	3.907	101	105	113	rBV2	42447	78291	3.72%	0.399%
6	4.248	158	163	166	rVB3	4147	7084	0.34%	0.036%
7	4.659	231	233	236	rVB2	3716	2954	0.14%	0.015%
8	4.812	257	259	262	rVB3	3858	4381	0.21%	0.022%
9	5.164	314	319	325	rVB4	4870	9076	0.43%	0.046%
10	5.529	378	381	383	rBV	2584	2647	0.13%	0.013%
11	5.634	397	399	402	rVB2	3268	2857	0.14%	0.015%
12	6.198	491	495	497	rVB	2009	3317	0.16%	0.017%
13	6.240	497	502	507	rBV2	3115	5150	0.24%	0.026%
14	6.527	549	551	553	rBV2	2758	2674	0.13%	0.014%
15	7.097	646	648	651	rBV	3212	2897	0.14%	0.015%
16	7.191	661	664	667	rBV	2001	2997	0.14%	0.015%
17	7.244	667	673	680	rVV2	89639	154297	7.33%	0.787%
18	7.415	694	702	711	rVB	200744	324099	15.40%	1.652%
19	7.620	730	737	745	rBV	243391	424455	20.17%	2.164%
20	8.096	809	818	825	rVB	178482	308470	14.66%	1.573%
21	8.413	871	872	877	rVB	1749	2714	0.13%	0.014%
22	8.625	904	908	910	rBV	1709	2628	0.12%	0.013%
23	8.719	920	924	927	rBV	2515	4026	0.19%	0.021%
24	8.795	930	937	943	rBV2	249710	428416	20.36%	2.184%
25	9.260	1009	1016	1024	rBV	305525	547862	26.04%	2.793%
26	9.365	1027	1034	1036	rBV4	5985	9343	0.44%	0.048%
27	9.459	1047	1050	1054	rBV2	2264	2874	0.14%	0.015%
28	9.688	1086	1089	1093	rVB2	2926	4574	0.22%	0.023%
29	9.806	1106	1109	1112	rVB2	4623	4861	0.23%	0.025%
30	9.982	1132	1139	1147	rVB2	284433	505453	24.02%	2.577%
31	10.205	1174	1177	1182	rBV2	2229	3834	0.18%	0.020%
32	10.523	1222	1231	1239	rBV2	395602	703695	33.44%	3.587%
33	10.911	1288	1297	1304	rBV	288209	513915	24.42%	2.620%
34	11.040	1312	1319	1328	rBV	312494	579648	27.55%	2.955%
35	11.422	1381	1384	1387	rBV	2790	4910	0.23%	0.025%
36	11.645	1414	1422	1424	rBV5	9224	17214	0.82%	0.088%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
 Data File : BG061938.D
 Acq On : 8 Jul 2024 12:04
 Operator : MA/JU
 Sample : P3059-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E1GM3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

37	11.663	1424	1425	1429	rVV	2437	3322	0.16%	0.017%
38	11.715	1432	1434	1437	rVB	2829	2884	0.14%	0.015%
39	11.780	1439	1445	1449	rBV2	3845	8892	0.42%	0.045%
40	12.479	1561	1564	1568	rBV2	6759	8633	0.41%	0.044%
41	12.567	1578	1579	1584	rBV	2669	4261	0.20%	0.022%
42	12.720	1602	1605	1607	rBV	2725	3044	0.14%	0.016%
43	13.272	1695	1699	1702	rBV	1834	2814	0.13%	0.014%
44	13.502	1735	1738	1741	rBV	2366	3855	0.18%	0.020%
45	13.772	1781	1784	1787	rBV	2877	3630	0.17%	0.019%
46	13.842	1793	1796	1799	rVB	2412	3299	0.16%	0.017%
47	13.884	1799	1803	1805	rBV	2462	3470	0.16%	0.018%
48	14.119	1836	1843	1850	rBV	749414	1096276	52.10%	5.589%
49	14.230	1859	1862	1864	rBV	2472	3093	0.15%	0.016%
50	14.412	1886	1893	1902	rVB2	773050	1215697	57.77%	6.197%
51	14.600	1922	1925	1928	rBV	2002	2765	0.13%	0.014%
52	14.641	1928	1932	1937	rVV2	6966	11492	0.55%	0.059%
53	14.718	1938	1945	1952	rVV	493144	776819	36.92%	3.960%
54	14.788	1955	1957	1961	rVB	2479	3054	0.15%	0.016%
55	14.906	1971	1977	1982	rBV2	120249	187657	8.92%	0.957%
56	15.059	2000	2003	2008	rVB3	4175	4897	0.23%	0.025%
57	15.123	2008	2014	2017	rBV4	5500	8370	0.40%	0.043%
58	15.299	2040	2044	2047	rVB2	2358	3307	0.16%	0.017%
59	15.441	2065	2068	2072	rVB3	7344	8292	0.39%	0.042%
60	15.576	2088	2091	2094	rBV	2390	3196	0.15%	0.016%
61	15.705	2107	2113	2120	rBV	1016598	1535616	72.98%	7.828%
62	15.817	2125	2132	2141	rBV2	427602	635297	30.19%	3.239%
63	15.946	2149	2154	2156	rVB3	4624	6556	0.31%	0.033%
64	15.969	2156	2158	2161	rVB	2939	2887	0.14%	0.015%
65	16.005	2161	2164	2166	rBV	2442	3057	0.15%	0.016%
66	16.140	2183	2187	2189	rBV	2827	4079	0.19%	0.021%
67	16.228	2200	2202	2205	rBV2	2631	2658	0.13%	0.014%
68	16.386	2226	2229	2231	rBV	4572	3183	0.15%	0.016%
69	16.439	2235	2238	2243	rBV2	3298	5253	0.25%	0.027%
70	16.974	2327	2329	2332	rBV2	3842	4205	0.20%	0.021%
71	17.133	2353	2356	2359	rVB2	3013	3416	0.16%	0.017%
72	17.156	2359	2360	2364	rBV	2589	3317	0.16%	0.017%
73	17.456	2404	2411	2418	rVB	687789	1005616	47.79%	5.126%
74	17.556	2421	2428	2435	rBV2	1164517	1799790	85.53%	9.175%
75	17.620	2437	2439	2441	rVB2	4842	3037	0.14%	0.015%
76	17.726	2453	2457	2459	rVB3	3307	3647	0.17%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
 Data File : BG061938.D
 Acq On : 8 Jul 2024 12:04
 Operator : MA/JU
 Sample : P3059-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E1GM3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

77	17.808	2466	2471	2475	rBV4	7729	16317	0.78%	0.083%
78	18.108	2519	2522	2525	rBV3	4360	5887	0.28%	0.030%
79	18.202	2536	2538	2540	rBV	3807	3044	0.14%	0.016%
80	18.408	2570	2573	2574	rBV2	3869	3999	0.19%	0.020%
81	18.619	2606	2609	2610	rBV2	2714	2658	0.13%	0.014%
82	18.748	2628	2631	2632	rBV	4220	4638	0.22%	0.024%
83	18.766	2632	2634	2637	rVV3	3490	3774	0.18%	0.019%
84	19.254	2715	2717	2718	rBV	3195	2646	0.13%	0.013%
85	19.359	2733	2735	2737	rBV2	3660	2892	0.14%	0.015%
86	19.401	2737	2742	2746	rVV2	20256	30966	1.47%	0.158%
87	19.471	2749	2754	2757	rVV3	15291	27447	1.30%	0.140%
88	19.500	2757	2759	2762	rVV3	7383	8865	0.42%	0.045%
89	19.530	2762	2764	2766	rVB3	7154	5274	0.25%	0.027%
90	19.782	2805	2807	2809	rBV2	5753	4054	0.19%	0.021%
91	19.835	2810	2816	2823	rVV	1357820	1933971	91.91%	9.859%
92	20.335	2899	2901	2902	rBV2	7289	4371	0.21%	0.022%
93	20.605	2945	2947	2948	rBV2	5754	2776	0.13%	0.014%
94	21.715	3130	3136	3147	rBV2	614653	1033890	49.13%	5.271%
95	23.190	3382	3387	3397	rVB7	72921	165693	7.87%	0.845%
96	24.735	3639	3650	3662	rBV2	731587	2104226	100.00%	10.727%
97	24.959	3679	3688	3699	rVB	391204	1152467	54.77%	5.875%


Sum of corrected areas: 19616508

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061938.D
Acq On : 8 Jul 2024 12:04
Operator : MA/JU
Sample : P3059-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1GM3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

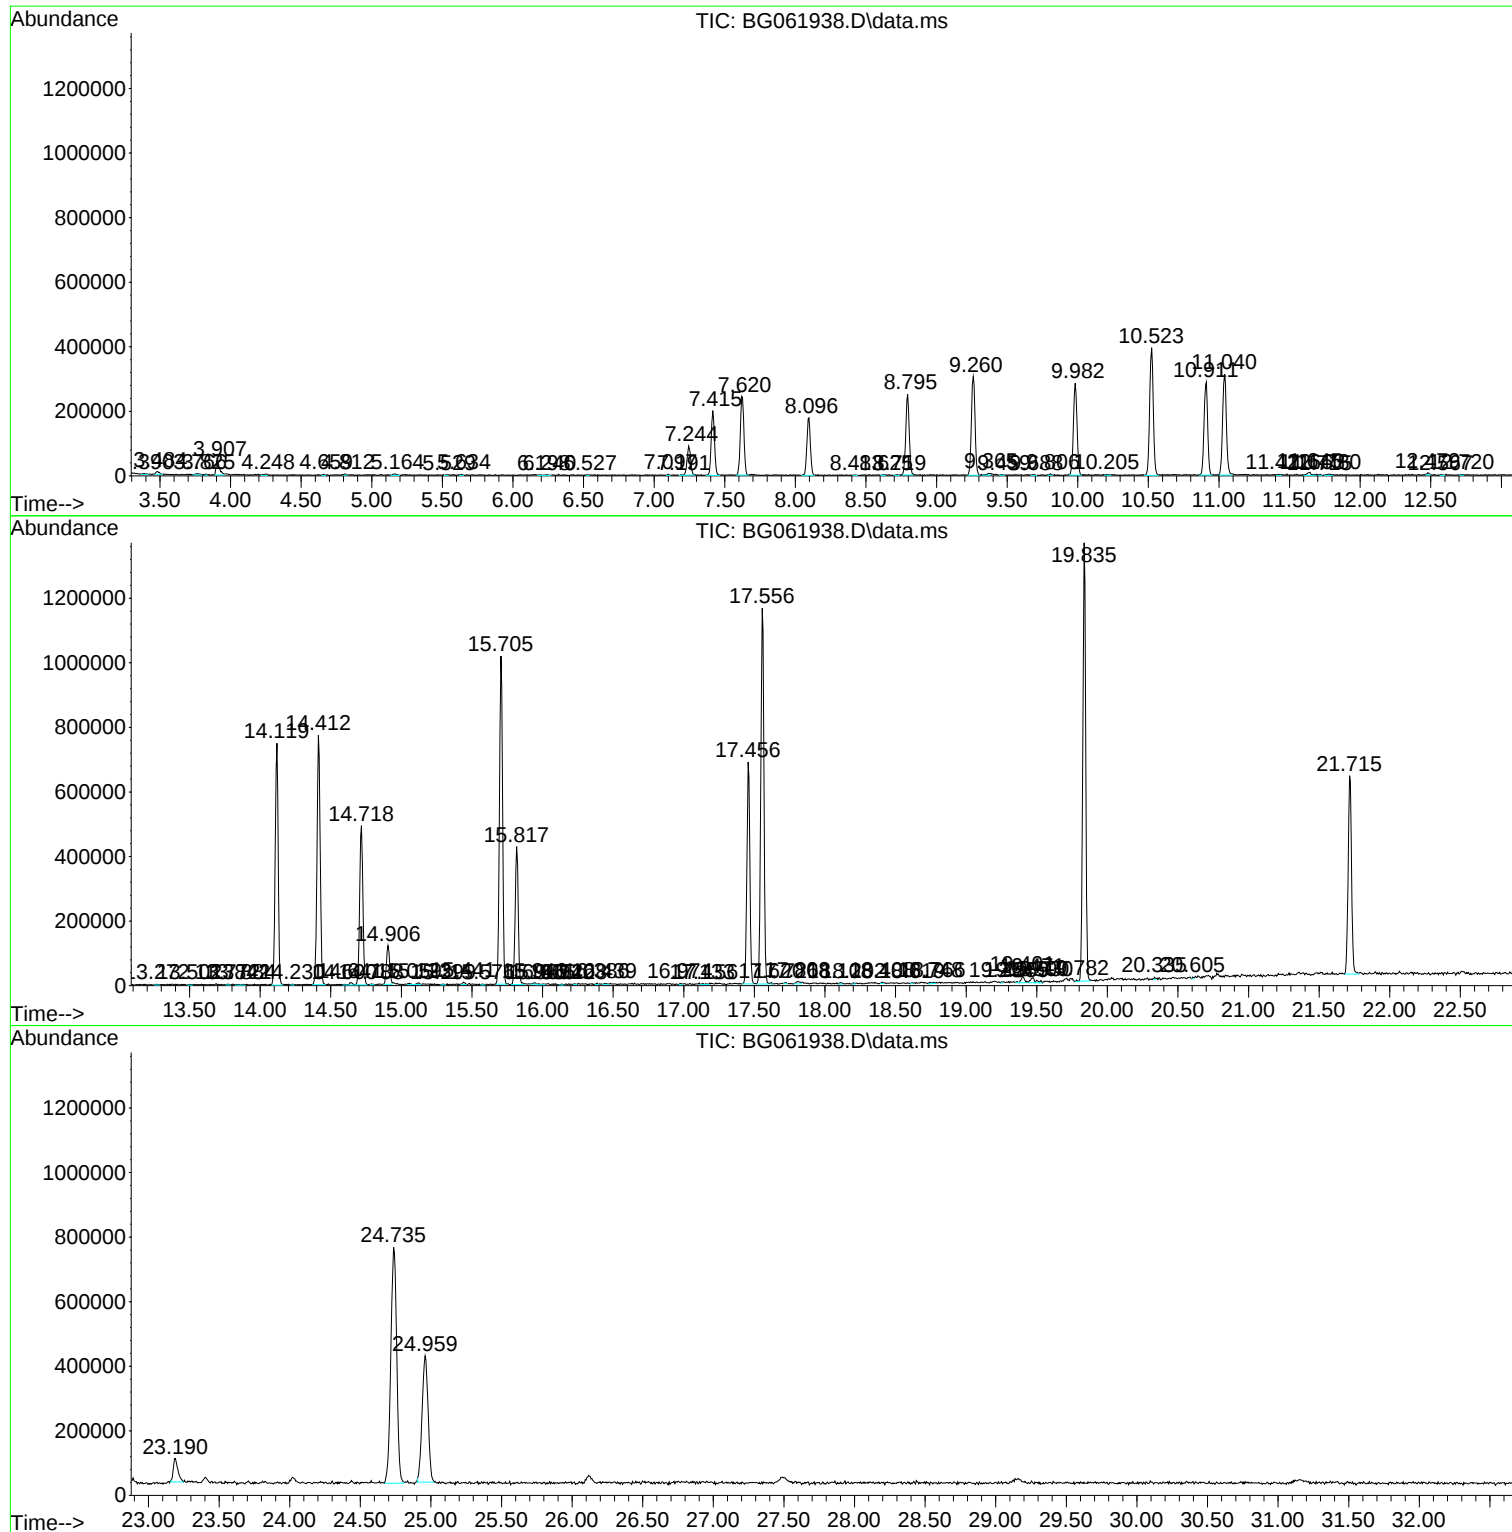

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061938.D
Acq On : 8 Jul 2024 12:04
Operator : MA/JU
Sample : P3059-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1GM3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzeneethanamine, 2-fluoro... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
23.190	3.21 ng/ul	165693	Chrysene-d12	21.715

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzeneethanamine, 2-fluoro-.bet...	229	C11H16FNO3	061338-98-5	64
2			Hexadecanamide	255	C16H33NO	000629-54-9	64
3			Octadecanamide	283	C18H37NO	000124-26-5	64
4			Tetradecanamide	227	C14H29NO	000638-58-4	50
5			Dodecanamide	199	C12H25NO	001120-16-7	50

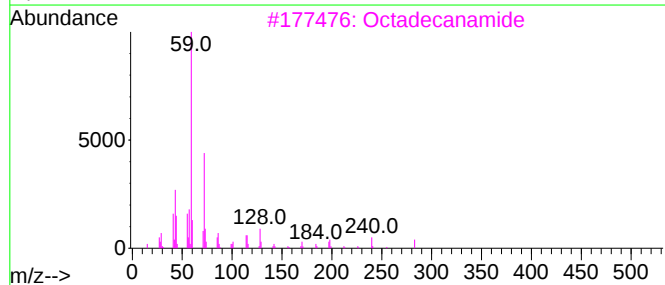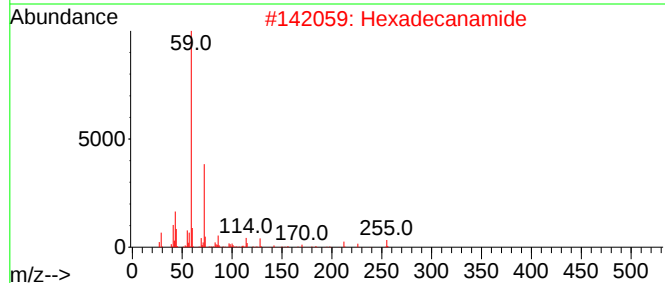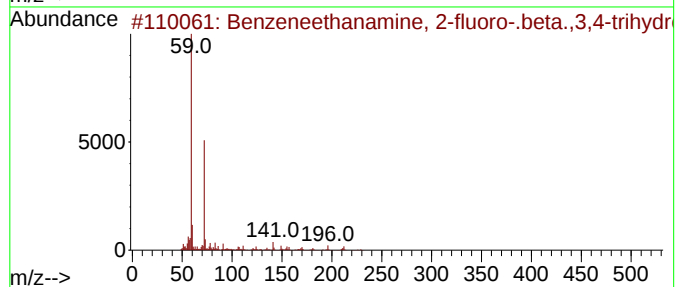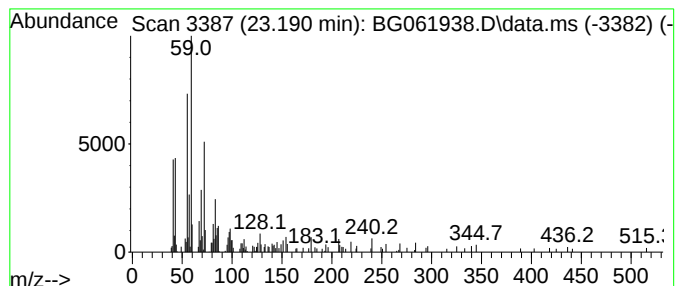

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061938.D
Acq On : 8 Jul 2024 12:04
Operator : MA/JU
Sample : P3059-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1GM3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzeneethanami...	23.190	3.2	ng/u1	165693	5	21.715	1033890	20.0