

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
 Data File : BG061945.D
 Acq On : 8 Jul 2024 16:47
 Operator : MA/JU
 Sample : P3059-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E1GN2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061945.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.482	26	33	42	rVB4	14870	28750	1.34%	0.148%
2	3.606	52	54	58	rVB3	4116	4623	0.22%	0.024%
3	3.735	74	76	78	rBV2	2187	2794	0.13%	0.014%
4	3.753	78	79	84	rVB3	3619	4421	0.21%	0.023%
5	3.905	103	105	114	rBV2	31455	50102	2.34%	0.258%
6	4.064	128	132	135	rVB3	3524	4679	0.22%	0.024%
7	4.810	254	259	262	rVB	2547	4044	0.19%	0.021%
8	5.163	313	319	322	rBV2	4730	5962	0.28%	0.031%
9	7.243	665	673	683	rBV2	109518	192244	8.99%	0.989%
10	7.413	695	702	712	rVB	204927	342370	16.01%	1.761%
11	7.625	730	738	747	rBV	275209	476686	22.29%	2.452%
12	7.695	747	750	752	rVV	3324	3470	0.16%	0.018%
13	8.095	810	818	825	rBV	179235	306195	14.32%	1.575%
14	8.706	916	922	924	rVB2	2309	3587	0.17%	0.018%
15	8.794	930	937	948	rBV2	280343	485860	22.72%	2.499%
16	9.170	1000	1001	1005	rVB	2463	2647	0.12%	0.014%
17	9.258	1009	1016	1025	rBV	324975	586351	27.42%	3.016%
18	9.804	1105	1109	1115	rBV2	6368	9237	0.43%	0.048%
19	9.986	1129	1140	1147	rBV2	294551	544457	25.46%	2.801%
20	10.521	1222	1231	1241	rBV	422303	759382	35.52%	3.907%
21	10.909	1289	1297	1305	rVB	276702	494856	23.14%	2.546%
22	11.038	1311	1319	1327	rVB2	223313	405409	18.96%	2.086%
23	11.555	1405	1407	1410	rVB	3226	2739	0.13%	0.014%
24	11.643	1416	1422	1424	rBV5	5186	9762	0.46%	0.050%
25	12.489	1558	1566	1570	rBV2	8031	16277	0.76%	0.084%
26	12.613	1583	1587	1590	rBV	3199	4008	0.19%	0.021%
27	12.677	1595	1598	1601	rBV2	2869	3305	0.15%	0.017%
28	13.001	1651	1653	1657	rVB	2160	2700	0.13%	0.014%
29	13.247	1692	1695	1697	rVB	2332	2719	0.13%	0.014%
30	13.523	1740	1742	1746	rVB3	2912	2611	0.12%	0.013%
31	14.117	1835	1843	1851	rBV	821416	1183736	55.36%	6.090%
32	14.193	1855	1856	1860	rBV	2771	2971	0.14%	0.015%
33	14.340	1879	1881	1884	rBV	1634	2726	0.13%	0.014%
34	14.411	1887	1893	1900	rVB	788675	1286638	60.18%	6.619%
35	14.505	1905	1909	1911	rBV	2047	3162	0.15%	0.016%
36	14.587	1919	1923	1925	rBV2	3154	3741	0.17%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
 Data File : BG061945.D
 Acq On : 8 Jul 2024 16:47
 Operator : MA/JU
 Sample : P3059-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E1GN2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

37	14.716	1938	1945	1952	rBV	480036	717692	33.57%	3.692%
38	14.904	1970	1977	1989	rBV	141796	234196	10.95%	1.205%
39	15.075	2004	2006	2010	rVB3	3969	4823	0.23%	0.025%
40	15.122	2010	2014	2017	rBV4	5567	8048	0.38%	0.041%
41	15.380	2053	2058	2060	rBV	2074	3783	0.18%	0.019%
42	15.421	2062	2065	2066	rBV	3109	3044	0.14%	0.016%
43	15.439	2066	2068	2070	rVB	3913	2943	0.14%	0.015%
44	15.703	2106	2113	2120	rBV	1040225	1616420	75.60%	8.315%
45	15.815	2124	2132	2140	rBV	457903	681436	31.87%	3.506%
46	15.950	2152	2155	2159	rVB3	6685	10124	0.47%	0.052%
47	16.003	2163	2164	2167	rBV2	3347	2949	0.14%	0.015%
48	16.079	2175	2177	2180	rVB	2548	2629	0.12%	0.014%
49	16.109	2180	2182	2185	rBV	1972	2707	0.13%	0.014%
50	16.332	2217	2220	2221	rVB2	3002	2988	0.14%	0.015%
51	16.473	2243	2244	2246	rBV	6119	3821	0.18%	0.020%
52	16.585	2259	2263	2265	rBV	2218	2712	0.13%	0.014%
53	16.626	2267	2270	2272	rVB2	3170	3110	0.15%	0.016%
54	16.755	2290	2292	2294	rVB	3230	2707	0.13%	0.014%
55	16.996	2331	2333	2336	rVB	4776	3619	0.17%	0.019%
56	17.031	2336	2339	2340	rBV2	2645	2777	0.13%	0.014%
57	17.131	2354	2356	2361	rBV4	2959	3575	0.17%	0.018%
58	17.202	2366	2368	2372	rVB3	4688	4469	0.21%	0.023%
59	17.366	2391	2396	2399	rBV3	4076	6081	0.28%	0.031%
60	17.454	2403	2411	2418	rBV	547105	870539	40.72%	4.478%
61	17.554	2422	2428	2437	rVB2	1176637	1814114	84.85%	9.332%
62	17.683	2448	2450	2452	rBV2	3214	3756	0.18%	0.019%
63	17.807	2470	2471	2473	rBV2	4249	3729	0.17%	0.019%
64	17.830	2473	2475	2480	rVB3	4073	6431	0.30%	0.033%
65	17.983	2500	2501	2504	rBV2	3906	2941	0.14%	0.015%
66	18.106	2518	2522	2525	rVB3	3804	5236	0.24%	0.027%
67	18.377	2566	2568	2569	rBV2	3620	2705	0.13%	0.014%
68	18.400	2570	2572	2576	rVB2	4807	4531	0.21%	0.023%
69	18.441	2576	2579	2581	rBV	4093	4590	0.21%	0.024%
70	18.676	2614	2619	2623	rBV5	6214	11734	0.55%	0.060%
71	18.741	2628	2630	2633	rBV4	3329	3015	0.14%	0.016%
72	18.999	2672	2674	2675	rBV2	3524	2989	0.14%	0.015%
73	19.152	2698	2700	2701	rBV2	4508	3315	0.16%	0.017%
74	19.405	2737	2743	2746	rVB4	19652	25120	1.17%	0.129%
75	19.469	2751	2754	2758	rVB2	14935	18422	0.86%	0.095%
76	19.740	2798	2800	2803	rVB3	11920	11872	0.56%	0.061%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061945.D
Acq On : 8 Jul 2024 16:47
Operator : MA/JU
Sample : P3059-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1GN2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Title : SVOA CALIBRATION

77	19.834	2810	2816	2823	rBV	1352905	1995645	93.34%	10.266%
78	21.720	3130	3137	3143	rBV2	537777	892294	41.73%	4.590%
79	24.740	3640	3651	3665	rBV	762045	2138120	100.00%	10.999%
80	24.957	3679	3688	3700	rVB	363905	1045735	48.91%	5.380%




Sum of corrected areas: 19438707

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061945.D
Acq On : 8 Jul 2024 16:47
Operator : MA/JU
Sample : P3059-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1GN2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

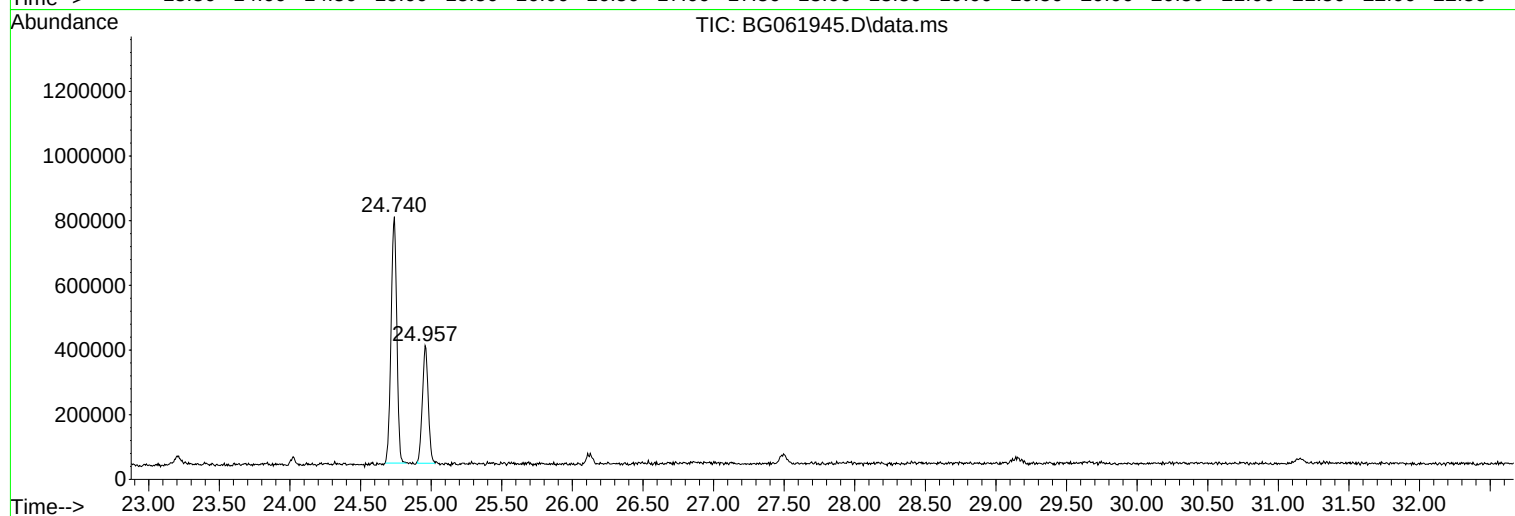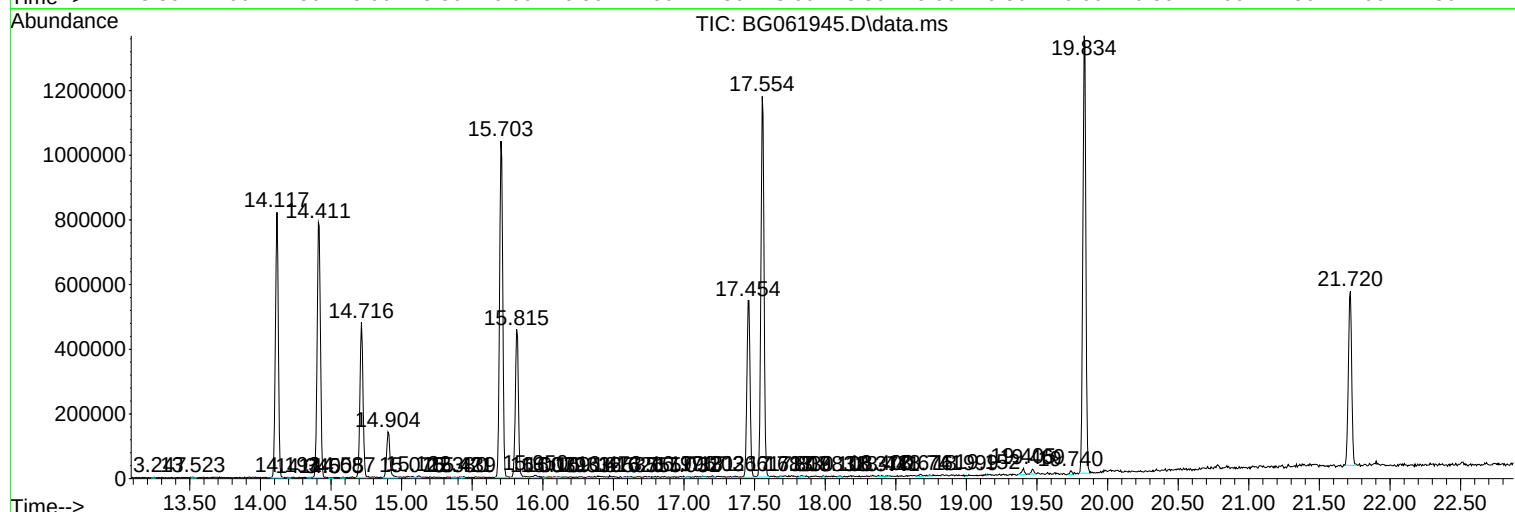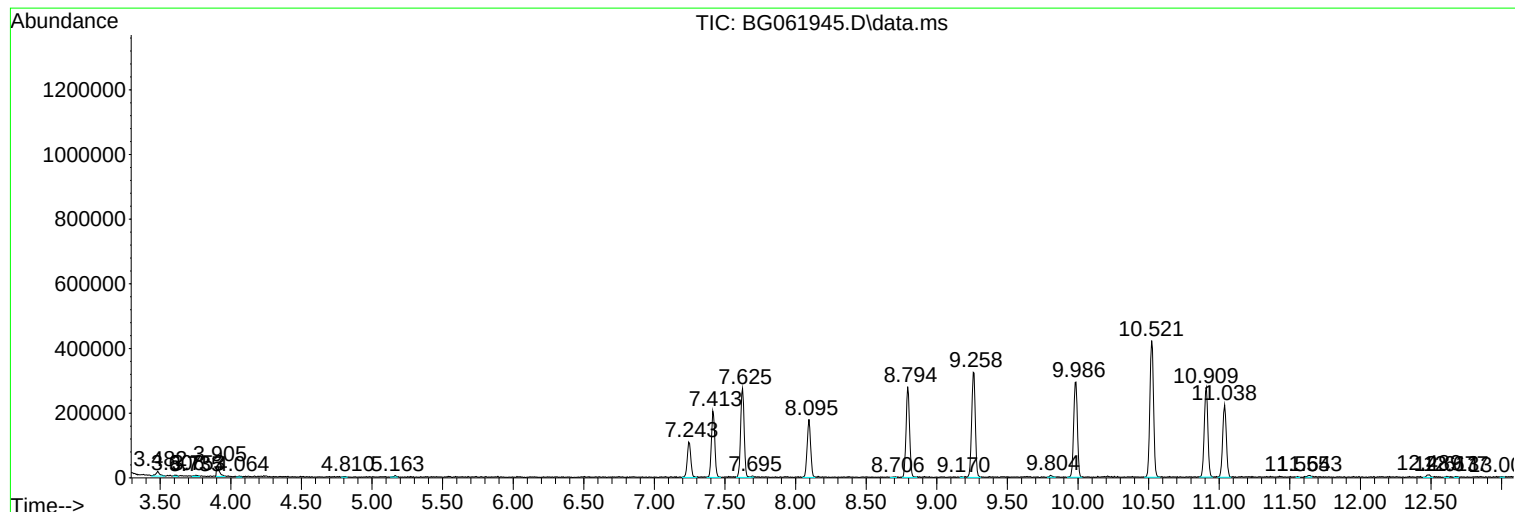

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061945.D
Acq On : 8 Jul 2024 16:47
Operator : MA/JU
Sample : P3059-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1GN2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061945.D
Acq On : 8 Jul 2024 16:47
Operator : MA/JU
Sample : P3059-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1GN2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc