

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
 Data File : BG061947.D
 Acq On : 8 Jul 2024 18:09
 Operator : MA/JU
 Sample : P3059-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E1GN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.482	28	33	37	rBV4	11971	17195	0.76%	0.086%
2	3.905	102	105	114	rBV2	47901	81535	3.60%	0.406%
3	4.234	159	161	164	rBV	2673	2888	0.13%	0.014%
4	4.375	181	185	188	rBV2	2546	3532	0.16%	0.018%
5	4.992	286	290	292	rBV	2359	3065	0.14%	0.015%
6	5.092	306	307	314	rVB3	2803	3686	0.16%	0.018%
7	5.162	314	319	320	rBV3	4381	6339	0.28%	0.032%
8	6.984	626	629	634	rVB2	2631	3365	0.15%	0.017%
9	7.095	642	648	651	rBV3	3335	4983	0.22%	0.025%
10	7.195	660	665	667	rBV2	2655	4555	0.20%	0.023%
11	7.242	667	673	685	rVB2	102880	173056	7.65%	0.862%
12	7.418	697	703	710	rVB	206093	330444	14.60%	1.646%
13	7.542	721	724	726	rBV	2712	3314	0.15%	0.017%
14	7.624	731	738	746	rVV	262356	452323	19.98%	2.253%
15	7.700	746	751	755	rVB	3324	4688	0.21%	0.023%
16	7.918	785	788	791	rBV	2180	2963	0.13%	0.015%
17	8.094	812	818	826	rVB2	184155	311528	13.76%	1.552%
18	8.464	880	881	886	rVB	2681	2880	0.13%	0.014%
19	8.793	930	937	946	rVB	264420	444206	19.62%	2.212%
20	9.081	983	986	991	rBV2	2308	3135	0.14%	0.016%
21	9.257	1009	1016	1025	rBV	312878	568646	25.12%	2.832%
22	9.381	1033	1037	1038	rBV2	4101	5101	0.23%	0.025%
23	9.710	1091	1093	1096	rBV	2809	3004	0.13%	0.015%
24	9.980	1132	1139	1151	rBV	283088	526862	23.28%	2.624%
25	10.521	1221	1231	1241	rBV2	420540	750510	33.16%	3.738%
26	10.908	1289	1297	1304	rVB	288022	520147	22.98%	2.591%
27	11.038	1310	1319	1326	rBV2	270188	481903	21.29%	2.400%
28	11.302	1360	1364	1366	rBV	2632	3026	0.13%	0.015%
29	11.637	1417	1421	1423	rBV4	6739	7787	0.34%	0.039%
30	11.942	1469	1473	1478	rVB	2466	4098	0.18%	0.020%
31	12.465	1559	1562	1563	rBV2	2483	3154	0.14%	0.016%
32	12.477	1563	1564	1569	rVB2	6861	9294	0.41%	0.046%
33	12.847	1624	1627	1630	rVB	2401	2830	0.13%	0.014%
34	14.116	1836	1843	1849	rBV	874812	1233307	54.49%	6.142%
35	14.157	1849	1850	1856	rVB3	3317	2991	0.13%	0.015%
36	14.357	1880	1884	1885	rBV2	2305	3117	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
 Data File : BG061947.D
 Acq On : 8 Jul 2024 18:09
 Operator : MA/JU
 Sample : P3059-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E1GN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

37	14.416	1887	1894	1901	rVB	846835	1342300	59.30%	6.685%
38	14.498	1905	1908	1910	rBV	2950	2823	0.12%	0.014%
39	14.716	1938	1945	1953	rVB	468086	750677	33.16%	3.739%
40	14.904	1971	1977	1984	rBV2	132587	214091	9.46%	1.066%
41	15.051	1997	2002	2003	rBV2	4199	3951	0.17%	0.020%
42	15.121	2010	2014	2019	rVB3	4331	6845	0.30%	0.034%
43	15.291	2039	2043	2045	rBV	3003	3206	0.14%	0.016%
44	15.327	2045	2049	2050	rBV	2955	3089	0.14%	0.015%
45	15.703	2106	2113	2121	rVB	1122639	1727957	76.34%	8.606%
46	15.814	2126	2132	2141	rVV	487212	705296	31.16%	3.513%
47	15.897	2145	2146	2149	rVB	3774	2923	0.13%	0.015%
48	15.944	2149	2154	2157	rBV3	8979	13824	0.61%	0.069%
49	16.308	2213	2216	2218	rBV2	2437	2959	0.13%	0.015%
50	16.373	2225	2227	2230	rBV2	2826	3707	0.16%	0.018%
51	16.743	2289	2290	2293	rVB	5433	4375	0.19%	0.022%
52	16.796	2297	2299	2301	rBV3	4338	4870	0.22%	0.024%
53	16.854	2306	2309	2312	rVV2	3439	4162	0.18%	0.021%
54	16.984	2329	2331	2334	rBV3	3337	3746	0.17%	0.019%
55	17.025	2334	2338	2341	rBV3	2286	3693	0.16%	0.018%
56	17.048	2341	2342	2345	rBV	3964	3269	0.14%	0.016%
57	17.130	2354	2356	2359	rVB2	3480	2863	0.13%	0.014%
58	17.189	2364	2366	2370	rVB3	5073	5048	0.22%	0.025%
59	17.242	2370	2375	2377	rBV3	4568	6231	0.28%	0.031%
60	17.459	2403	2412	2418	rBV	579164	900230	39.77%	4.483%
61	17.553	2422	2428	2436	rVB2	1249636	1896908	83.81%	9.447%
62	17.730	2456	2458	2462	rVB4	4282	5622	0.25%	0.028%
63	17.900	2485	2487	2488	rBV2	3506	2979	0.13%	0.015%
64	18.100	2520	2521	2525	rVB4	6760	6112	0.27%	0.030%
65	18.135	2525	2527	2529	rBV3	3241	3597	0.16%	0.018%
66	18.435	2576	2578	2580	rBV3	2545	3199	0.14%	0.016%
67	18.529	2592	2594	2596	rBV3	3855	3191	0.14%	0.016%
68	18.552	2596	2598	2599	rBV2	3465	2995	0.13%	0.015%
69	18.828	2642	2645	2646	rBV3	6741	7401	0.33%	0.037%
70	18.975	2668	2670	2672	rBV3	3616	2809	0.12%	0.014%
71	19.146	2697	2699	2700	rBV2	4218	3387	0.15%	0.017%
72	19.369	2736	2737	2739	rBV2	4696	3441	0.15%	0.017%
73	19.398	2739	2742	2748	rVB5	22104	30564	1.35%	0.152%
74	19.463	2751	2753	2758	rVB3	16517	21433	0.95%	0.107%
75	19.833	2810	2816	2822	rBV	1452532	2104758	92.99%	10.482%
76	20.051	2851	2853	2856	rBV4	8046	7276	0.32%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061947.D
Acq On : 8 Jul 2024 18:09
Operator : MA/JU
Sample : P3059-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1GN4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Title : SVOA CALIBRATION

77	21.719	3130	3137	3143	rVB	566946	925395	40.88%	4.609%
78	24.739	3641	3651	3662	rVB	792757	2263478	100.00%	11.273%
79	24.957	3680	3688	3701	rVB3	363679	1076738	47.57%	5.363%




Sum of corrected areas: 20078875

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061947.D
Acq On : 8 Jul 2024 18:09
Operator : MA/JU
Sample : P3059-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1GN4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

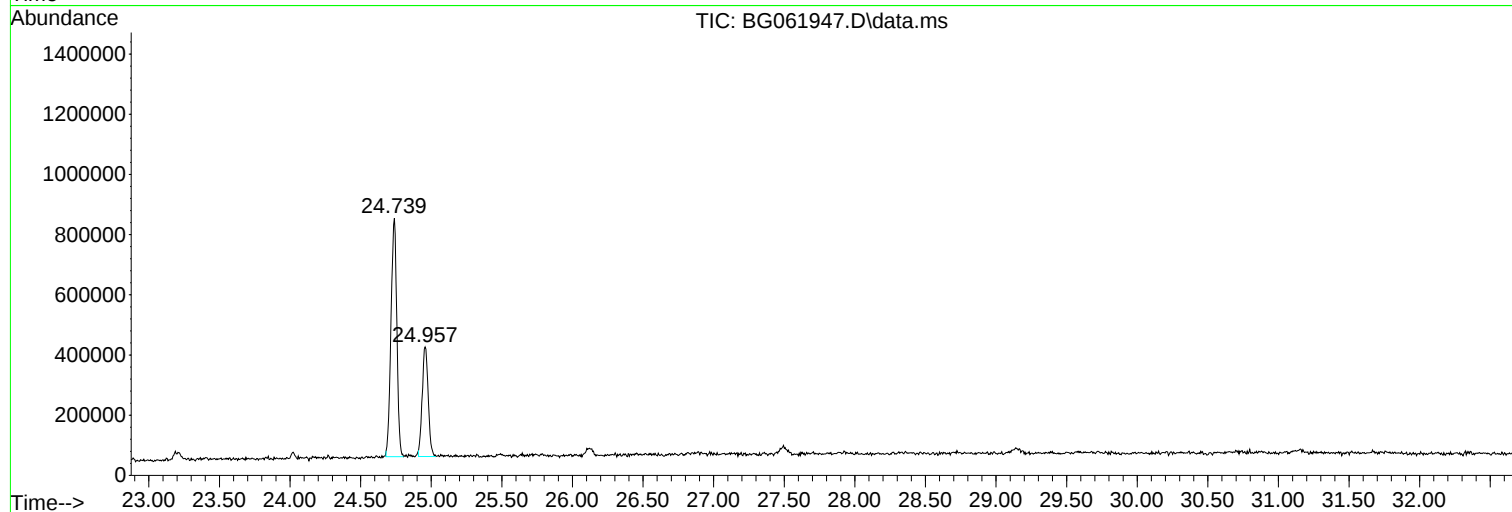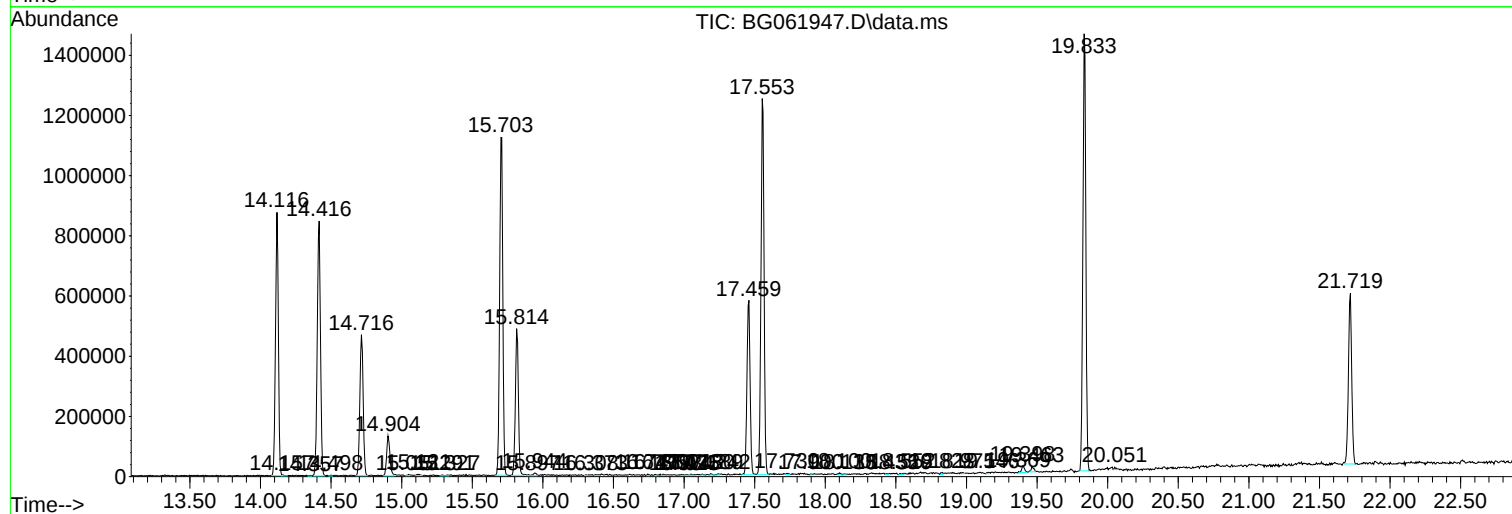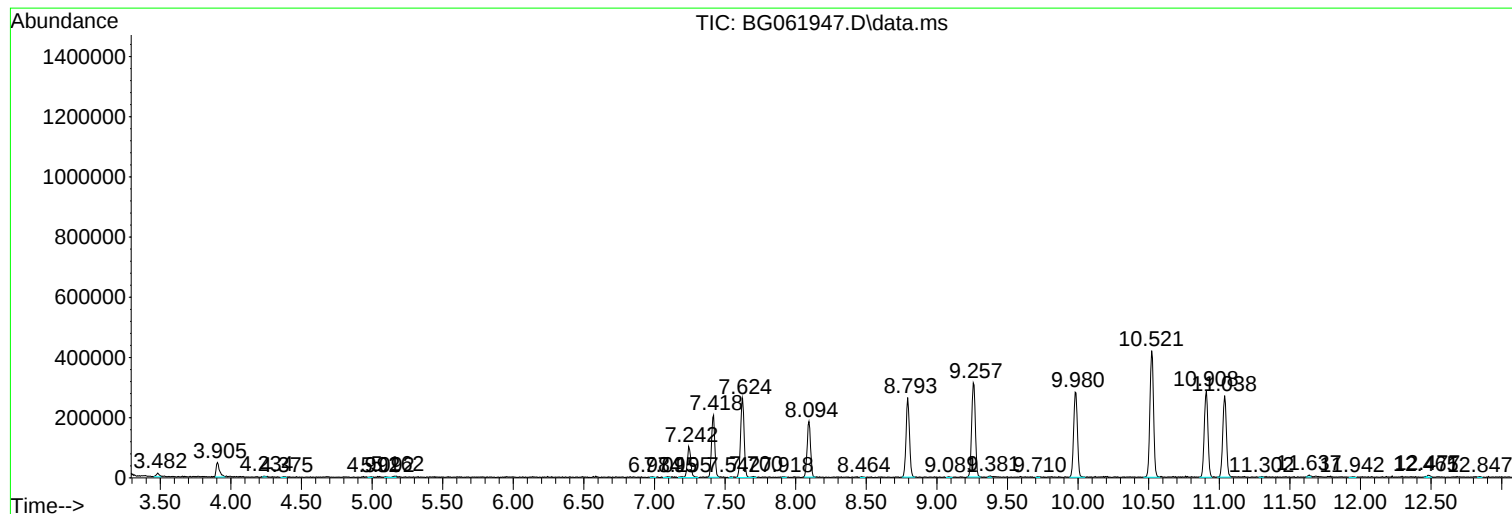

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061947.D
Acq On : 8 Jul 2024 18:09
Operator : MA/JU
Sample : P3059-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1GN4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061947.D
Acq On : 8 Jul 2024 18:09
Operator : MA/JU
Sample : P3059-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1GN4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc