

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
 Data File : BG061976.D
 Acq On : 9 Jul 2024 16:38
 Operator : MA/JU
 Sample : PB161901BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK901

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.482	29	33	37	rBV3	13111	20367	1.27%	0.118%
2	3.676	64	66	68	rBV2	3452	4033	0.25%	0.023%
3	3.899	100	104	115	rBV	172989	288425	17.95%	1.675%
4	4.240	160	162	166	rBV3	4860	5216	0.32%	0.030%
5	4.510	206	208	211	rVB2	2187	2741	0.17%	0.016%
6	4.552	211	215	217	rBV	2434	4057	0.25%	0.024%
7	4.957	281	284	285	rBV	2175	2442	0.15%	0.014%
8	5.151	315	317	321	rVB2	2567	2704	0.17%	0.016%
9	5.186	321	323	325	rBV	3081	2522	0.16%	0.015%
10	5.474	370	372	375	rVB	2341	2364	0.15%	0.014%
11	5.509	377	378	383	rBV2	2297	4123	0.26%	0.024%
12	5.856	436	437	441	rBV2	1788	2373	0.15%	0.014%
13	5.932	447	450	453	rVB2	2030	2398	0.15%	0.014%
14	6.044	465	469	471	rBV2	2528	2668	0.17%	0.015%
15	6.297	511	512	517	rBV	2214	2719	0.17%	0.016%
16	7.248	663	674	680	rBV	236148	414690	25.81%	2.409%
17	7.348	689	691	693	rBV	2708	2289	0.14%	0.013%
18	7.413	696	702	712	rVB	144948	246198	15.32%	1.430%
19	7.624	731	738	746	rVB	208337	362987	22.59%	2.108%
20	8.095	811	818	825	rVB	170703	290880	18.10%	1.690%
21	8.500	884	887	890	rBV	1990	2968	0.18%	0.017%
22	8.635	908	910	917	rBV	2592	4440	0.28%	0.026%
23	8.794	930	937	949	rBV2	282116	510683	31.78%	2.966%
24	9.258	1008	1016	1023	rBV	230302	416987	25.95%	2.422%
25	9.440	1044	1047	1050	rVB	2788	2987	0.19%	0.017%
26	9.793	1104	1107	1110	rVB2	3040	2823	0.18%	0.016%
27	9.904	1121	1126	1128	rBV	1890	2891	0.18%	0.017%
28	9.981	1131	1139	1149	rVV2	220951	399747	24.88%	2.322%
29	10.227	1179	1181	1185	rBV	1806	2399	0.15%	0.014%
30	10.521	1223	1231	1239	rBV	316439	560226	34.87%	3.254%
31	10.733	1265	1267	1269	rBV	2297	2754	0.17%	0.016%
32	10.903	1289	1296	1305	rVB	268885	499024	31.06%	2.899%
33	10.979	1307	1309	1311	rBV	2507	2561	0.16%	0.015%
34	11.038	1311	1319	1326	rBV	257525	478055	29.75%	2.777%
35	11.167	1338	1341	1343	rBV	2565	2721	0.17%	0.016%
36	11.696	1428	1431	1433	rVB	2179	2496	0.16%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
 Data File : BG061976.D
 Acq On : 9 Jul 2024 16:38
 Operator : MA/JU
 Sample : PB161901BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK901

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

37	12.478	1560	1564	1568	rBV5	8173	11956	0.74%	0.069%
38	12.513	1568	1570	1574	rVB	2291	2664	0.17%	0.015%
39	12.589	1579	1583	1585	rVB	2647	2918	0.18%	0.017%
40	13.359	1711	1714	1717	rVV	1857	2635	0.16%	0.015%
41	13.500	1733	1738	1739	rBV	2202	2345	0.15%	0.014%
42	13.612	1752	1757	1758	rVB	1970	2482	0.15%	0.014%
43	13.688	1765	1770	1773	rBV	3350	4946	0.31%	0.029%
44	13.811	1789	1791	1794	rVB	2564	2701	0.17%	0.016%
45	14.117	1837	1843	1849	rVB	636922	893125	55.59%	5.188%
46	14.411	1887	1893	1901	rVB	619318	970751	60.42%	5.639%
47	14.616	1925	1928	1929	rBV	2634	2669	0.17%	0.016%
48	14.716	1939	1945	1952	rVB2	491667	758832	47.23%	4.408%
49	14.810	1958	1961	1963	rBV	2581	3291	0.20%	0.019%
50	14.904	1970	1977	1989	rBV2	315236	513441	31.96%	2.982%
51	15.180	2021	2024	2026	rBV	3530	2860	0.18%	0.017%
52	15.327	2044	2049	2050	rVB	1880	2382	0.15%	0.014%
53	15.550	2085	2087	2089	rBV	2719	3126	0.19%	0.018%
54	15.703	2106	2113	2121	rBV	825049	1241601	77.28%	7.212%
55	15.815	2125	2132	2139	rBV	345648	505987	31.49%	2.939%
56	15.915	2146	2149	2151	rBV	3592	3541	0.22%	0.021%
57	15.950	2151	2155	2159	rVV3	5308	7175	0.45%	0.042%
58	16.026	2165	2168	2171	rVV3	2958	2980	0.19%	0.017%
59	16.062	2171	2174	2175	rVB	2606	2552	0.16%	0.015%
60	16.209	2196	2199	2202	rVB2	3672	5465	0.34%	0.032%
61	16.244	2202	2205	2206	rBV2	2689	3141	0.20%	0.018%
62	16.467	2240	2243	2245	rBV	3289	3929	0.24%	0.023%
63	16.496	2245	2248	2249	rVB	3444	3279	0.20%	0.019%
64	16.620	2265	2269	2272	rBV	3474	5401	0.34%	0.031%
65	16.690	2278	2281	2284	rBV	2450	2307	0.14%	0.013%
66	16.726	2284	2287	2289	rVB2	3017	2877	0.18%	0.017%
67	16.837	2304	2306	2310	rVB	2430	3262	0.20%	0.019%
68	16.884	2310	2314	2315	rVB	2435	2421	0.15%	0.014%
69	17.213	2368	2370	2373	rBV	2970	3189	0.20%	0.019%
70	17.307	2383	2386	2389	rBV	2367	2860	0.18%	0.017%
71	17.337	2389	2391	2394	rBV	2286	2724	0.17%	0.016%
72	17.454	2404	2411	2421	rBV	626564	964734	60.04%	5.604%
73	17.554	2421	2428	2436	rVB	903420	1353306	84.23%	7.861%
74	17.719	2455	2456	2459	rVB3	3343	2823	0.18%	0.016%
75	17.783	2466	2467	2472	rBV2	3429	2559	0.16%	0.015%
76	17.948	2493	2495	2497	rBV	3205	2659	0.17%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
 Data File : BG061976.D
 Acq On : 9 Jul 2024 16:38
 Operator : MA/JU
 Sample : PB161901BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK901

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

77	18.100	2516	2521	2522	rBV	4059	5500	0.34%	0.032%
78	18.206	2536	2539	2541	rBV2	4743	4928	0.31%	0.029%
79	18.353	2562	2564	2567	rBV2	2014	2644	0.16%	0.015%
80	18.476	2581	2585	2586	rBV2	2551	2850	0.18%	0.017%
81	18.518	2589	2592	2594	rVV2	3553	3561	0.22%	0.021%
82	18.676	2616	2619	2620	rBV2	4080	3586	0.22%	0.021%
83	18.770	2633	2635	2639	rVB3	3656	3343	0.21%	0.019%
84	18.882	2652	2654	2657	rBV2	2340	2363	0.15%	0.014%
85	18.947	2663	2665	2668	rBV2	3401	4929	0.31%	0.029%
86	19.082	2686	2688	2690	rBV2	3633	4161	0.26%	0.024%
87	19.399	2738	2742	2747	rVB5	15123	23595	1.47%	0.137%
88	19.464	2750	2753	2757	rBV2	11225	15063	0.94%	0.087%
89	19.540	2765	2766	2769	rBV2	2820	2295	0.14%	0.013%
90	19.622	2778	2780	2781	rBV	3460	2660	0.17%	0.015%
91	19.657	2784	2786	2789	rBV3	4052	4178	0.26%	0.024%
92	19.740	2797	2800	2804	rVB5	11006	13129	0.82%	0.076%
93	19.834	2809	2816	2824	rBV	1052361	1499606	93.33%	8.711%
94	20.198	2874	2878	2881	rBV6	5315	7764	0.48%	0.045%
95	21.714	3130	3136	3144	rVB2	593627	972564	60.53%	5.649%
96	24.117	3543	3545	3548	rVB4	7960	4801	0.30%	0.028%
97	24.728	3639	3649	3665	rVB2	568166	1606717	100.00%	9.333%
98	24.951	3677	3687	3699	rVB3	375174	1140114	70.96%	6.622%
99	28.277	4251	4253	4255	rBV3	8129	4741	0.30%	0.028%
100	29.252	4417	4419	4421	rBV3	9802	7048	0.44%	0.041%


Sum of corrected areas: 17215994

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061976.D
Acq On : 9 Jul 2024 16:38
Operator : MA/JU
Sample : PB161901BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK901

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

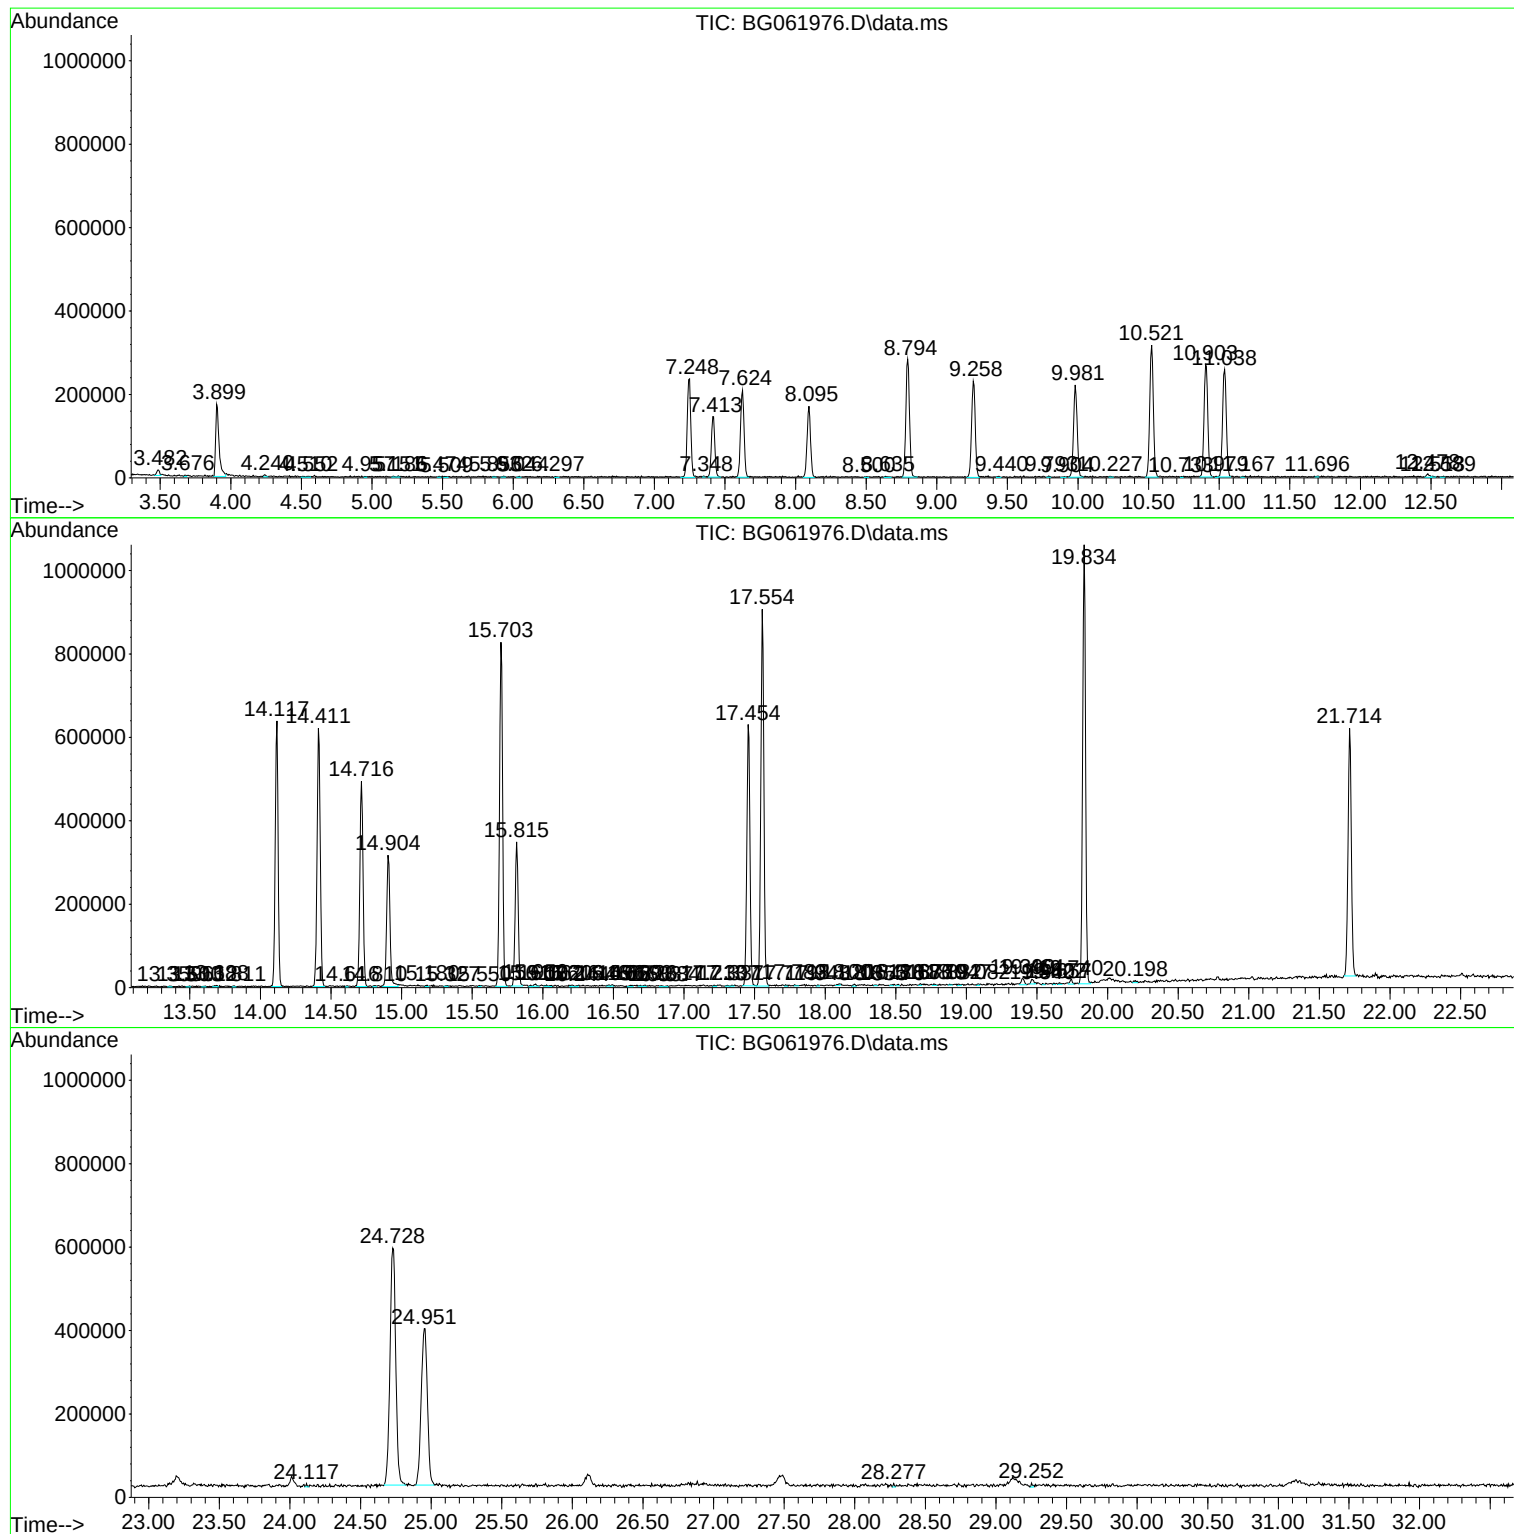

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061976.D
Acq On : 9 Jul 2024 16:38
Operator : MA/JU
Sample : PB161901BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK901

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG070824\
Data File : BG061976.D
Acq On : 9 Jul 2024 16:38
Operator : MA/JU
Sample : PB161901BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK901

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc