


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070915\
Data File : BG017802.D
Acq On : 9 Jul 2015 10:43
Operator : TP/UM
Sample : DFTPP10
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD16043

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG070915.M
Title : SVOA CALIBRATION
Last Update : Fri Jul 10 14:57:03 2015

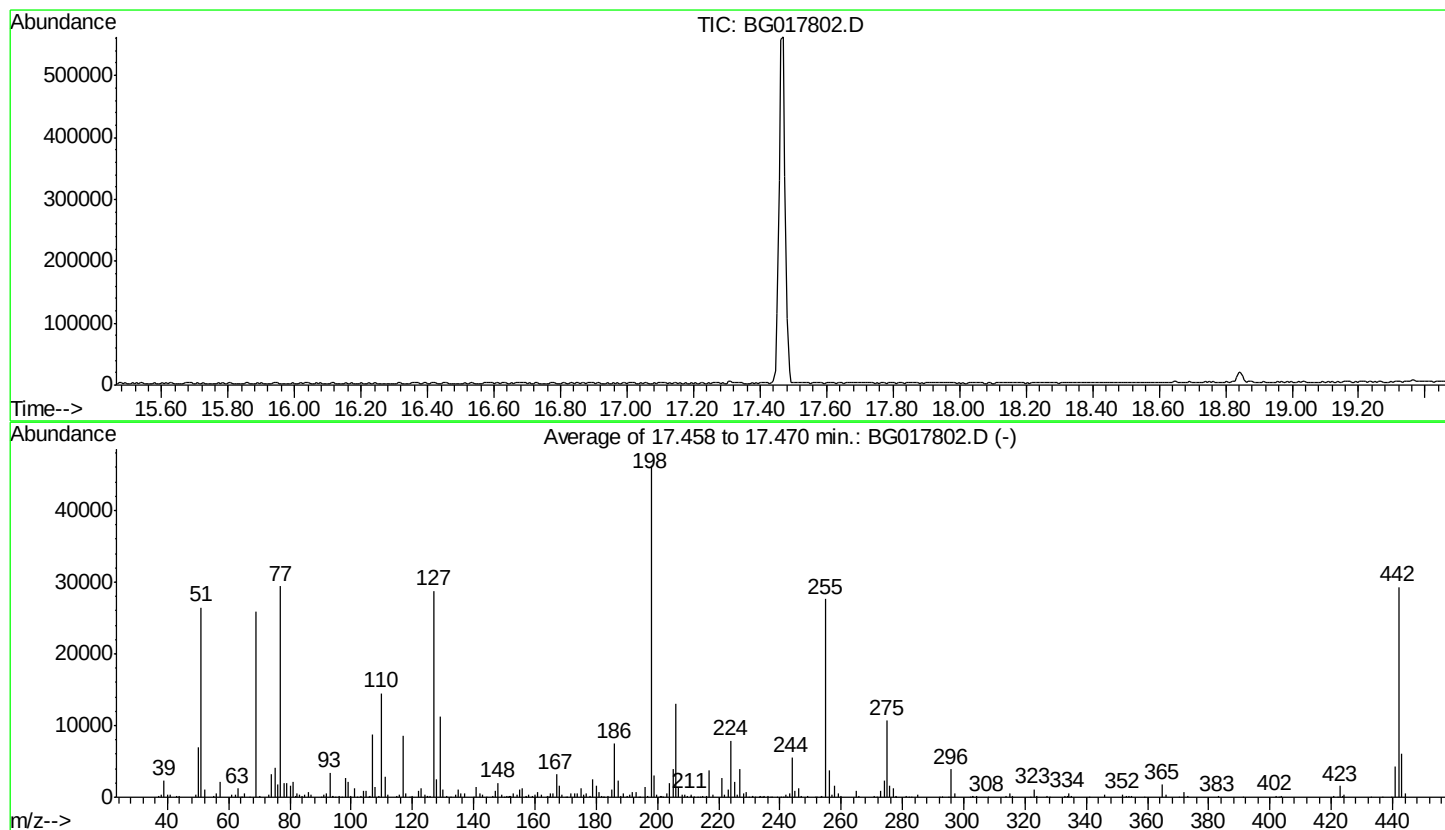

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.1	26435	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	56.0	25898	PASS
70	69	0.00	2	1.0	258	PASS
127	198	10	80	62.3	28805	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46256	PASS
199	198	5	9	6.6	3063	PASS
275	198	10	60	23.0	10647	PASS
365	198	1	100	3.8	1758	PASS
441	442	0.01	24	14.6	4297	PASS
442	198	50	100	63.5	29366	PASS
443	442	15	24	20.7	6067	PASS

m/z	Abundance
36.90	178.0
38.00	341.0
39.00	1569.0
40.00	1601.0
41.10	227.0
44.00	551.0
49.10	470.0
50.00	5514.0
51.00	19904.0
52.00	1091.0
55.10	327.0
55.90	574.0
57.00	1637.0
57.90	165.0
61.00	346.0
62.00	394.0
63.00	780.0
65.00	443.0
69.00	19904.0
70.10	161.0
73.00	245.0
74.00	2792.0
74.90	3385.0
76.00	1337.0
77.00	23304.0
78.00	1395.0
79.00	1841.0
80.00	1373.0
80.90	1431.0
81.90	559.0
83.00	385.0
84.10	184.0
85.00	302.0
86.00	463.0
91.00	632.0
91.80	579.0
93.00	2933.0
93.80	290.0
94.80	210.0
96.00	170.0
97.90	1700.0
98.90	1756.0
99.80	189.0
101.00	1006.0
103.00	478.0
104.00	910.0
104.90	703.0
105.80	245.0
107.00	6183.0
108.00	1205.0
110.00	10573.0
111.00	1857.0
112.10	239.0
115.80	279.0
117.00	5696.0
118.00	559.0
120.00	159.0
121.90	542.0
122.90	929.0
124.00	204.0
124.90	158.0
127.00	18952.0
128.00	1939.0
129.00	7614.0
129.90	810.0
130.90	254.0
133.90	221.0
135.00	991.0
135.90	193.0
136.90	658.0
141.00	1261.0
142.00	306.0
142.90	250.0
147.00	896.0
148.00	1525.0
149.00	371.0
151.80	236.0
153.00	341.0
155.00	692.0
155.90	711.0
156.90	211.0
157.90	286.0
160.00	356.0
160.90	561.0
162.00	243.0
164.70	198.0
165.90	468.0
166.90	2296.0
168.00	771.0
169.00	216.0
171.80	266.0

Instrument :
BNA_G
ClientSampleId :
SSTD16043

172.90	435.0
174.00	484.0
175.00	838.0
175.80	177.0
177.00	346.0
179.00	1662.0
180.00	1161.0
180.90	336.0
181.90	167.0
183.80	177.0
184.90	834.0
186.00	4981.0
187.00	1541.0
188.00	208.0
188.90	398.0
190.90	415.0
191.90	574.0
193.00	671.0
195.90	694.0
196.60	361.0
197.90	30784.0
198.90	2345.0
199.80	250.0
201.40	169.0
202.90	660.0
204.00	1318.0
205.00	2767.0
206.00	9203.0
207.00	1490.0
208.00	266.0
208.90	267.0
210.90	521.0
211.80	156.0
213.70	188.0
216.90	1934.0
218.00	381.0
221.00	1601.0
222.00	340.0
222.90	595.0
224.00	4747.0
225.00	1377.0
225.90	373.0
226.90	2608.0
228.00	271.0
228.90	683.0
231.00	254.0
233.70	309.0
239.10	154.0
242.20	193.0
242.90	557.0
244.00	3154.0
245.00	603.0
245.90	892.0
246.80	295.0
248.90	213.0
255.00	17840.0
255.90	2258.0
256.90	322.0
258.00	1449.0
259.00	375.0
265.00	615.0
265.90	159.0
272.90	663.0
273.90	1280.0
274.90	7538.0
276.00	1015.0
276.90	752.0
281.00	350.0
284.90	211.0
296.00	1885.0
296.90	346.0
315.00	190.0
323.00	540.0
327.00	203.0
333.90	620.0
341.00	170.0
345.90	176.0
352.00	240.0
364.90	993.0
365.90	173.0
370.20	167.0
372.00	311.0
373.00	160.0
383.00	151.0
421.00	199.0
423.10	717.0
423.80	318.0
441.00	2116.0
442.00	14722.0
442.90	3211.0
444.00	210.0

Instrument :
BNA_G
ClientSampleId :
SSTD16043

m/z	Abundance
36.90	153.0
38.00	396.0
39.00	3172.0
40.00	1191.0
41.10	336.0
43.00	343.0
44.00	471.0
49.20	610.0
50.00	8379.0
51.00	31048.0
52.00	1090.0
55.10	527.0
56.00	1052.0
57.00	2800.0
60.90	260.0
62.10	603.0
63.00	1615.0
63.90	151.0
65.10	489.0
67.00	226.0
69.00	28928.0
70.10	271.0
73.10	354.0
74.00	3438.0
75.00	4370.0
76.00	1928.0
77.00	34520.0
78.00	2408.0
79.00	2314.0
80.00	1743.0
81.00	2625.0
82.10	776.0
83.00	600.0
83.90	314.0
84.90	479.0
85.90	960.0
87.00	421.0
90.00	179.0
90.90	554.0
92.00	669.0
93.00	4403.0
94.00	328.0
96.10	208.0
96.90	164.0
98.00	2880.0
99.00	2216.0
99.70	172.0
101.00	1003.0
101.80	199.0
103.90	731.0
105.00	999.0
106.00	340.0
107.00	10073.0
107.90	1399.0
108.90	476.0
110.00	17776.0
110.90	3453.0
112.00	423.0
114.90	233.0
116.90	10154.0
117.90	430.0
118.90	193.0
120.00	330.0
121.90	982.0
122.90	1278.0
123.80	258.0
124.80	566.0
127.00	33256.0
127.90	2662.0
129.00	13691.0
129.90	1210.0
131.00	278.0
132.40	178.0
134.00	494.0
135.00	1089.0
135.90	708.0
136.90	651.0
139.90	173.0
140.90	1744.0
142.00	530.0
142.90	468.0
146.00	482.0
147.00	921.0
148.00	2545.0
149.00	457.0
150.90	174.0
151.50	251.0
153.00	528.0
154.00	580.0
154.90	1185.0
155.90	1383.0

Instrument :
BNA_G
ClientSampleId :
SSTD16043

157.10	330.0
157.90	445.0
159.90	645.0
160.90	700.0
162.00	337.0
164.10	173.0
164.90	1061.0
165.90	528.0
167.00	3678.0
168.00	1659.0
169.00	196.0
169.90	169.0
170.50	154.0
171.90	636.0
173.00	803.0
174.00	827.0
175.00	1457.0
176.00	491.0
176.80	530.0
177.90	314.0
178.90	2543.0
179.90	1877.0
180.90	880.0
181.90	174.0
182.20	214.0
182.40	198.0
183.90	317.0
185.00	1228.0
186.00	7548.0
186.90	2585.0
188.10	373.0
189.00	729.0
189.90	308.0
190.90	333.0
192.00	891.0
192.90	591.0
193.80	231.0
195.90	1730.0
197.90	56064.0
198.90	3497.0
199.90	347.0
201.10	152.0
201.50	236.0
202.90	332.0
204.00	2293.0
205.00	3938.0
206.00	14630.0
207.00	2747.0
207.90	692.0
208.80	353.0
209.80	151.0
211.10	462.0
212.00	202.0
214.90	289.0
216.90	4411.0
217.90	403.0
220.90	3100.0
223.00	1161.0
224.00	9800.0
225.00	2662.0
226.00	254.0
227.00	4567.0
227.90	640.0
229.00	785.0
230.80	218.0
231.80	233.0
233.00	155.0
234.00	274.0
234.90	277.0
235.90	212.0
237.10	169.0
240.10	207.0
241.90	524.0
243.00	505.0
244.00	6715.0
244.90	1194.0
245.90	1673.0
246.90	284.0
248.90	224.0
251.40	244.0
252.10	151.0
255.00	30840.0
255.90	4290.0
257.00	415.0
257.90	1542.0
258.90	481.0
264.90	869.0
271.00	180.0
273.00	1164.0
274.00	3013.0
275.00	12158.0
276.00	1862.0
276.90	1459.0
277.80	240.0
284.90	448.0

Instrument :
BNA_G
ClientSampleId :
SSTD16043

292.80	275.0
296.00	4845.0
297.00	711.0
301.90	217.0
302.80	521.0
304.00	330.0
307.80	203.0
314.00	439.0
315.00	668.0
316.00	284.0
323.00	1128.0
324.00	175.0
327.10	236.0
328.10	174.0
334.10	611.0
334.90	274.0
345.90	322.0
351.80	436.0
353.00	232.0
353.80	287.0
354.90	161.0
358.90	212.0
365.00	2048.0
366.00	377.0
372.00	723.0
373.10	179.0
401.90	220.0
420.90	324.0
422.00	155.0
423.00	1710.0
424.10	567.0
436.70	162.0
441.00	4890.0
442.00	32304.0
443.00	6532.0
444.00	508.0

Instrument :
BNA_G
ClientSampleId :
SSTD16043

m/z	Abundance
37.00	172.0
38.10	392.0
39.00	2012.0
39.90	1350.0
41.00	267.0
44.10	353.0
48.90	326.0
50.00	7280.0
51.00	28832.0
52.10	1171.0
55.00	186.0
55.90	722.0
57.00	1908.0
60.90	383.0
62.00	310.0
63.00	1316.0
64.10	178.0
65.00	490.0
69.00	28864.0
70.00	344.0
73.20	356.0
74.00	3287.0
75.00	4653.0
76.00	2130.0
77.00	30544.0
78.00	2560.0
79.00	1827.0
80.00	1762.0
81.00	2394.0
82.10	663.0
82.90	961.0
84.90	465.0
85.90	800.0
86.90	480.0
90.90	606.0
91.90	843.0
93.00	3094.0
94.10	295.0
95.90	200.0
98.00	3462.0
99.00	2473.0
99.90	172.0
101.00	1510.0
102.80	185.0
103.90	846.0
105.00	1086.0
107.00	9884.0
107.90	1668.0
110.00	15134.0
111.00	3049.0
112.00	418.0
114.70	158.0
115.90	706.0
117.00	9638.0
117.90	435.0
122.00	926.0
123.00	1441.0
123.90	404.0
125.00	538.0
125.90	336.0
127.00	34208.0
128.00	2965.0
128.90	12675.0
129.90	1127.0
131.00	278.0
133.90	291.0
134.90	1168.0
136.00	480.0
137.00	486.0
140.90	1497.0
142.00	701.0
142.80	306.0
144.00	184.0
146.00	321.0
146.90	980.0
147.90	1971.0
149.00	438.0
149.90	233.0
151.00	197.0
151.20	205.0
151.50	165.0
151.90	420.0
153.00	493.0
154.00	450.0
155.00	1223.0
156.00	1603.0
157.00	362.0
157.90	319.0
159.00	293.0
159.80	336.0
160.90	638.0

Instrument :
BNA_G
ClientSampleId :
SSTD16043

161.90	266.0
163.80	208.0
164.20	226.0
165.00	728.0
166.00	557.0
166.90	3561.0
167.90	2212.0
168.90	547.0
172.00	509.0
172.80	373.0
173.90	452.0
175.00	1288.0
176.00	342.0
176.90	788.0
177.90	234.0
178.90	3313.0
180.00	1753.0
181.00	804.0
183.90	231.0
185.00	1383.0
186.00	9769.0
186.90	2930.0
188.90	489.0
191.00	351.0
191.90	868.0
192.90	916.0
194.10	200.0
196.00	1659.0
197.90	51920.0
198.90	3348.0
199.80	267.0
201.00	215.0
201.70	159.0
202.90	372.0
203.90	2239.0
205.00	4993.0
206.00	15254.0
207.00	2165.0
207.80	947.0
209.00	227.0
209.70	219.0
210.90	698.0
213.00	229.0
214.80	163.0
215.90	552.0
216.90	4911.0
217.90	483.0
221.00	3574.0
221.80	664.0
222.90	1226.0
224.00	9274.0
225.00	2611.0
226.00	289.0
226.90	4580.0
228.00	466.0
228.90	961.0
229.90	245.0
231.10	316.0
234.20	203.0
235.00	407.0
236.00	259.0
236.80	261.0
241.00	226.0
242.00	657.0
243.00	469.0
244.00	6601.0
244.90	1036.0
245.90	1228.0
253.10	270.0
253.80	394.0
255.00	34200.0
255.90	4647.0
256.90	439.0
258.00	2090.0
259.00	551.0
259.80	347.0
264.90	1124.0
265.90	243.0
270.80	230.0
271.60	158.0
273.00	890.0
273.90	2547.0
275.00	12247.0
275.90	1830.0
277.00	1822.0
278.00	404.0
282.00	255.0
282.80	229.0
285.00	385.0
291.90	166.0
293.00	281.0
294.80	182.0
296.00	4935.0
297.00	645.0
303.00	735.0

Instrument :
BNA_G
ClientSampleId :
SSTD16043

313.90	227.0
315.00	573.0
316.00	275.0
321.80	202.0
322.90	1608.0
323.90	318.0
327.00	279.0
333.00	449.0
334.00	1093.0
335.00	260.0
346.00	429.0
351.90	559.0
353.10	357.0
353.90	477.0
354.90	232.0
365.00	2234.0
365.90	315.0
371.90	917.0
383.10	204.0
390.90	171.0
402.00	451.0
403.00	257.0
403.80	317.0
420.80	184.0
423.00	2364.0
424.00	370.0
432.70	161.0
439.40	232.0
441.00	5886.0
442.00	41072.0
443.00	8459.0
444.00	976.0

Instrument :
BNA_G
ClientSampleId :
SSTD16043

Scan 2510 (17.434 min): BG017802.D
DFTPP10

m/z	Abundance
39.90	1000.0
44.00	325.0
48.90	280.0
50.00	168.0
51.00	159.0
55.00	192.0
56.00	182.0
58.00	186.0
78.00	178.0
83.10	205.0
91.00	192.0
207.00	652.0
208.10	225.0
270.10	154.0

Instrument :
BNA_G
ClientSampleId :
SSTD16043