
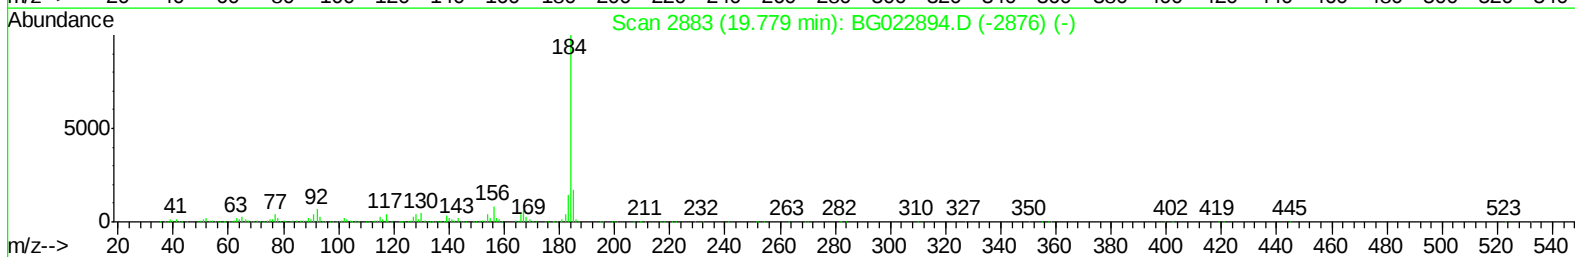
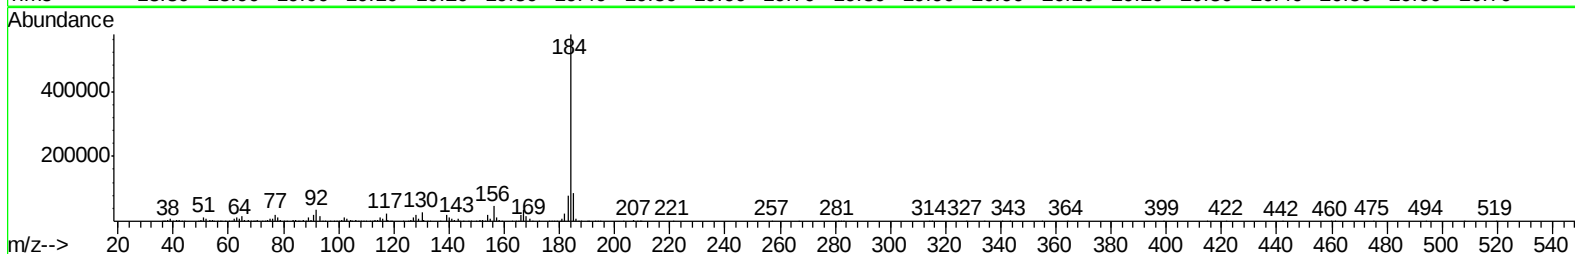


Data Path : Z:\HPCHEM1\BNA_G\Data\BG070916\
Data File : BG022934.D
Acq On : 8 Jul 2016 17:24
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 08:17:59 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 16:51:07 2016
Response via : Initial Calibration

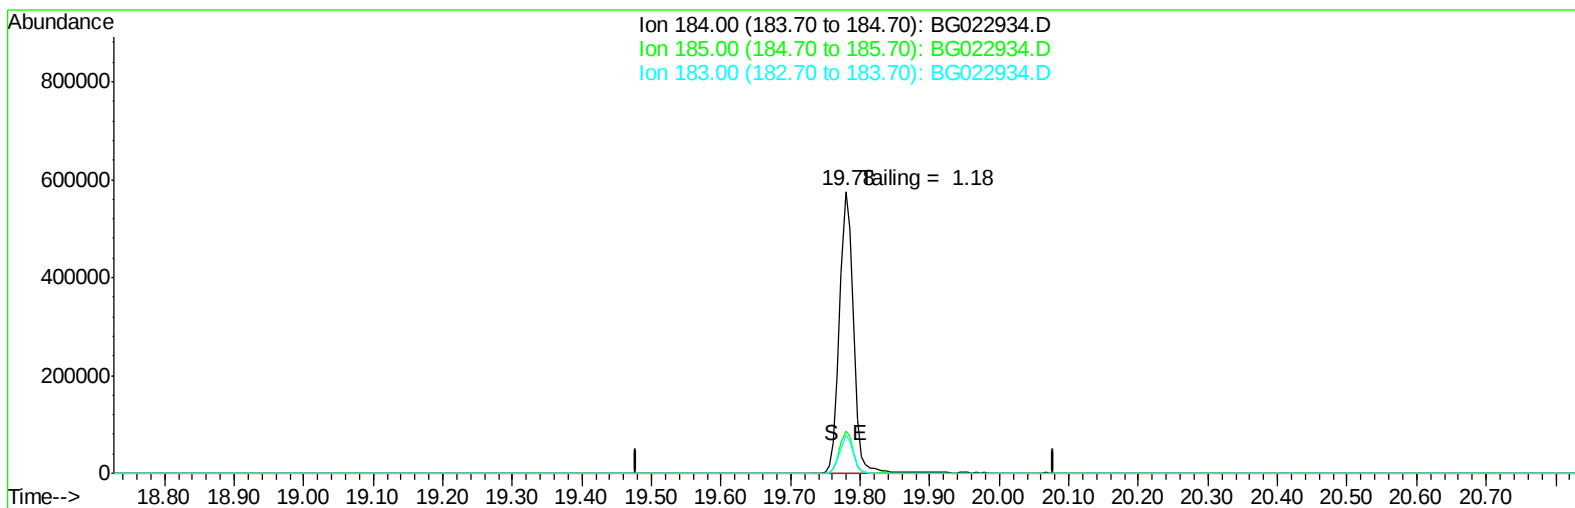

TIC: BG022934.D

(76) Benzidine




19.779min (-19.779) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	15.80	0.00#
183.00	13.40	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG070916\
Data File : BG022934.D
Acq On : 8 Jul 2016 17:24
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 08:17:59 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 16:51:07 2016
Response via : Initial Calibration

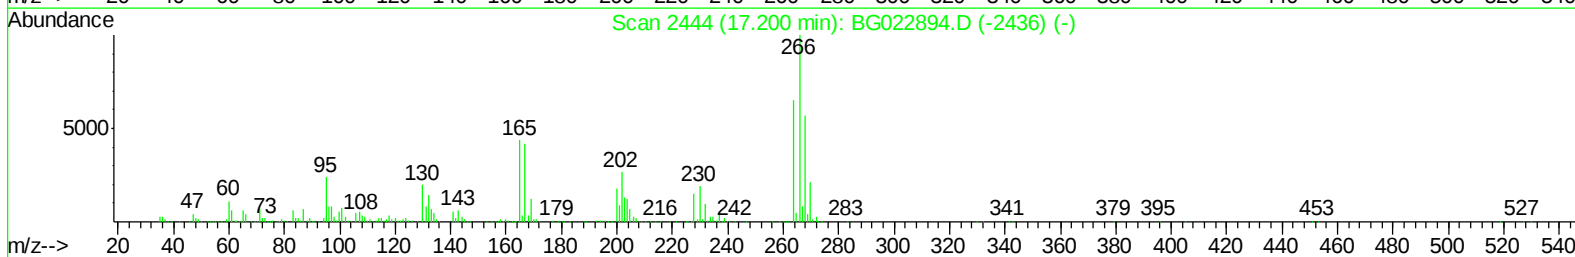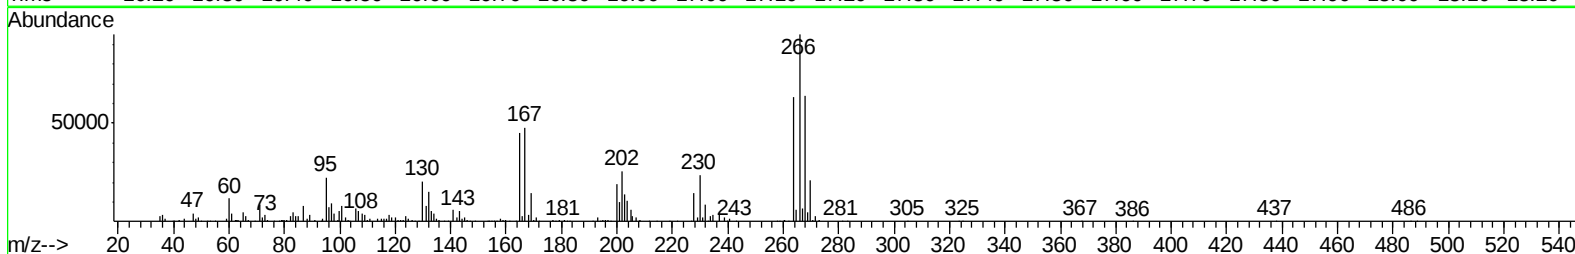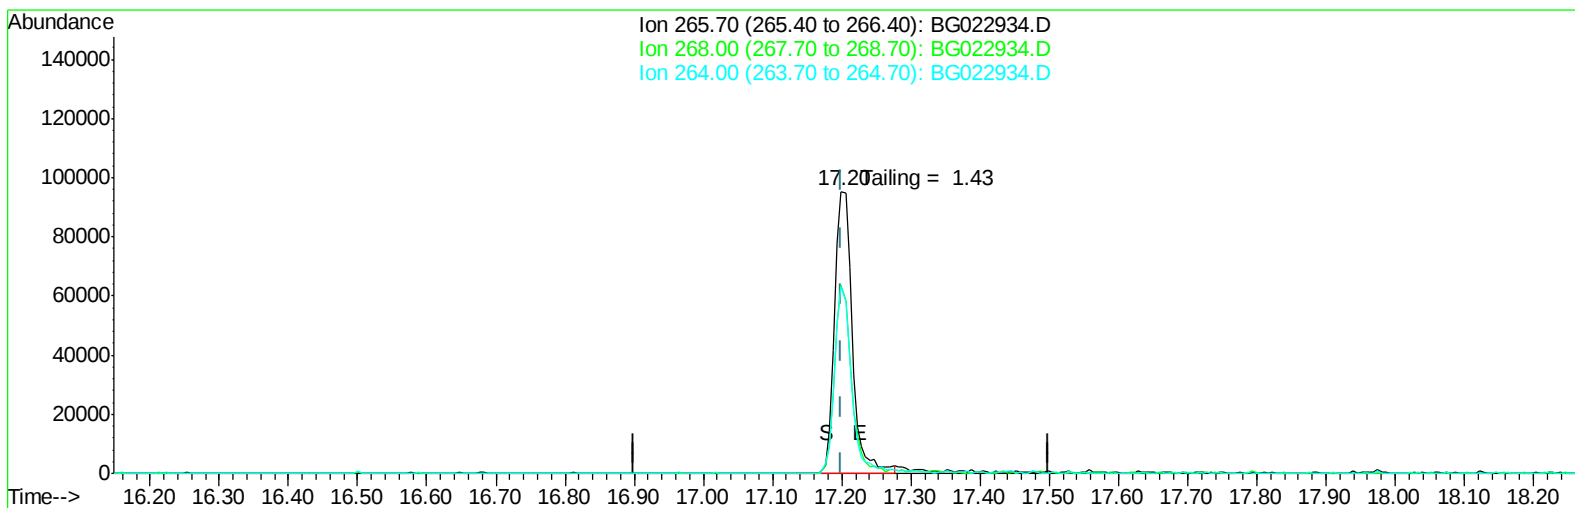

TIC: BG022934.D

(69) Pentachlorophenol (C)

17.199min (-0.001) 223062.58ng

response 167564

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	66.91
264.00	63.20	66.30
0.00	0.00	0.00