


Data Path : V:\HPCHEM1\BNA G\DATA\BG070916\
 Data File : BG022934.D
 Acq On : 8 Jul 2016 17:24
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 07 16:51:07 2016

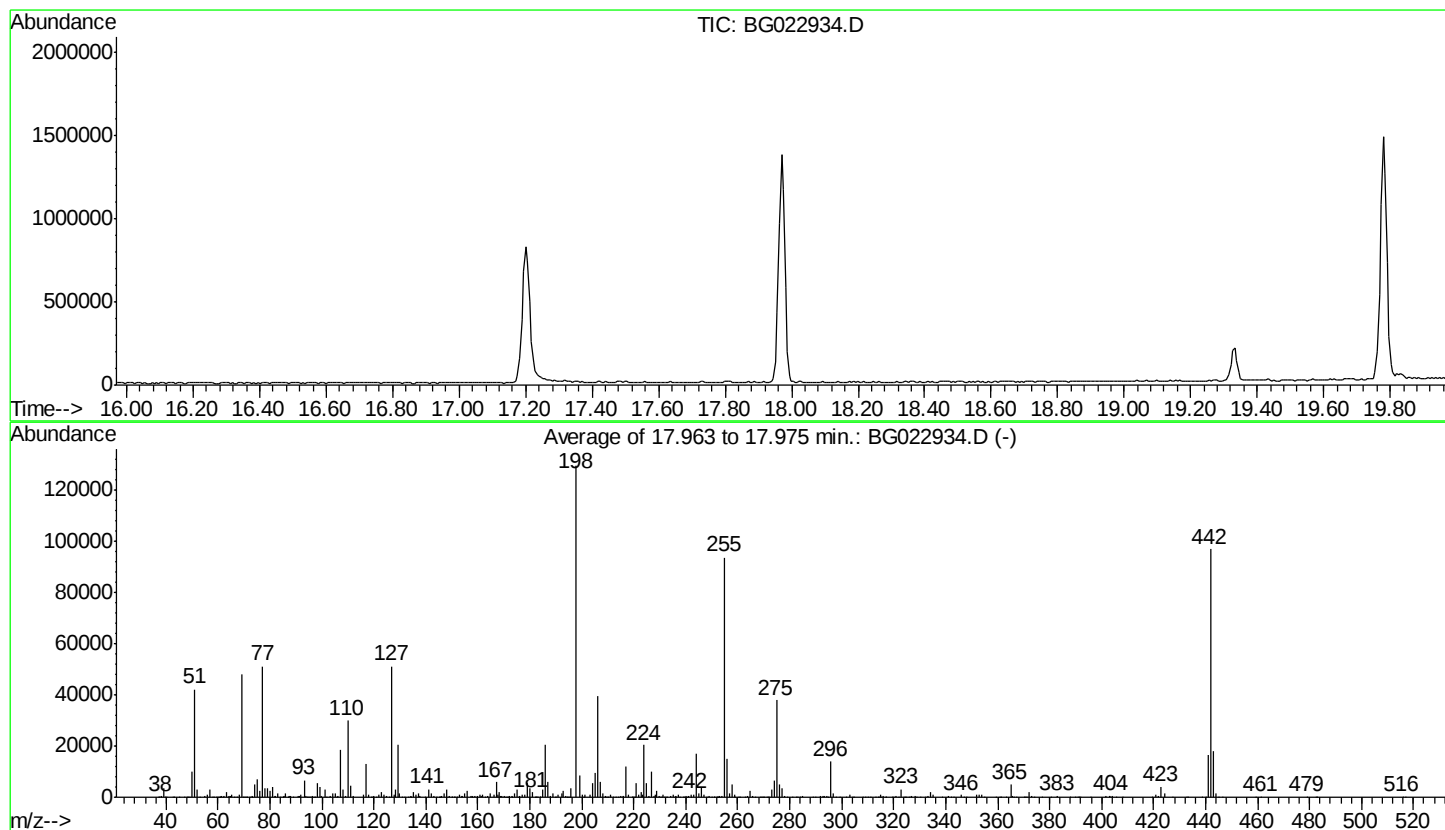

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	42112	PASS
68	69	0.00	2	1.7	835	PASS
69	198	0.00	100	36.9	47758	PASS
70	69	0.00	2	0.2	116	PASS
127	198	10	80	39.5	51101	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	129362	PASS
199	198	5	9	6.6	8587	PASS
275	198	10	60	29.2	37768	PASS
365	198	1	100	3.8	4874	PASS
441	442	0.01	24	16.9	16340	PASS
442	198	50	100	74.8	96728	PASS
443	442	15	24	18.4	17813	PASS