


Data Path : V:\HPCHEM1\BNA G\DATA\BG070916\
Data File : BG022950.D
Acq On : 9 Jul 2016 4:06
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 07 16:51:07 2016

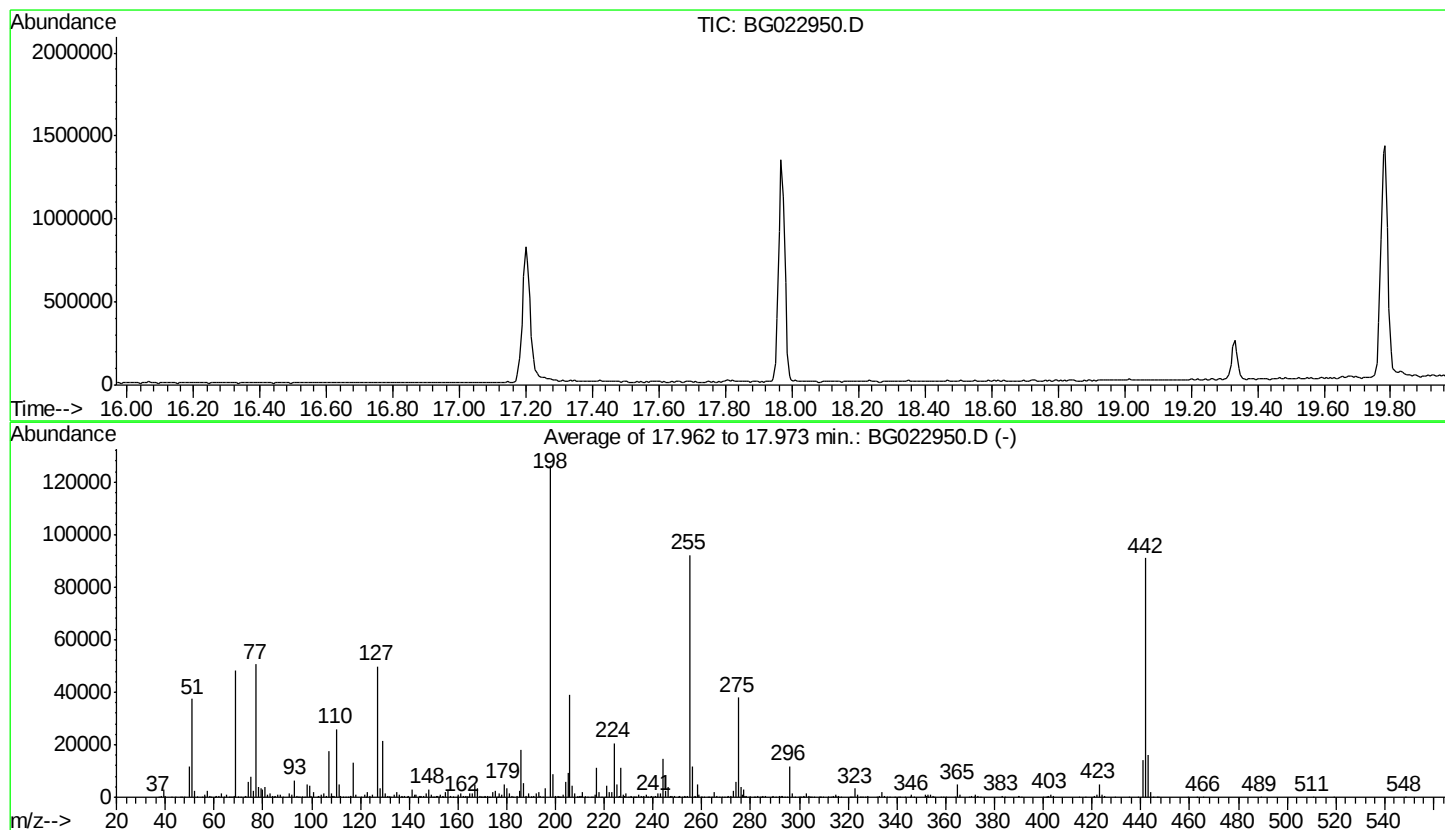

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.6	37352	PASS
68	69	0.00	2	1.1	547	PASS
69	198	0.00	100	38.1	48053	PASS
70	69	0.00	2	0.3	142	PASS
127	198	10	80	39.4	49792	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	126245	PASS
199	198	5	9	7.1	8984	PASS
275	198	10	60	29.9	37810	PASS
365	198	1	100	3.8	4818	PASS
441	442	0.01	24	15.3	13935	PASS
442	198	50	100	72.1	91026	PASS
443	442	15	24	17.7	16076	PASS