
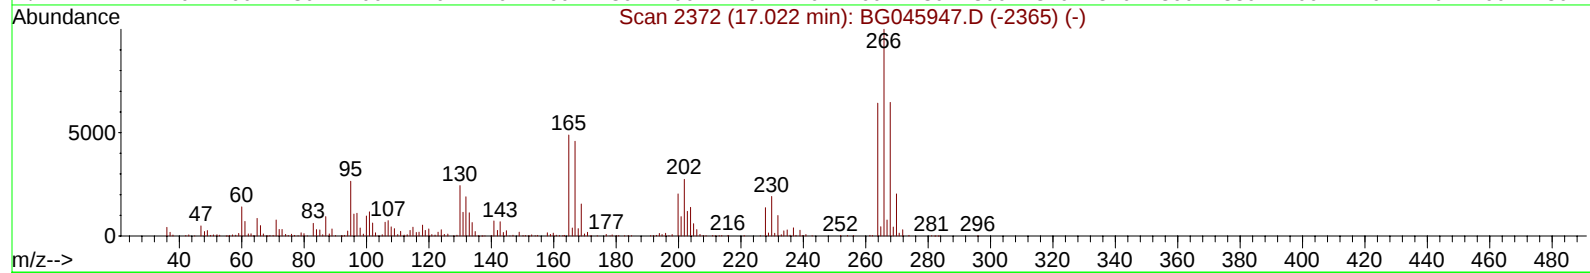
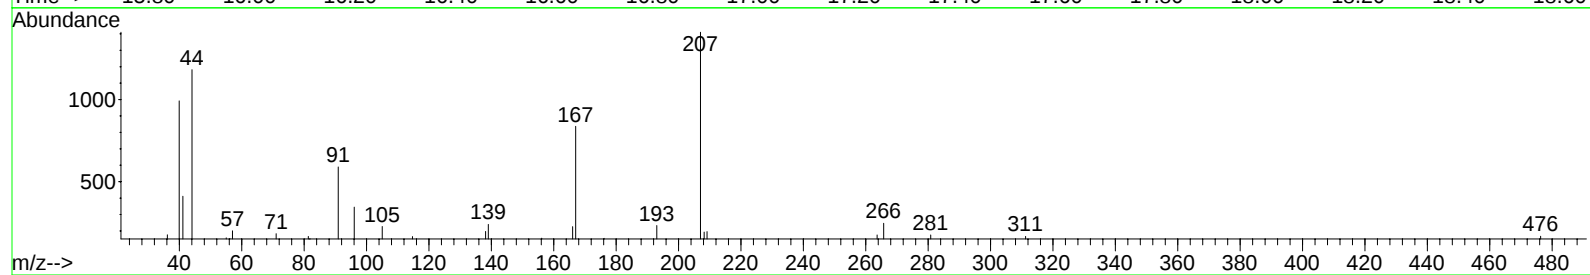


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070920\
Data File : BG045986.D
Acq On : 9 Jul 2020 8:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 09 16:09:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG070620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 07 09:58:42 2020
Response via : Initial Calibration

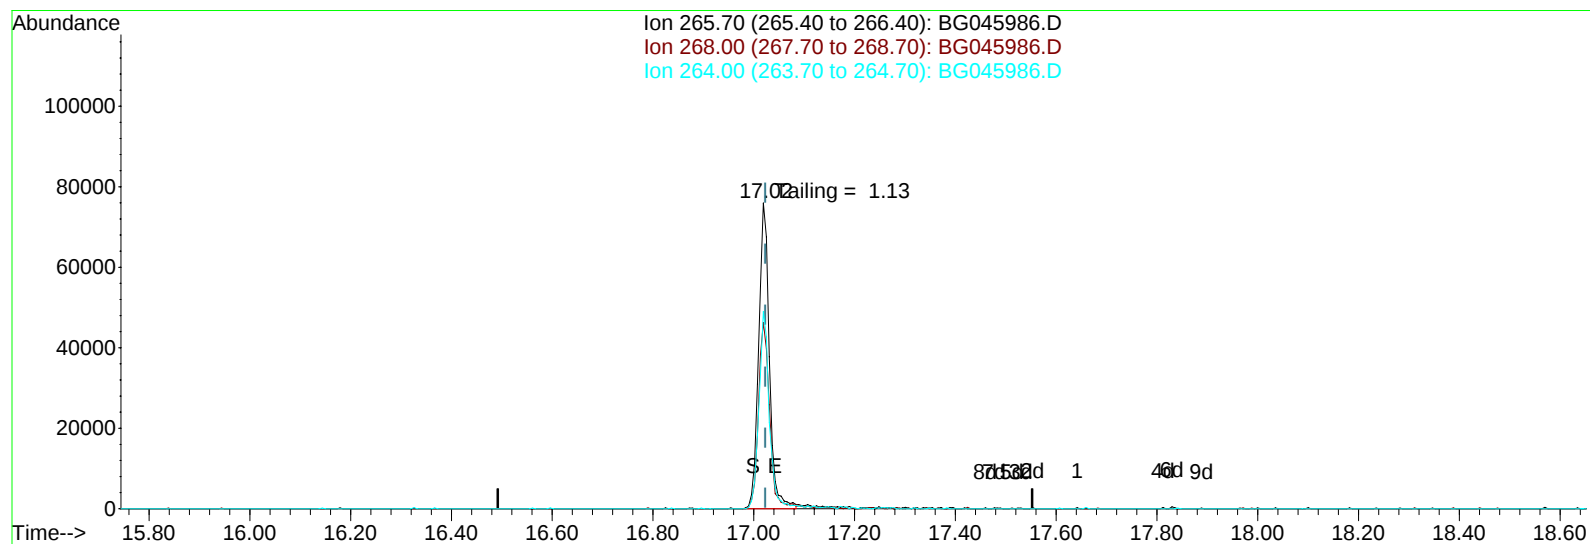

TIC: BG045986.D

(70) Pentachlorophenol (C)




17.642min (+0.619) 208.39ng

response 87

Ion	Exp%	Act%
265.70	100	100
268.00	64.80	0.00#
264.00	64.20	0.00#
0.00	0.00	0.00

```
Data Path   : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG070920\  
Data File   : BG045986.D  
Acq On      : 9 Jul 2020      8:23  
Operator    : CG/JU  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Jul 09 16:09:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG070620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 07 09:58:42 2020
Response via : Initial Calibration

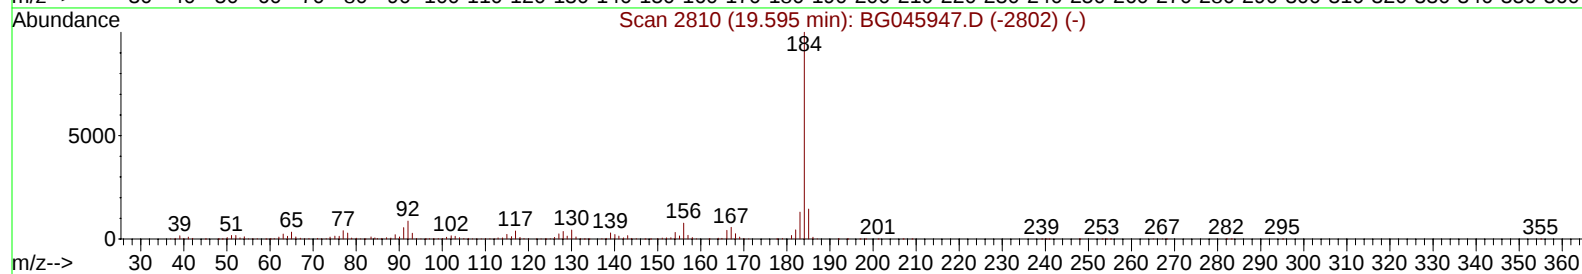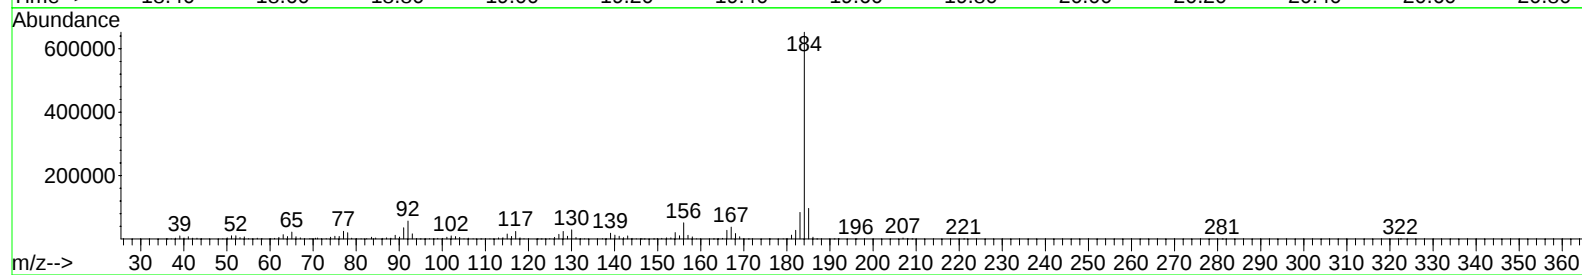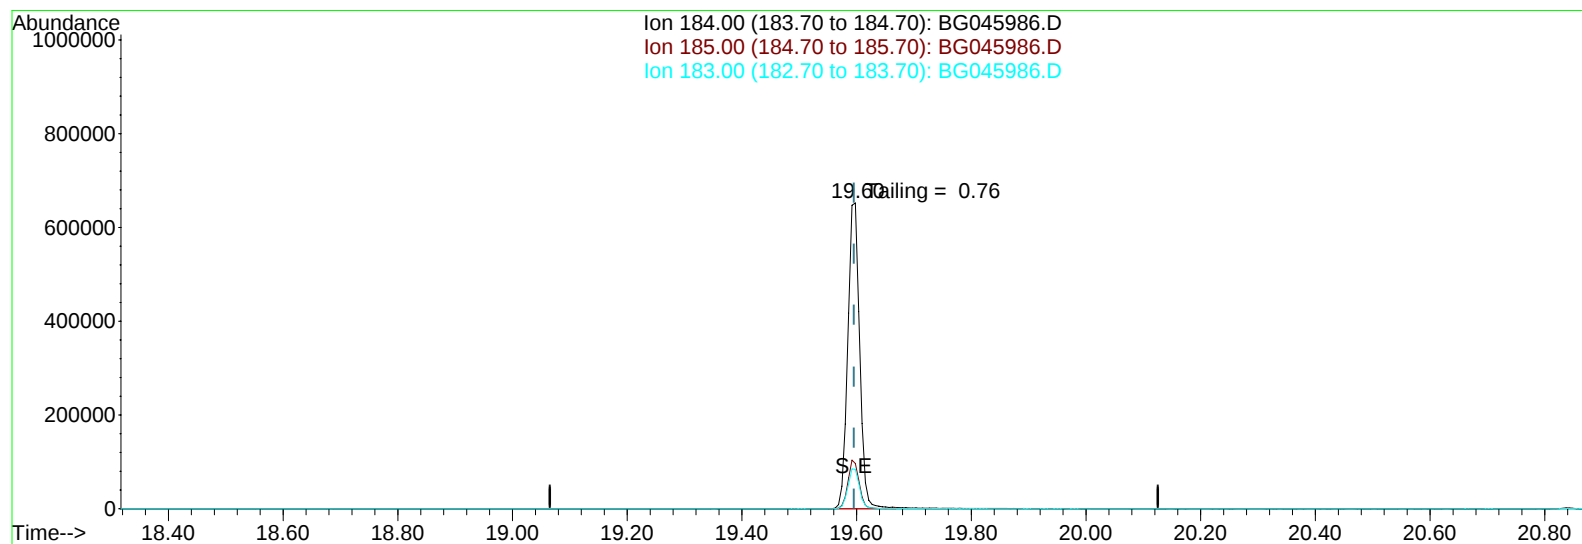

TIC: BG045986.D

(77) Benzidine

19.598min (+0.002) 446932.79ng

response 932864

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	14.82
183.00	13.00	12.87
0.00	0.00	0.00