


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG070920\
 Data File : BG045986.D
 Acq On : 9 Jul 2020 8:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG070620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 07 09:58:42 2020

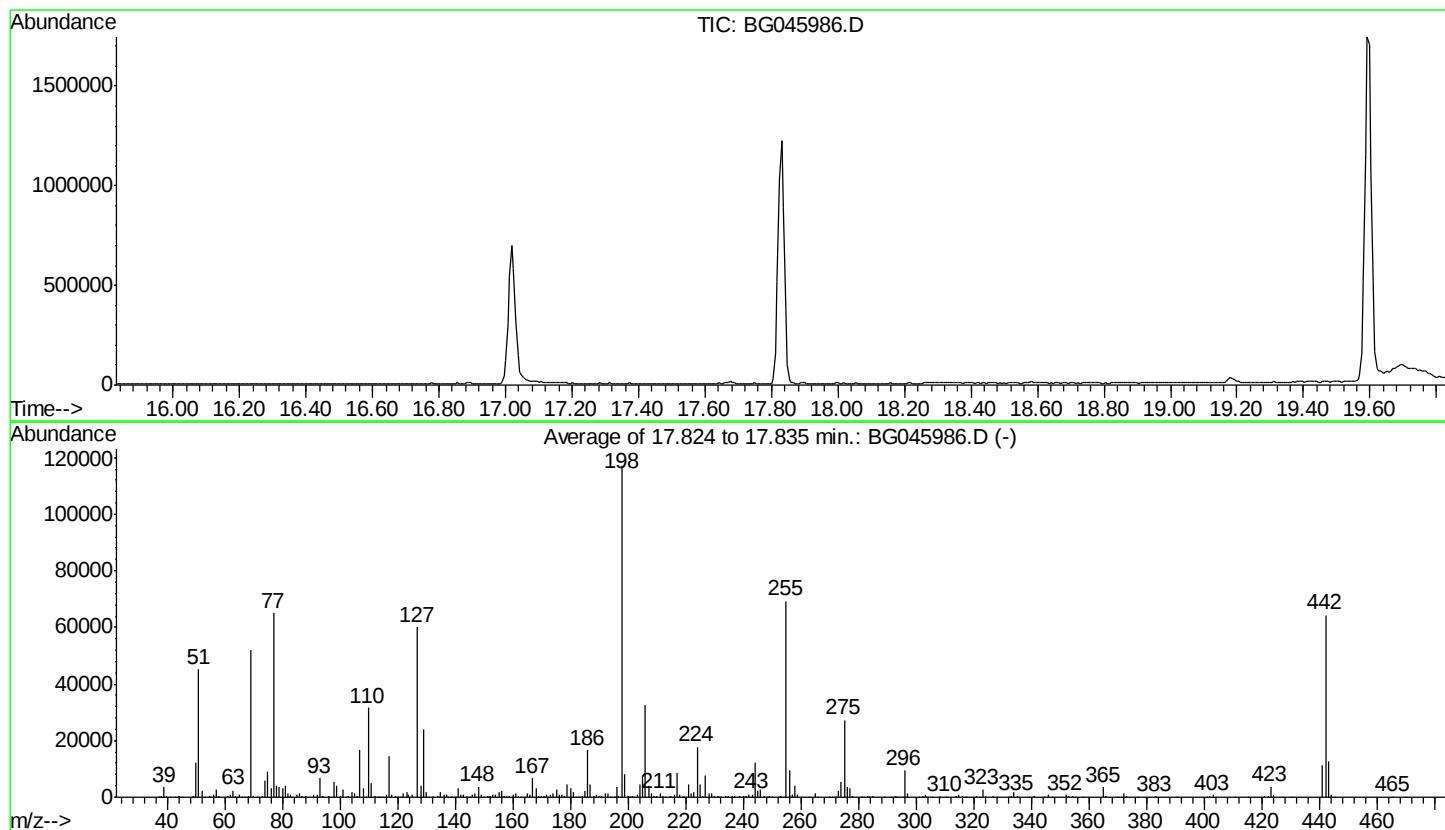

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	45221	PASS
68	69	0.00	2	1.3	649	PASS
69	198	0.00	100	44.3	51859	PASS
70	69	0.00	2	0.7	343	PASS
127	198	10	80	51.3	60136	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	117149	PASS
199	198	5	9	7.1	8332	PASS
275	198	10	60	23.3	27338	PASS
365	198	1	100	3.1	3593	PASS
441	198	0.01	100	9.6	11205	PASS
442	198	50	100	54.9	64373	PASS
443	442	15	24	19.9	12798	PASS