

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071016\
 Data File : BG022973.D
 Acq On : 9 Jul 2016 20:08
 Operator : UM/SJ
 Sample : H3889-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SS-5

Quant Time: Jul 11 02:29:15 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 16:51:07 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	105788	20.00	ng	0.00
21) Naphthalene-d8	10.98	136	487025	20.00	ng	0.00
38) Acenaphthene-d10	14.79	164	378649	20.00	ng	0.00
63) Phenanthrene-d10	17.55	188	883870	20.00	ng	0.00
75) Chrysene-d12	21.84	240	962043	20.00	ng	0.00
86) Perylene-d12	25.21	264	972367	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.70	112	566107	87.52	ng	0.00
7) Phenol-d6	7.30	99	1072968	105.91	ng	0.00
23) Nitrobenzene-d5	9.32	82	787758	69.26	ng	0.00
41) 2,4,6-Tribromophenol	16.29	330	679544	99.86	ng	0.00
44) 2-Fluorobiphenyl	13.41	172	1774639	73.82	ng	0.00
78) Terphenyl-d14	20.15	244	2491096	80.49	ng	0.00
Target Compounds						
49) Dimethylphthalate	14.24	163	356007	11.51	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071016\
Data File : BG022973.D
Acq On : 9 Jul 2016 20:08
Operator : UM/SJ
Sample : H3889-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SS-5

Quant Time: Jul 11 02:29:15 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 16:51:07 2016
Response via : Initial Calibration

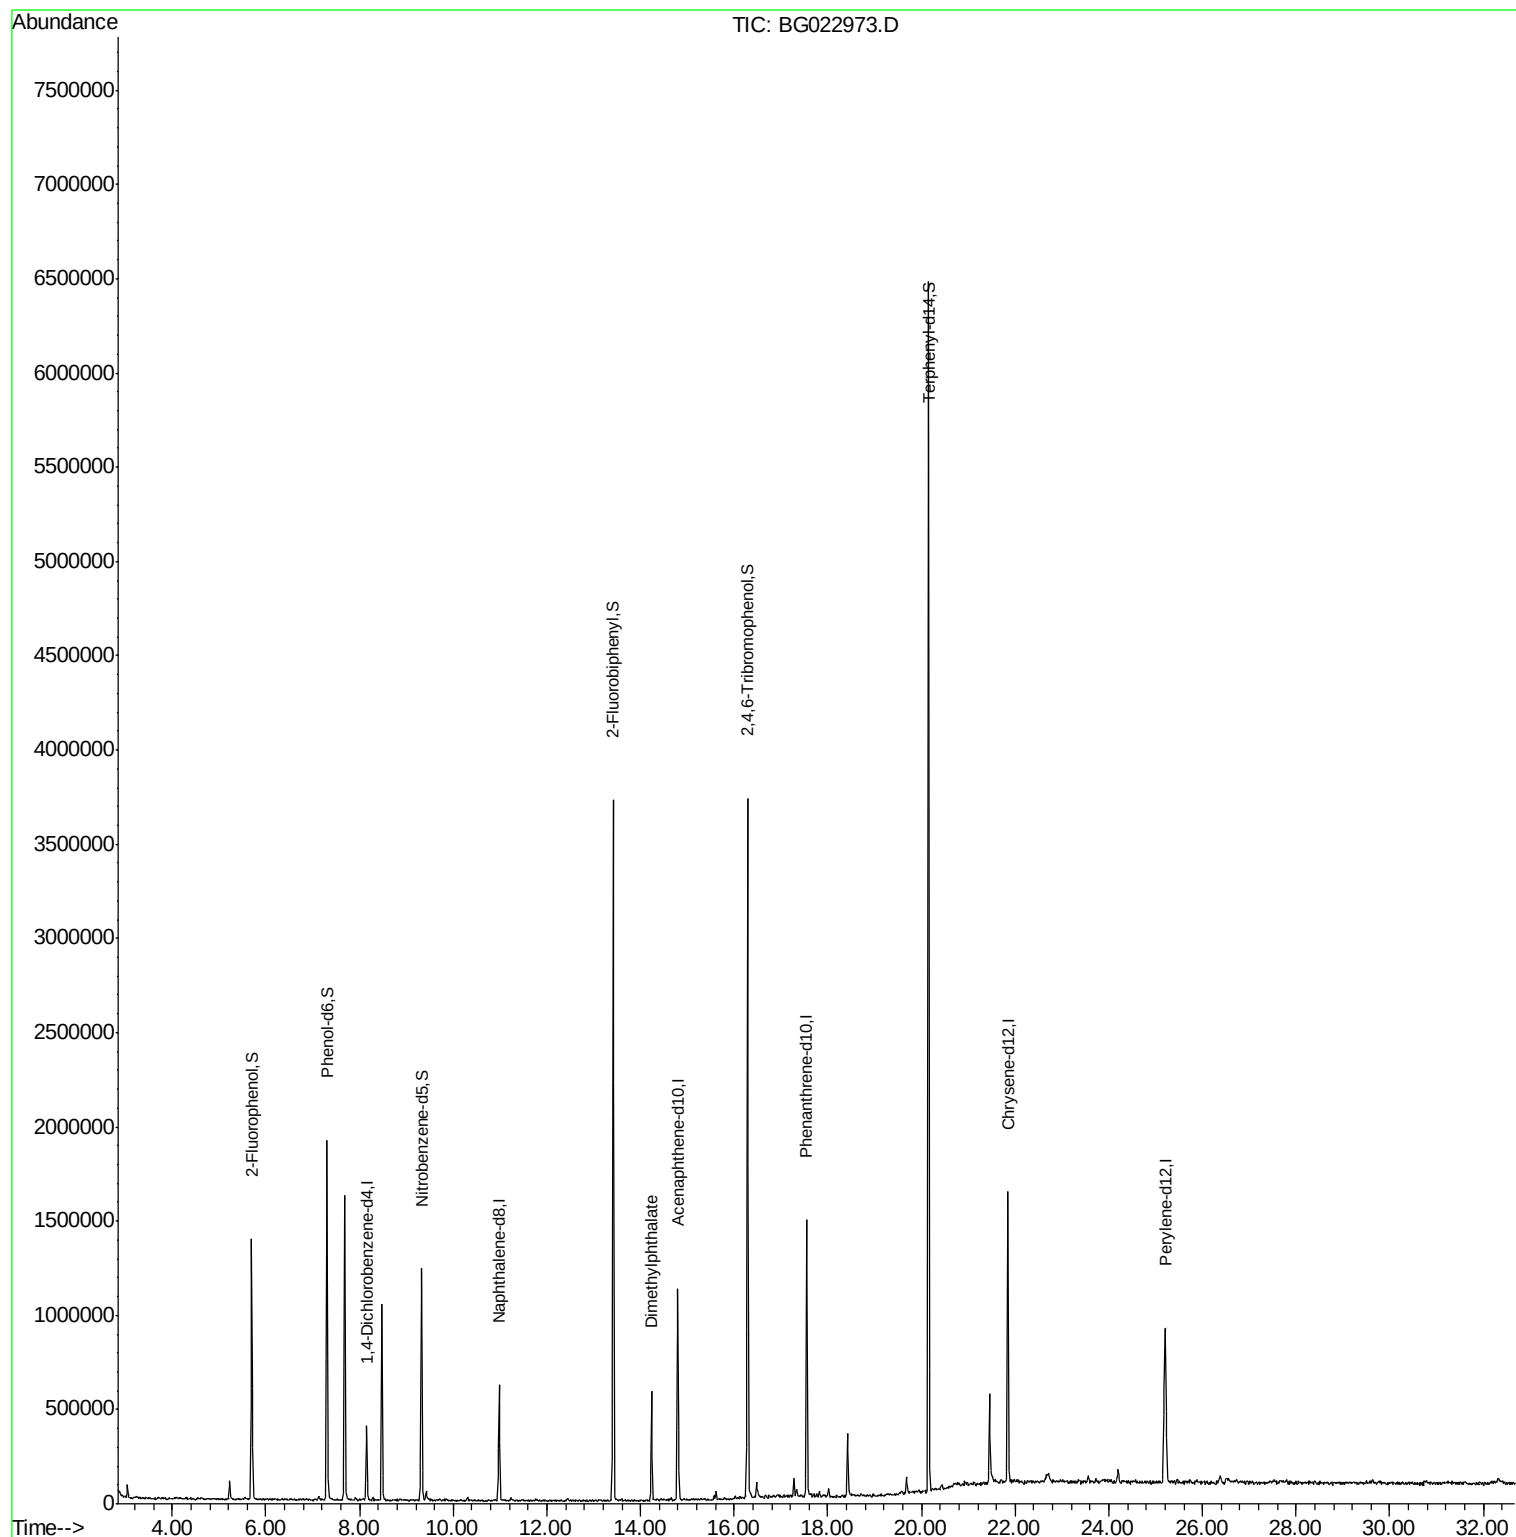

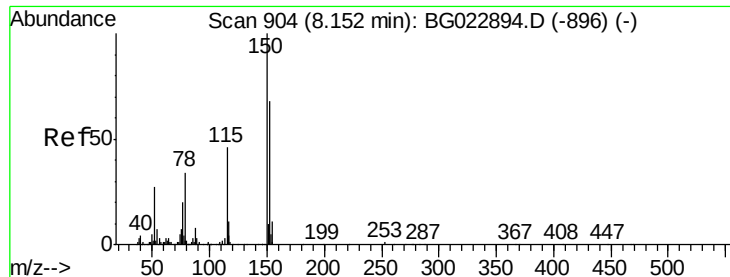

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.15 min Scan# 905

Delta R.T. 0.00 min

Lab File: BG022973.D

Acq: 9 Jul 2016 20:08

Instrument :

BNA_G

ClientSampleId :

SS-5


Tgt Ion:152 Resp: 105788

Ion Ratio Lower Upper

152 100

150 147.3 144.7 217.1




115 60.2 64.0 96.0#

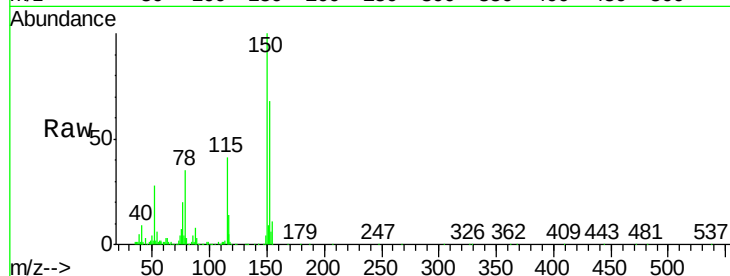

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

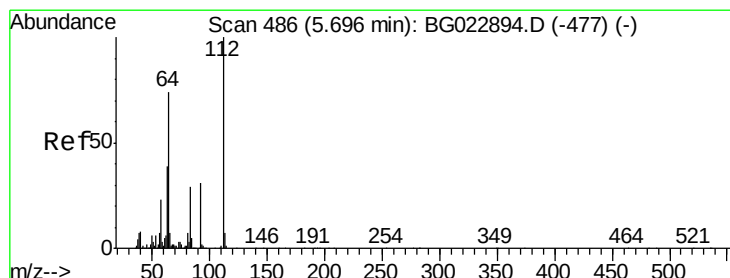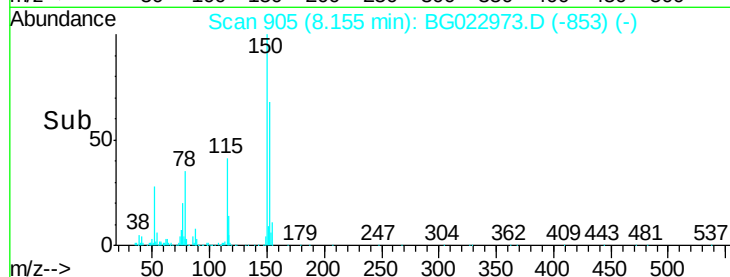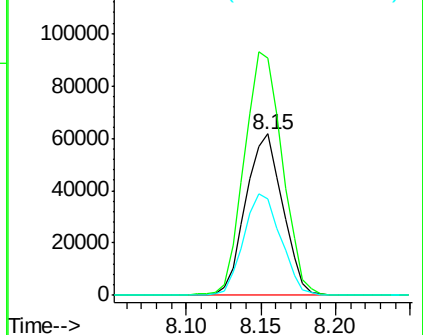

#5

2-Fluorophenol

Concen: 87.52 ng

RT: 5.70 min Scan# 487

Delta R.T. 0.00 min

Lab File: BG022973.D

Acq: 9 Jul 2016 20:08


Tgt Ion:112 Resp: 566107

Ion Ratio Lower Upper

112 100

64 67.5 59.0 88.4



63 41.1 37.8 56.8

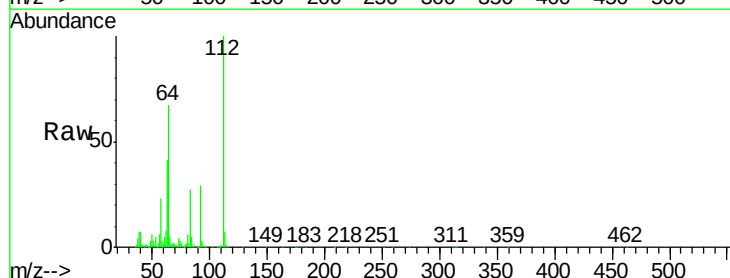


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG0

Ion 63.00 (62.70 to 63.70): BG0

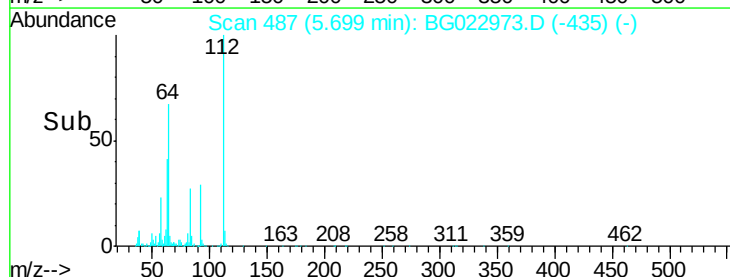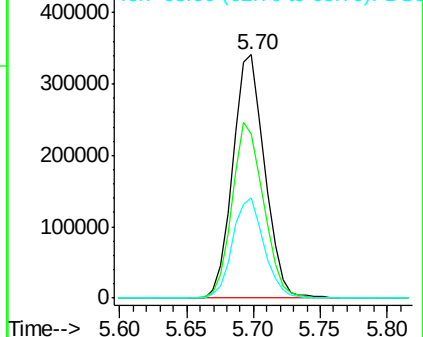

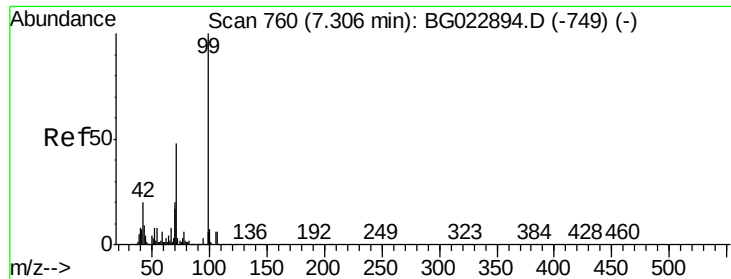

#7

Phenol-d6

Concen: 105.91 ng

RT: 7.30 min Scan# 760

Delta R.T. -0.00 min

Lab File: BG022973.D

Acq: 9 Jul 2016 20:08

Instrument :

BNA_G

ClientSampleId :

SS-5


Tgt Ion: 99 Resp: 1072968

Ion Ratio Lower Upper




99 100

42 20.3 17.8 26.6

71 48.1 41.5 62.3

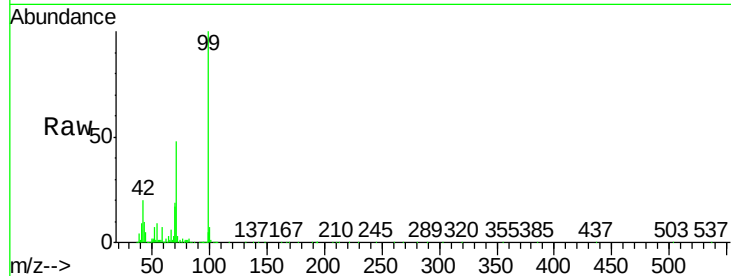

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

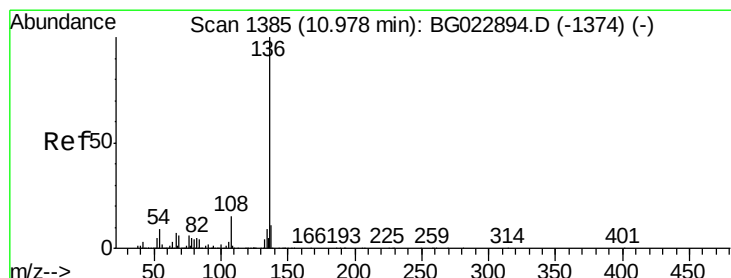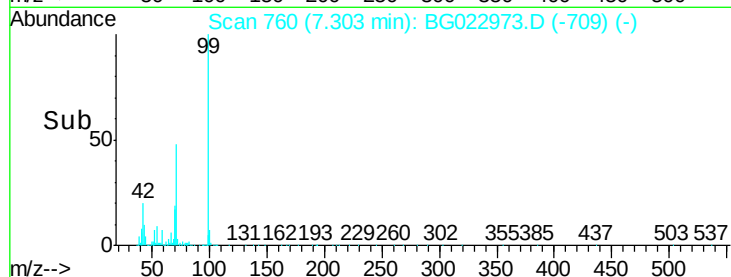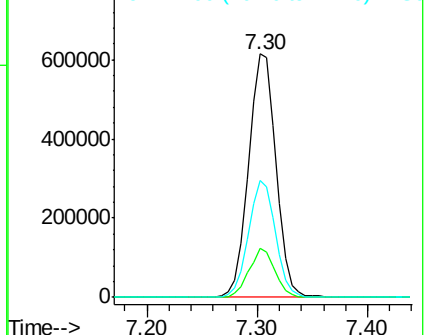

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.98 min Scan# 1386

Delta R.T. 0.00 min

Lab File: BG022973.D

Acq: 9 Jul 2016 20:08

Tgt Ion: 136 Resp: 487025


Ion Ratio Lower Upper

136 100



137 10.3 9.6 14.4


54 8.4 7.3 10.9

68 6.1 5.3 7.9

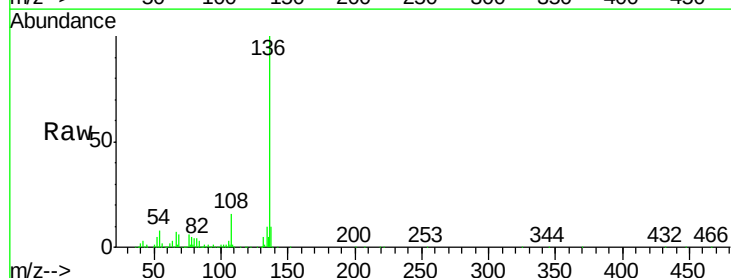

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



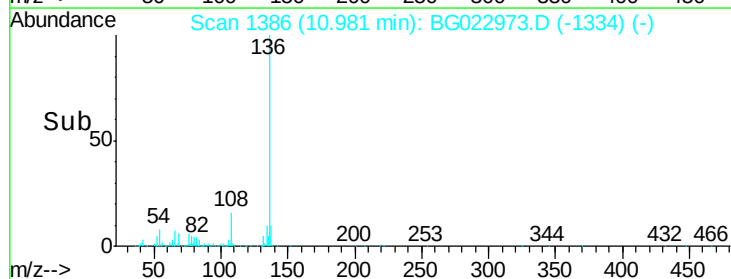
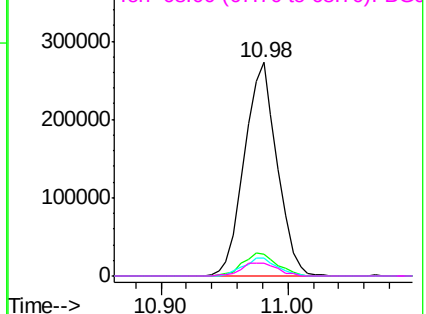


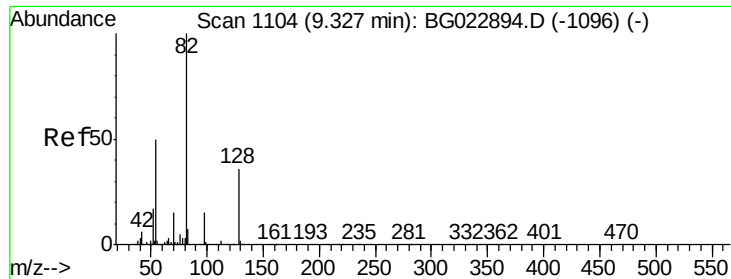

#23
 Nitrobenzene-d5
 Concen: 69.26 ng
 RT: 9.32 min Scan# 1104
 Delta R.T. -0.00 min
 Lab File: BG022973.D
 Acq: 9 Jul 2016 20:08




Instrument :
 BNA_G
 ClientSampled :
 SS-5


Tgt Ion	Ratio	Lower	Upper
82	100		
128	33.3	24.4	36.6
54	49.3	41.4	62.0

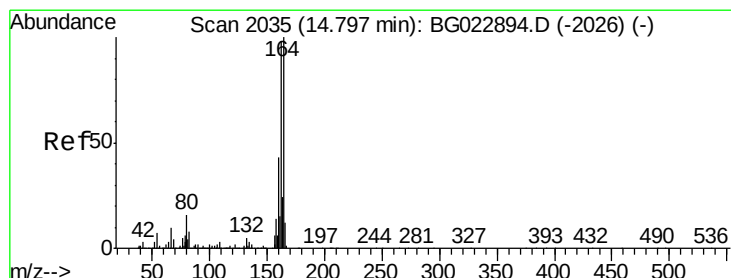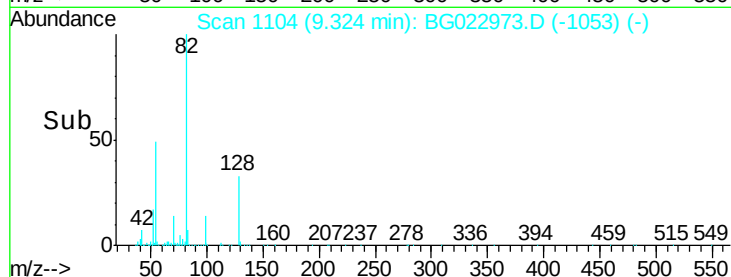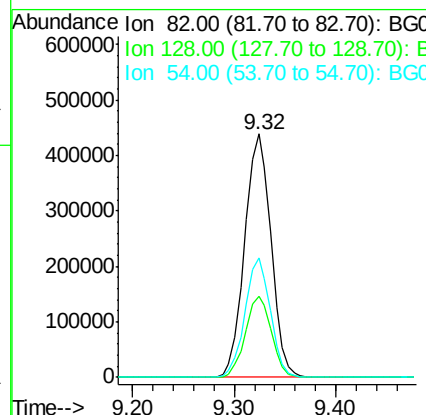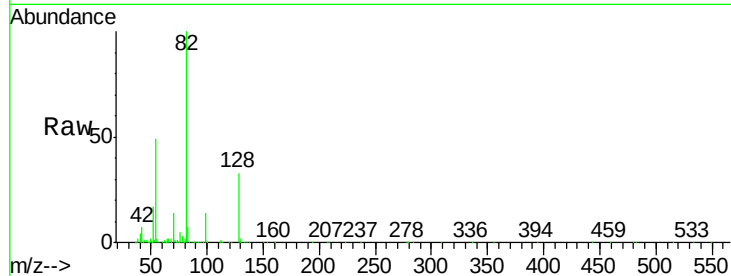

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.79 min Scan# 2035
 Delta R.T. -0.00 min
 Lab File: BG022973.D
 Acq: 9 Jul 2016 20:08

Tgt Ion	Ratio	Lower	Upper
164	100		
162	105.2	87.7	131.5
160	43.8	37.2	55.8

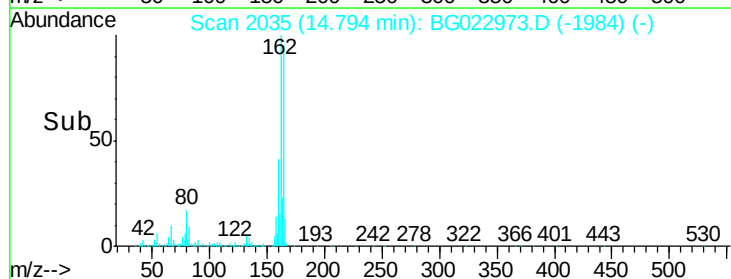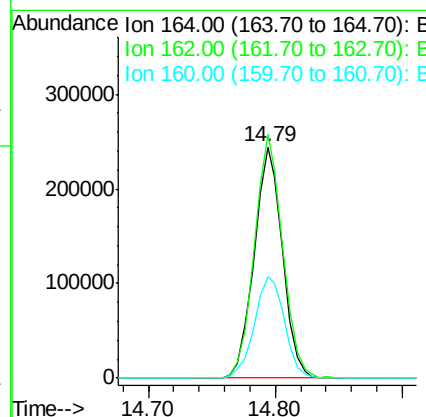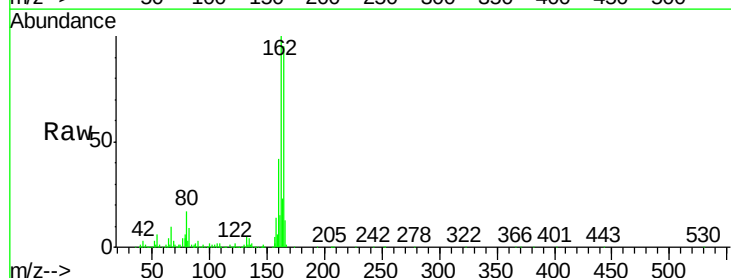


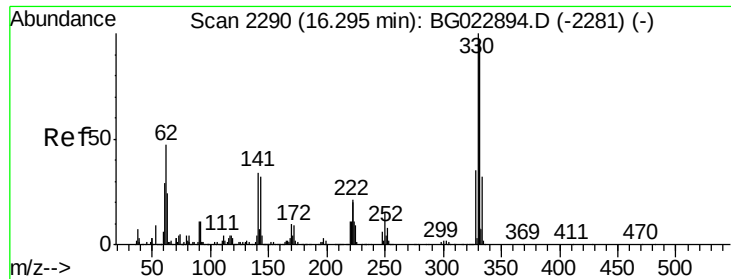




#41
 2,4,6-Tribromophenol
 Concen: 99.86 ng
 RT: 16.29 min Scan# 2289
 Delta R.T. -0.01 min
 Lab File: BG022973.D
 Acq: 9 Jul 2016 20:08

Instrument :
 BNA_G
 ClientSampleId :
 SS-5

Tgt Ion:330 Resp: 679544
 Ion Ratio Lower Upper
 330 100
 332 97.4 77.4 116.2
 141 37.6 31.7 47.5

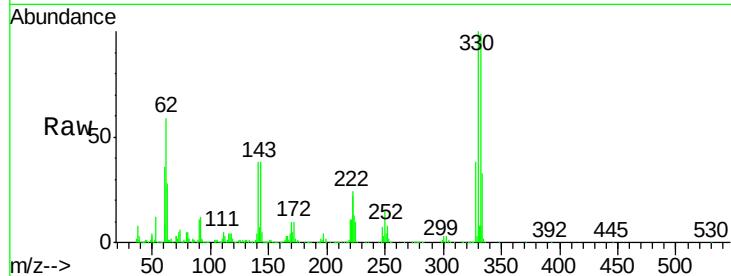


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

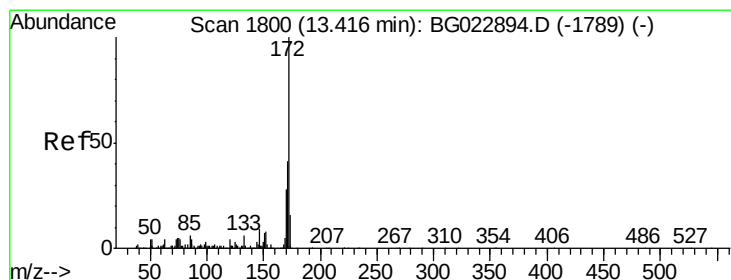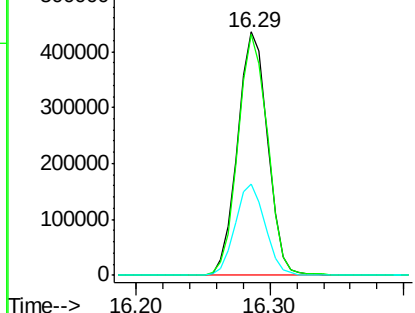
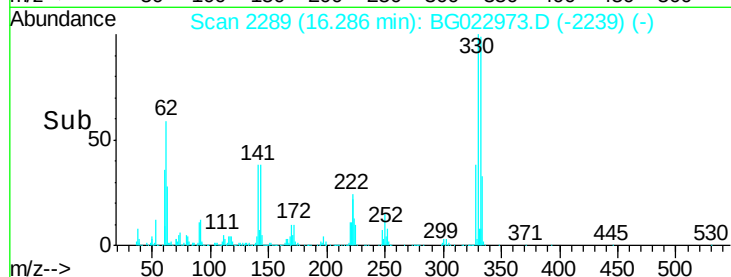



#44
 2-Fluorobiphenyl
 Concen: 73.82 ng
 RT: 13.41 min Scan# 1800
 Delta R.T. -0.00 min
 Lab File: BG022973.D
 Acq: 9 Jul 2016 20:08

Tgt Ion:172 Resp: 1774639
 Ion Ratio Lower Upper
 172 100
 171 39.3 31.6 47.4
 170 27.2 21.3 31.9

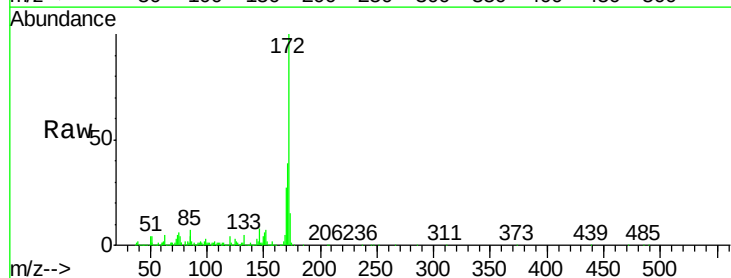

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



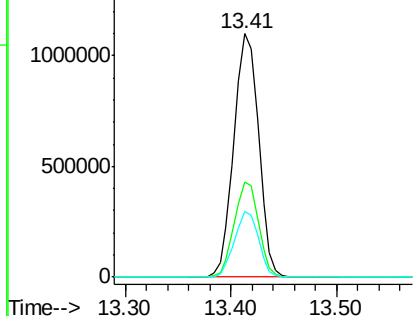
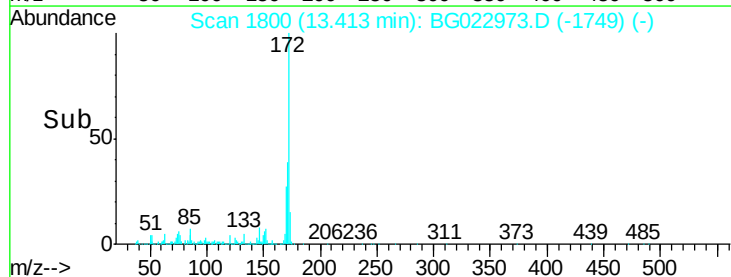


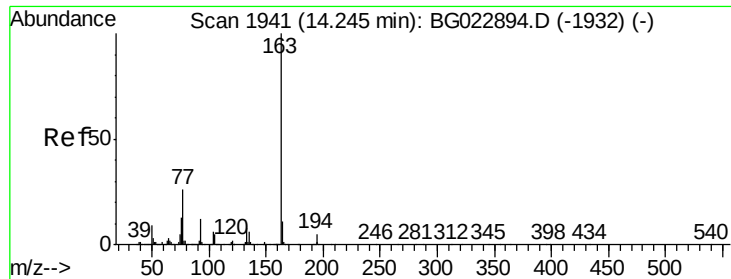

#49
Dimethylphthalate
Concen: 11.51 ng
RT: 14.24 min Scan# 1940
Delta R.T. -0.01 min
Lab File: BG022973.D
Acq: 9 Jul 2016 20:08




Instrument :
BNA_G
ClientSampleId :
SS-5


Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.6	5.4
164	10.8	8.1	12.1

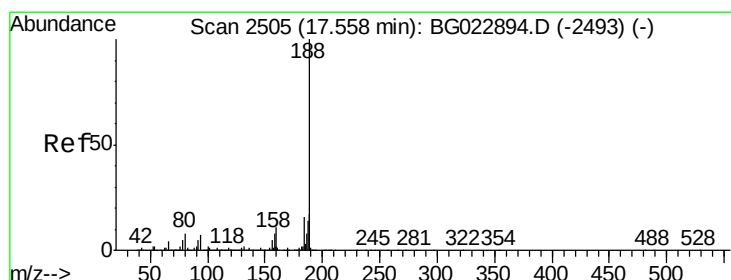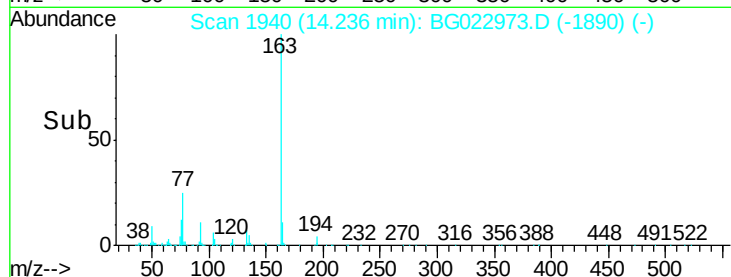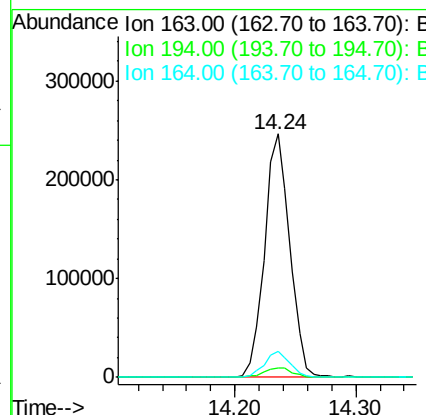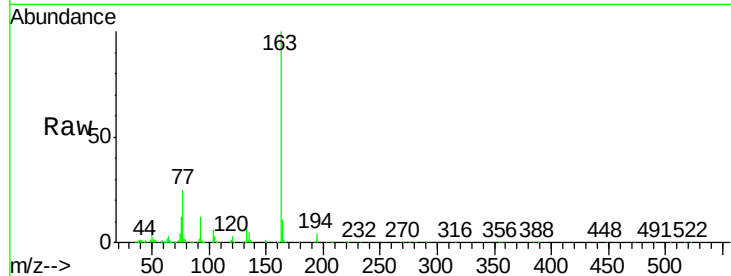

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.55 min Scan# 2504
Delta R.T. -0.01 min
Lab File: BG022973.D
Acq: 9 Jul 2016 20:08

Tgt Ion	Ratio	Lower	Upper
188	100		
94	7.0	5.2	7.8
80	8.7	7.2	10.8


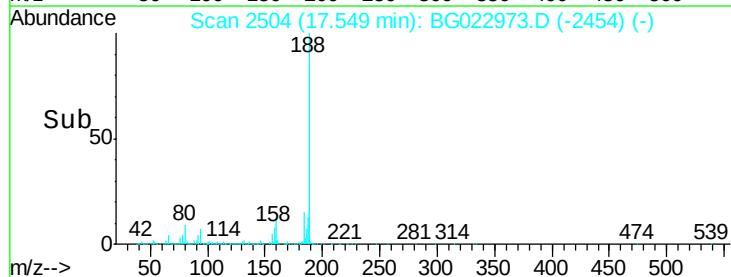
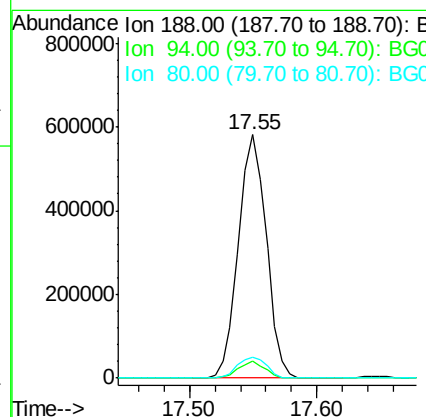
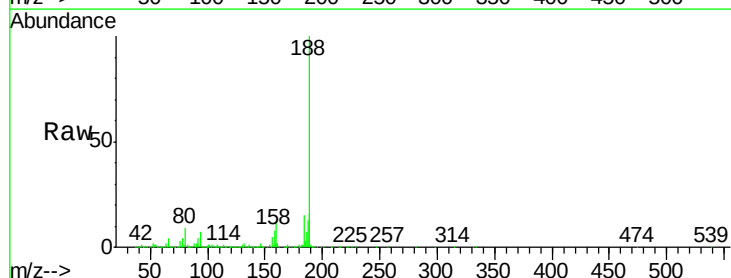


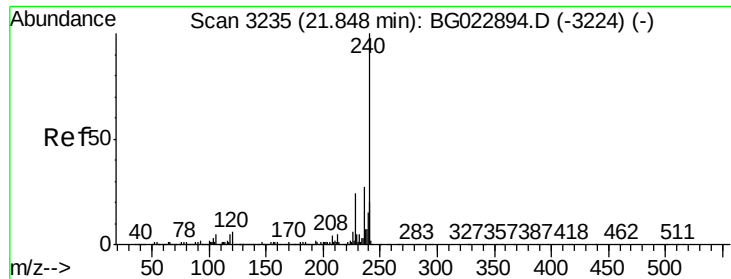

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 21.84 min Scan# 3235
 Delta R.T. -0.00 min
 Lab File: BG022973.D
 Acq: 9 Jul 2016 20:08




Instrument :
 BNA_G
 ClientSampleId :
 SS-5


Tgt Ion:240 Resp: 962043
 Ion Ratio Lower Upper
 240 100
 120 5.9 4.1 6.1
 236 28.7 21.1 31.7

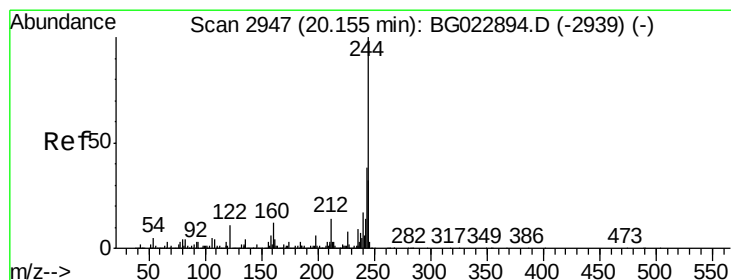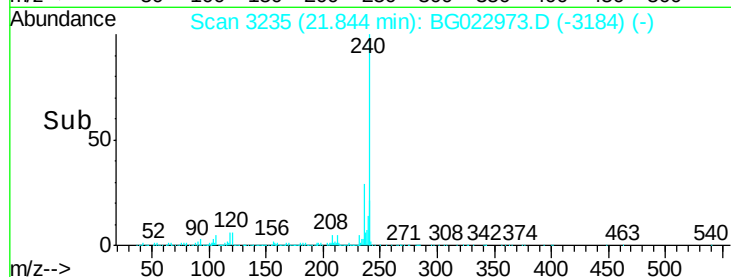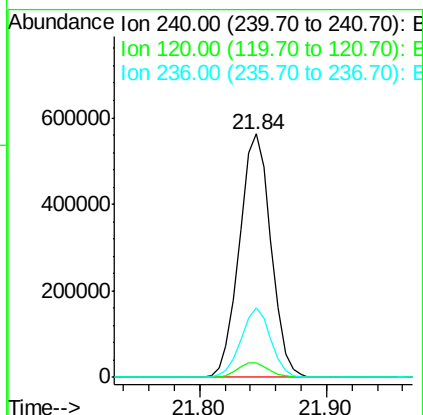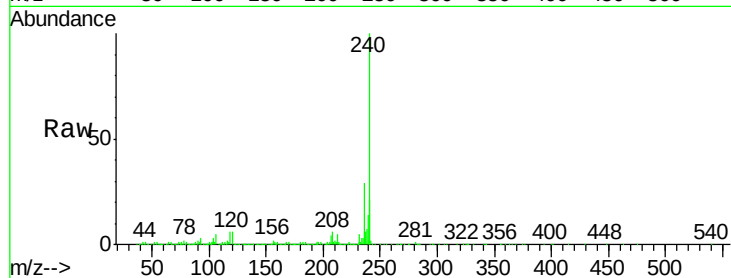

#78
 Terphenyl-d14
 Concen: 80.49 ng
 RT: 20.15 min Scan# 2947
 Delta R.T. -0.00 min
 Lab File: BG022973.D
 Acq: 9 Jul 2016 20:08

Tgt Ion:244 Resp: 2491096
 Ion Ratio Lower Upper
 244 100
 212 12.4 10.8 16.2
 122 9.7 8.0 12.0

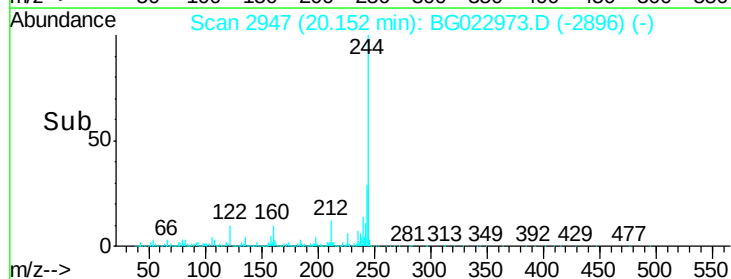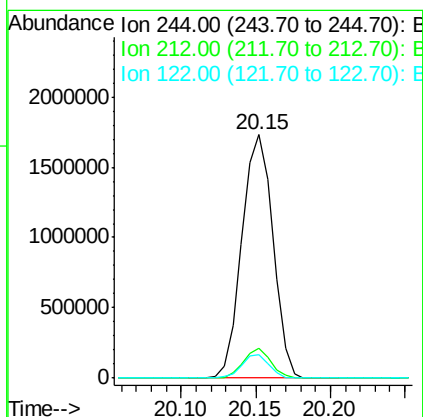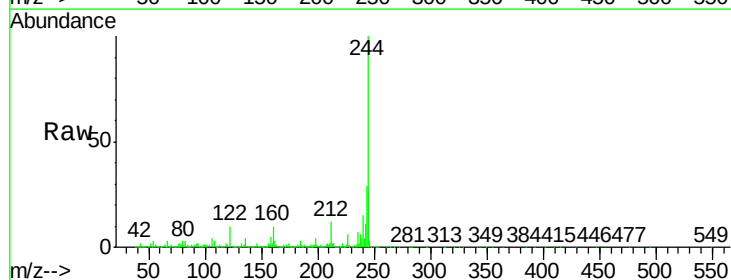

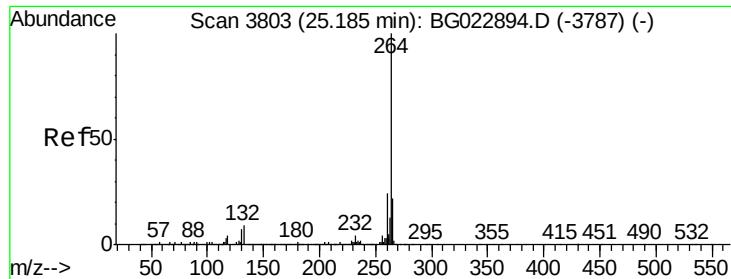

#86
Perylene-d12
Concen: 20.00 ng
RT: 25.21 min Scan# 3807
Delta R.T. 0.02 min
Lab File: BG022973.D
Acq: 9 Jul 2016 20:08

Instrument :
BNA_G
ClientSampleId :
SS-5

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.7	18.4	27.6
265	23.2	18.9	28.3

