
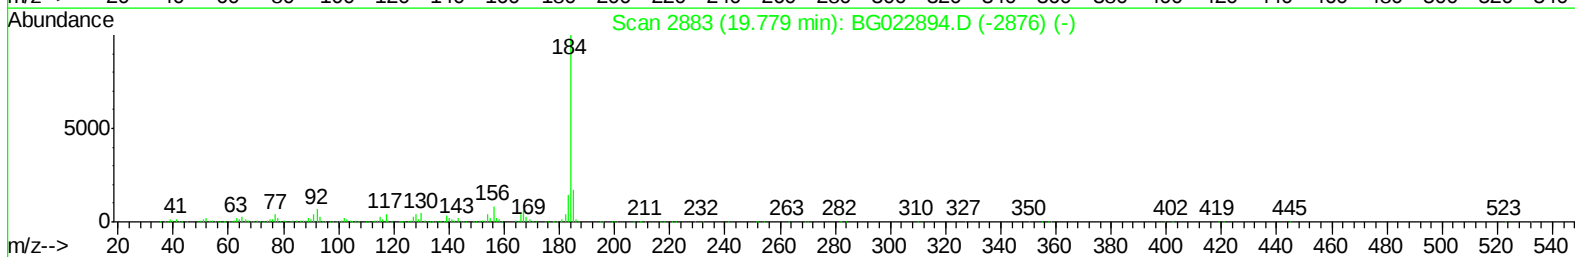
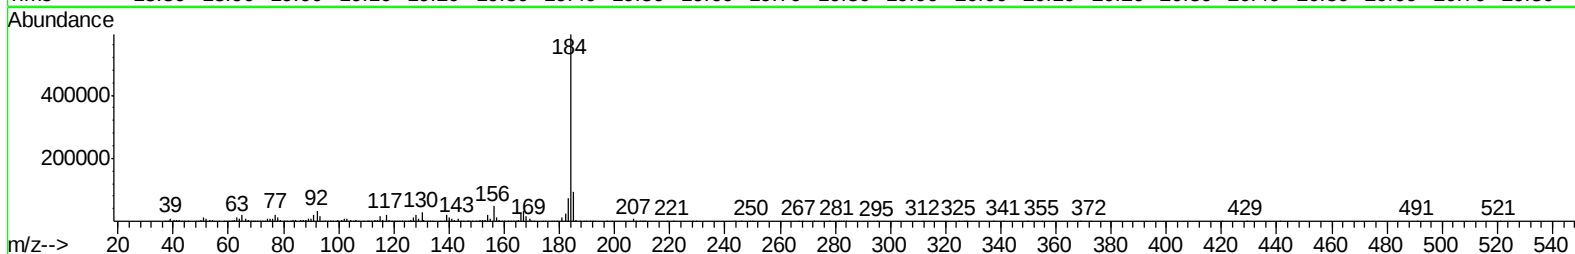


Data Path : Z:\HPCHEM1\BNA_G\Data\BG071016\
Data File : BG022966.D
Acq On : 9 Jul 2016 15:28
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 08:24:42 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 16:51:07 2016
Response via : Initial Calibration

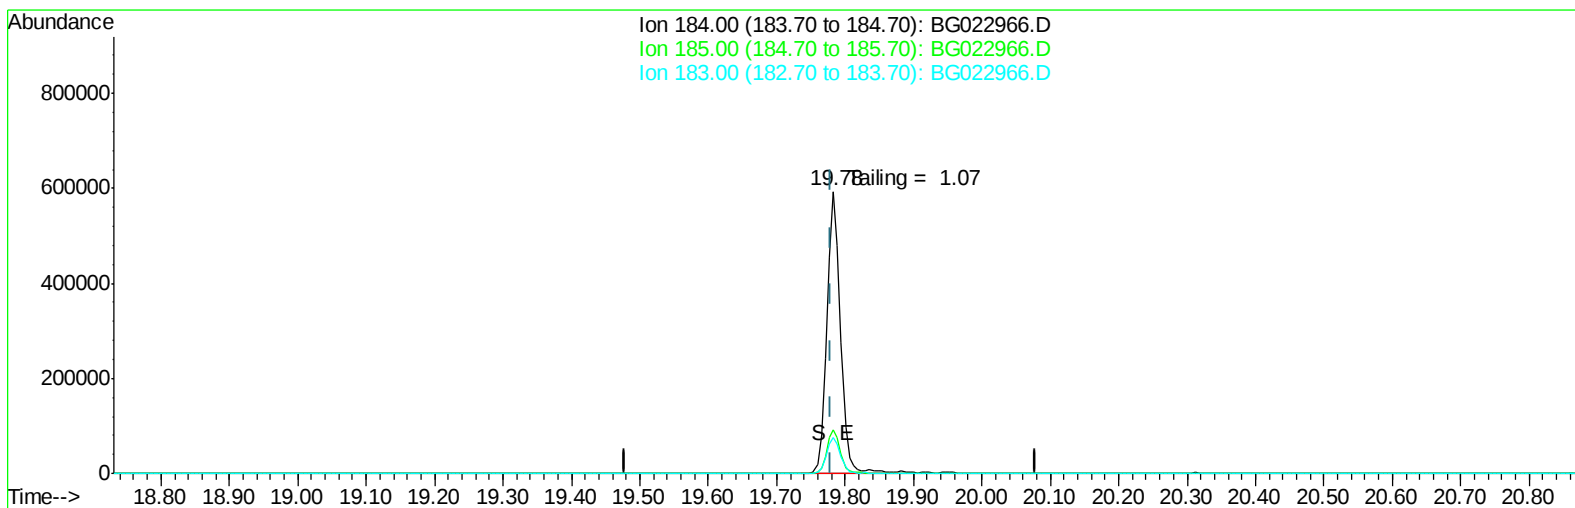

TIC: BG022966.D

(76) Benzidine




19.783min (+0.003) 488065.29ng

response 825537

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.46
183.00	13.40	12.66
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG071016\
Data File : BG022966.D
Acq On : 9 Jul 2016 15:28
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 08:24:42 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 16:51:07 2016
Response via : Initial Calibration

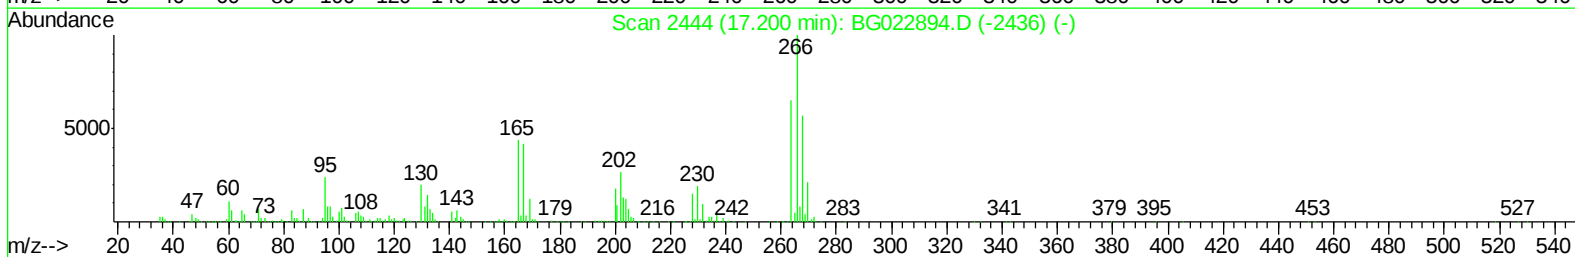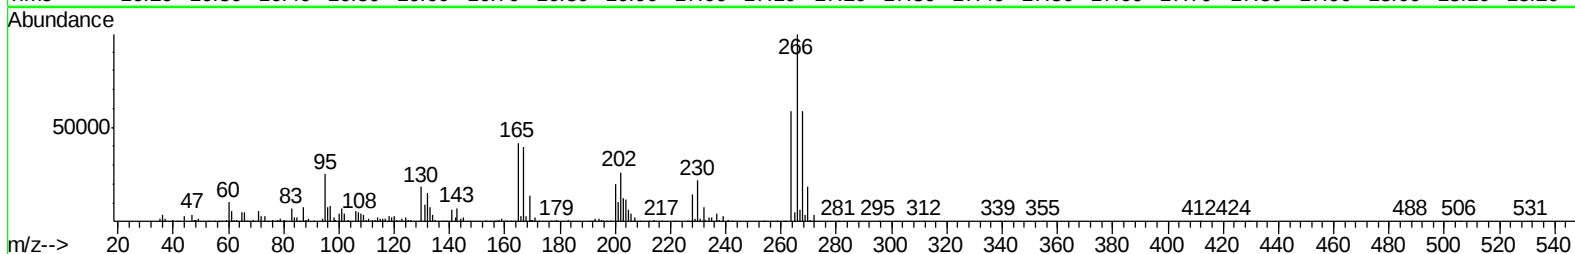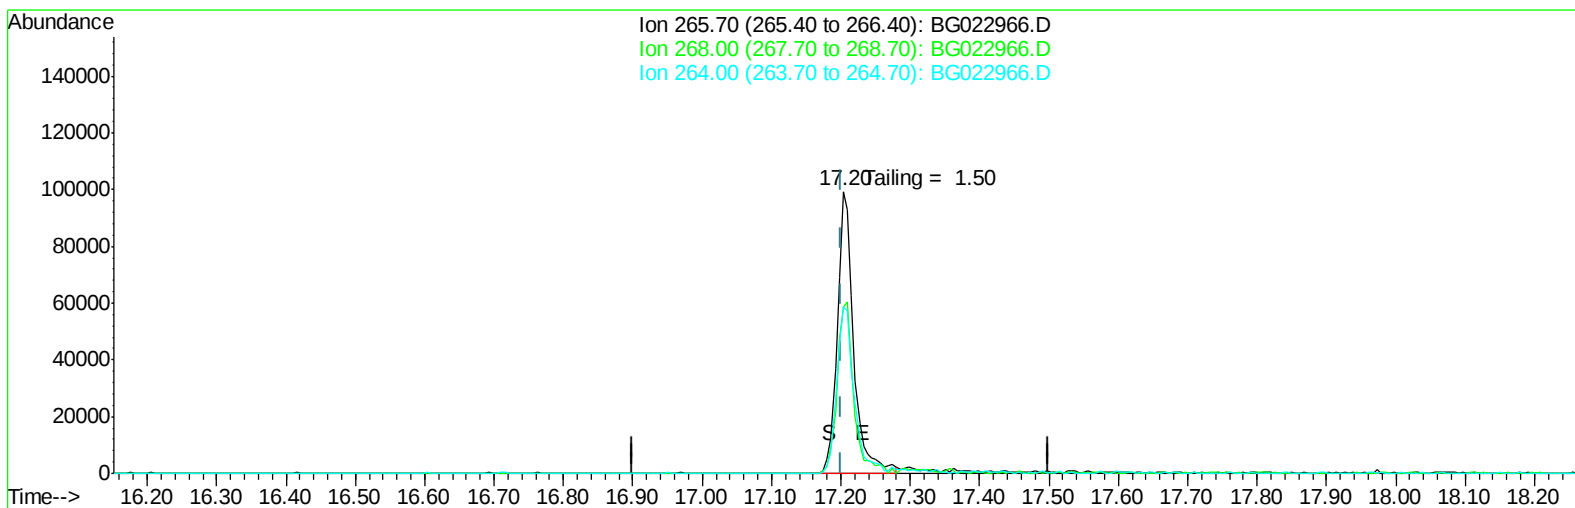

TIC: BG022966.D

(69) Pentachlorophenol (C)

17.204min (+0.003) 281670.27ng

response 162563

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	59.20
264.00	63.20	59.05
0.00	0.00	0.00