
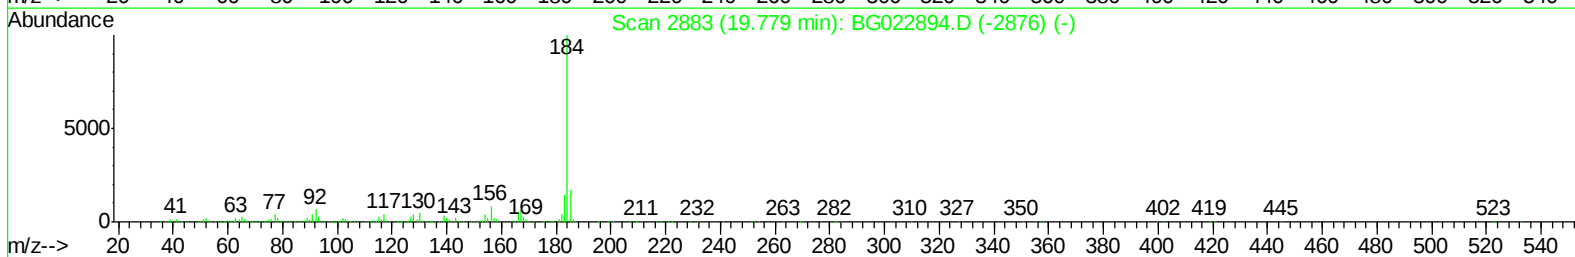
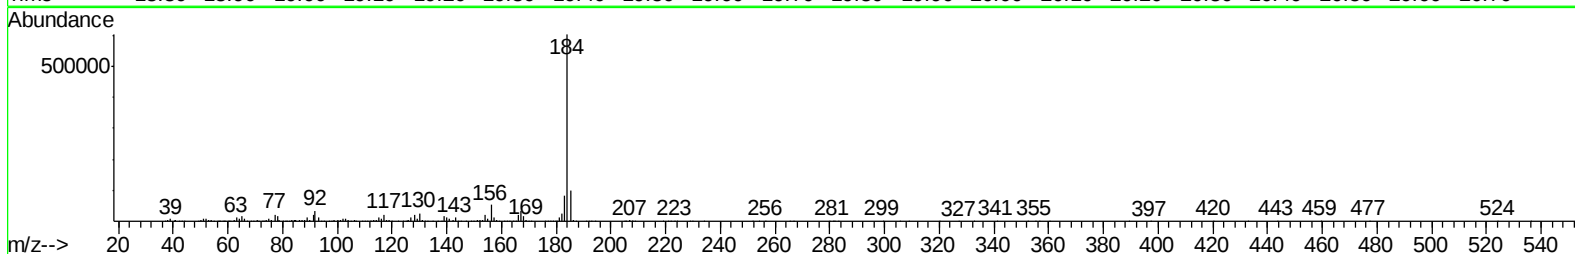


Data Path : Z:\HPCHEM1\BNA_G\Data\BG071016\
Data File : BG022982.D
Acq On : 10 Jul 2016 2:49
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 08:25:36 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 16:51:07 2016
Response via : Initial Calibration

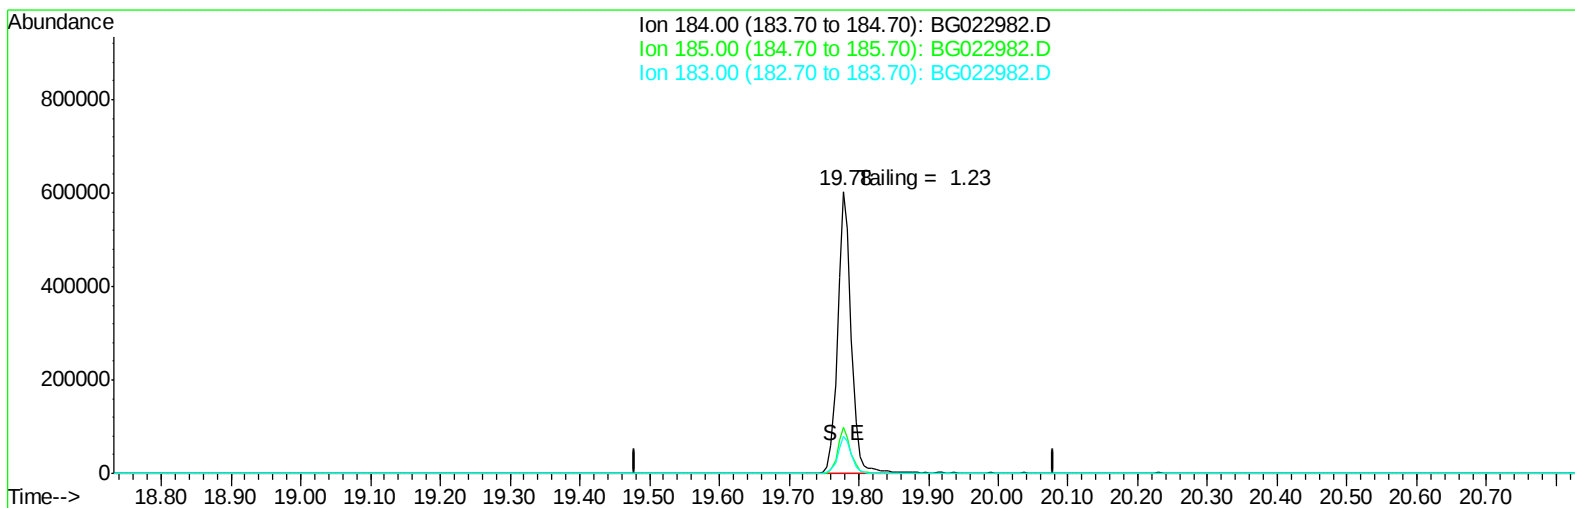

TIC: BG022982.D

(76) Benzidine




19.779min (-19.779) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	15.80	0.00#
183.00	13.40	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG071016\
Data File : BG022982.D
Acq On : 10 Jul 2016 2:49
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 08:25:36 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 16:51:07 2016
Response via : Initial Calibration

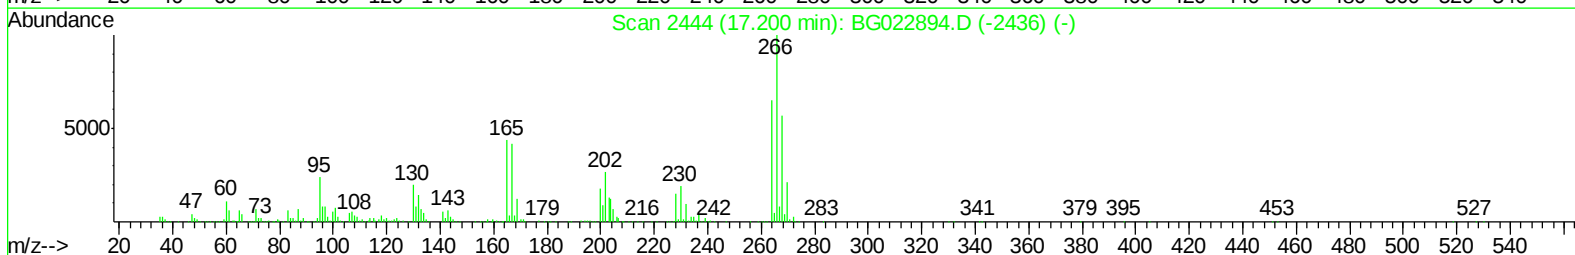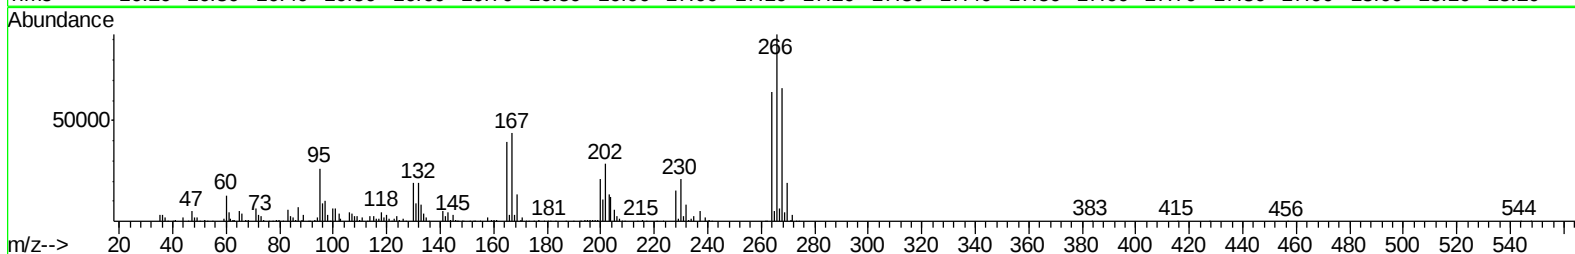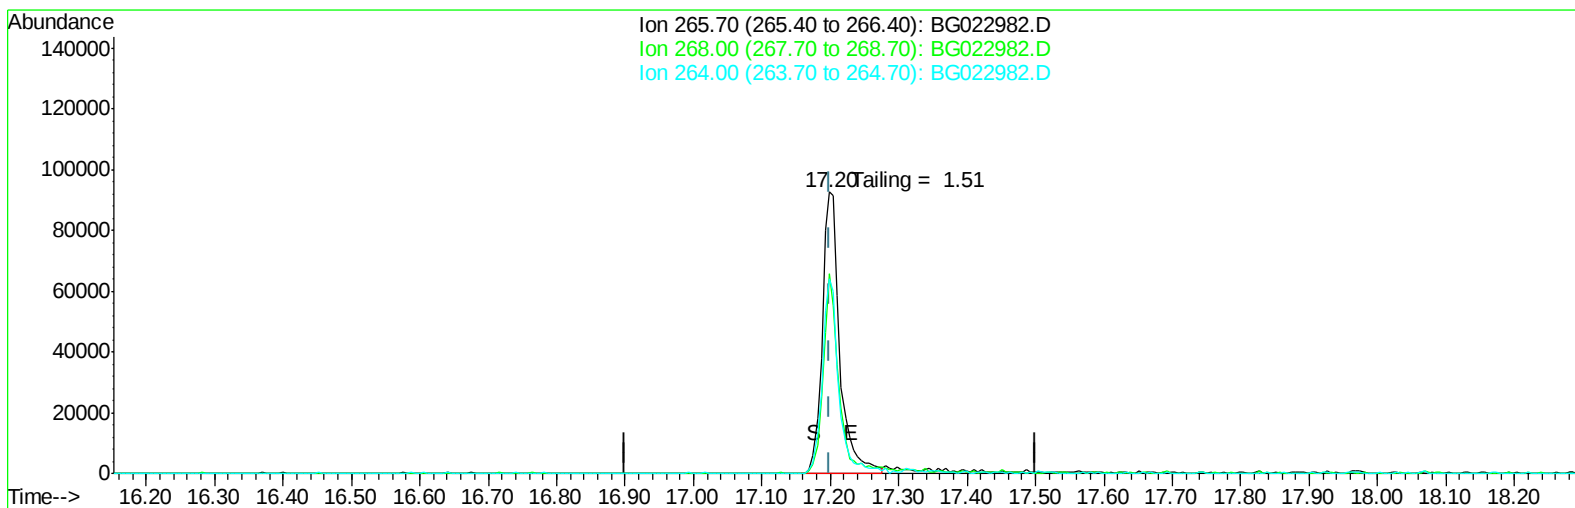

TIC: BG022982.D

(69) Pentachlorophenol (C)

17.198min (-0.002) 137484.12ng

response 158695

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	71.12
264.00	63.20	68.99
0.00	0.00	0.00