


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071016\
 Data File : BG022966.D
 Acq On : 9 Jul 2016 15:28
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 07 16:51:07 2016

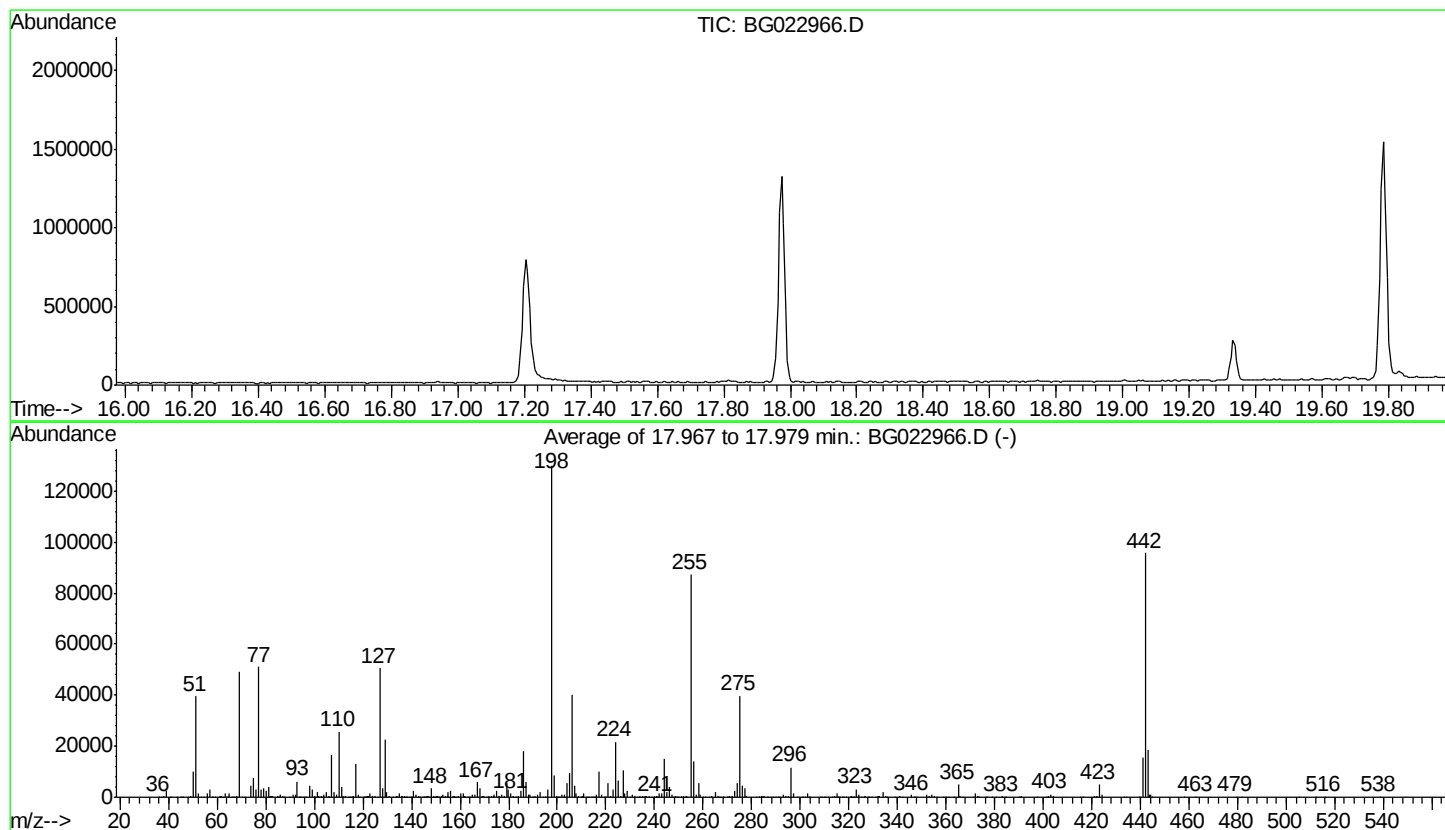

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	39528	PASS
68	69	0.00	2	0.7	354	PASS
69	198	0.00	100	38.0	49331	PASS
70	69	0.00	2	0.2	105	PASS
127	198	10	80	38.8	50488	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	129962	PASS
199	198	5	9	6.6	8526	PASS
275	198	10	60	30.6	39706	PASS
365	198	1	100	3.8	4925	PASS
441	442	0.01	24	16.4	15676	PASS
442	198	50	100	73.6	95701	PASS
443	442	15	24	19.2	18338	PASS