


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071016\
 Data File : BG022982.D
 Acq On : 10 Jul 2016 2:49
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 07 16:51:07 2016

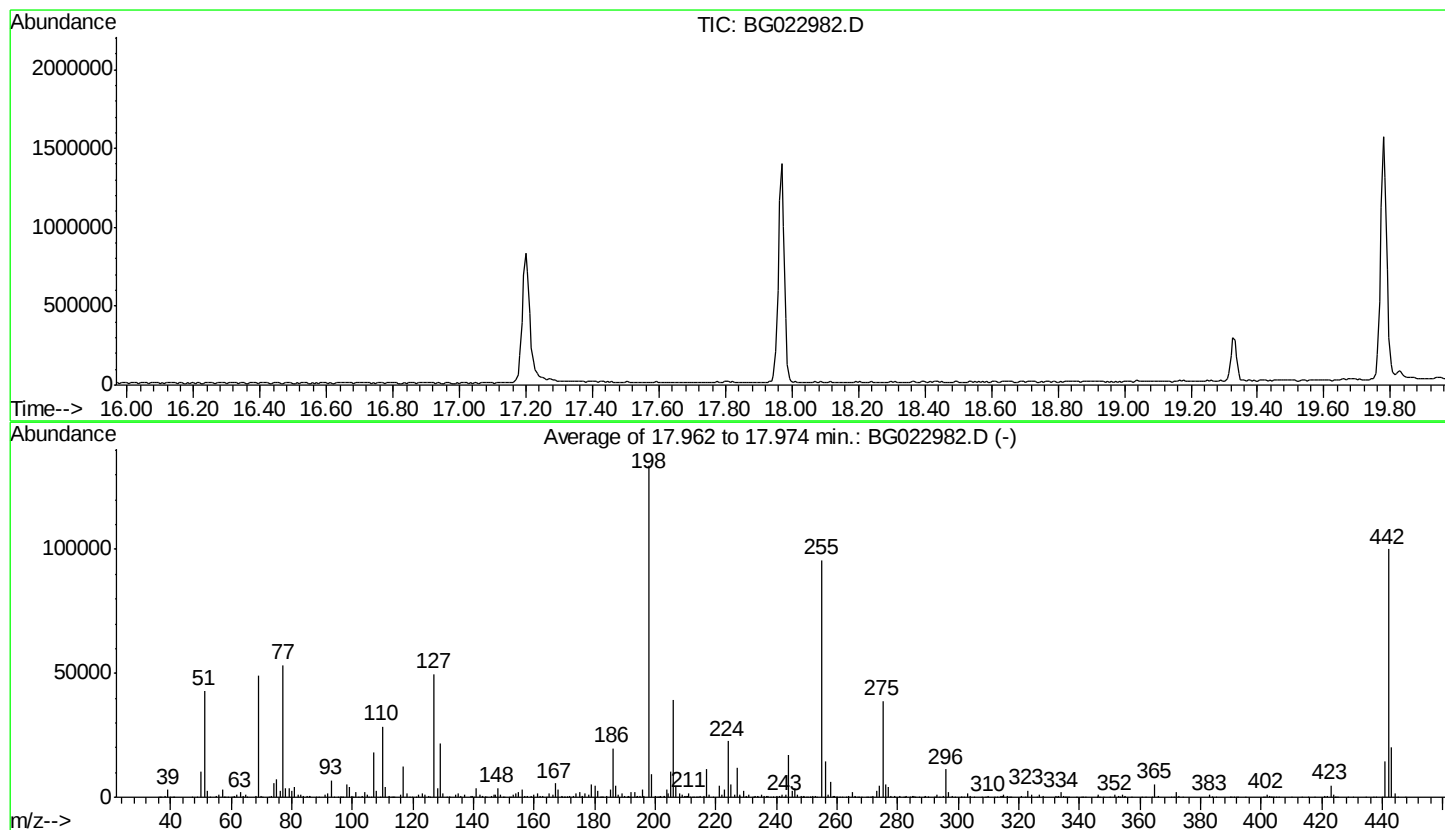

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.1	42962	PASS
68	69	0.00	2	0.6	311	PASS
69	198	0.00	100	36.8	49305	PASS
70	69	0.00	2	0.8	371	PASS
127	198	10	80	37.2	49829	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	133808	PASS
199	198	5	9	7.0	9311	PASS
275	198	10	60	29.0	38794	PASS
365	198	1	100	4.0	5317	PASS
441	442	0.01	24	14.3	14296	PASS
442	198	50	100	74.9	100165	PASS
443	442	15	24	20.1	20156	PASS