

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071017\
 Data File : BG027916.D
 Acq On : 11 Jul 2017 17:09
 Operator : SJ/JU
 Sample : I4132-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CLINTON-AVE-69KV-COMP-(DRUM)

Quant Time: Jul 11 18:03:21 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 11 15:32:18 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.42	152	44034	20.00	ng	0.00
21) Naphthalene-d8	11.23	136	184218	20.00	ng	-0.01
38) Acenaphthene-d10	15.01	164	98684	20.00	ng	-0.01
63) Phenanthrene-d10	17.76	188	231792	20.00	ng	-0.01
75) Chrysene-d12	22.10	240	292494	20.00	ng	-0.02
86) Perylene-d12	25.67	264	282202	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	6.00	112	398256	139.27	ng	0.00
7) Phenol-d6	7.57	99	464729	106.38	ng	0.00
23) Nitrobenzene-d5	9.58	82	279722	84.64	ng	-0.01
41) 2,4,6-Tribromophenol	16.50	330	239124	176.66	ng	-0.02
44) 2-Fluorobiphenyl	13.64	172	733239	106.12	ng	-0.01
78) Terphenyl-d14	20.34	244	1274955	102.19	ng	-0.01
Target Compounds						
76) Benzidine	19.94	184	250	3.251	ng	Qvalue # 64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071017\
Data File : BG027916.D
Acq On : 11 Jul 2017 17:09
Operator : SJ/JU
Sample : I4132-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CLINTON-AVE-69KV-COMP-(DRUM

Quant Time: Jul 11 18:03:21 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 11 15:32:18 2017
Response via : Initial Calibration




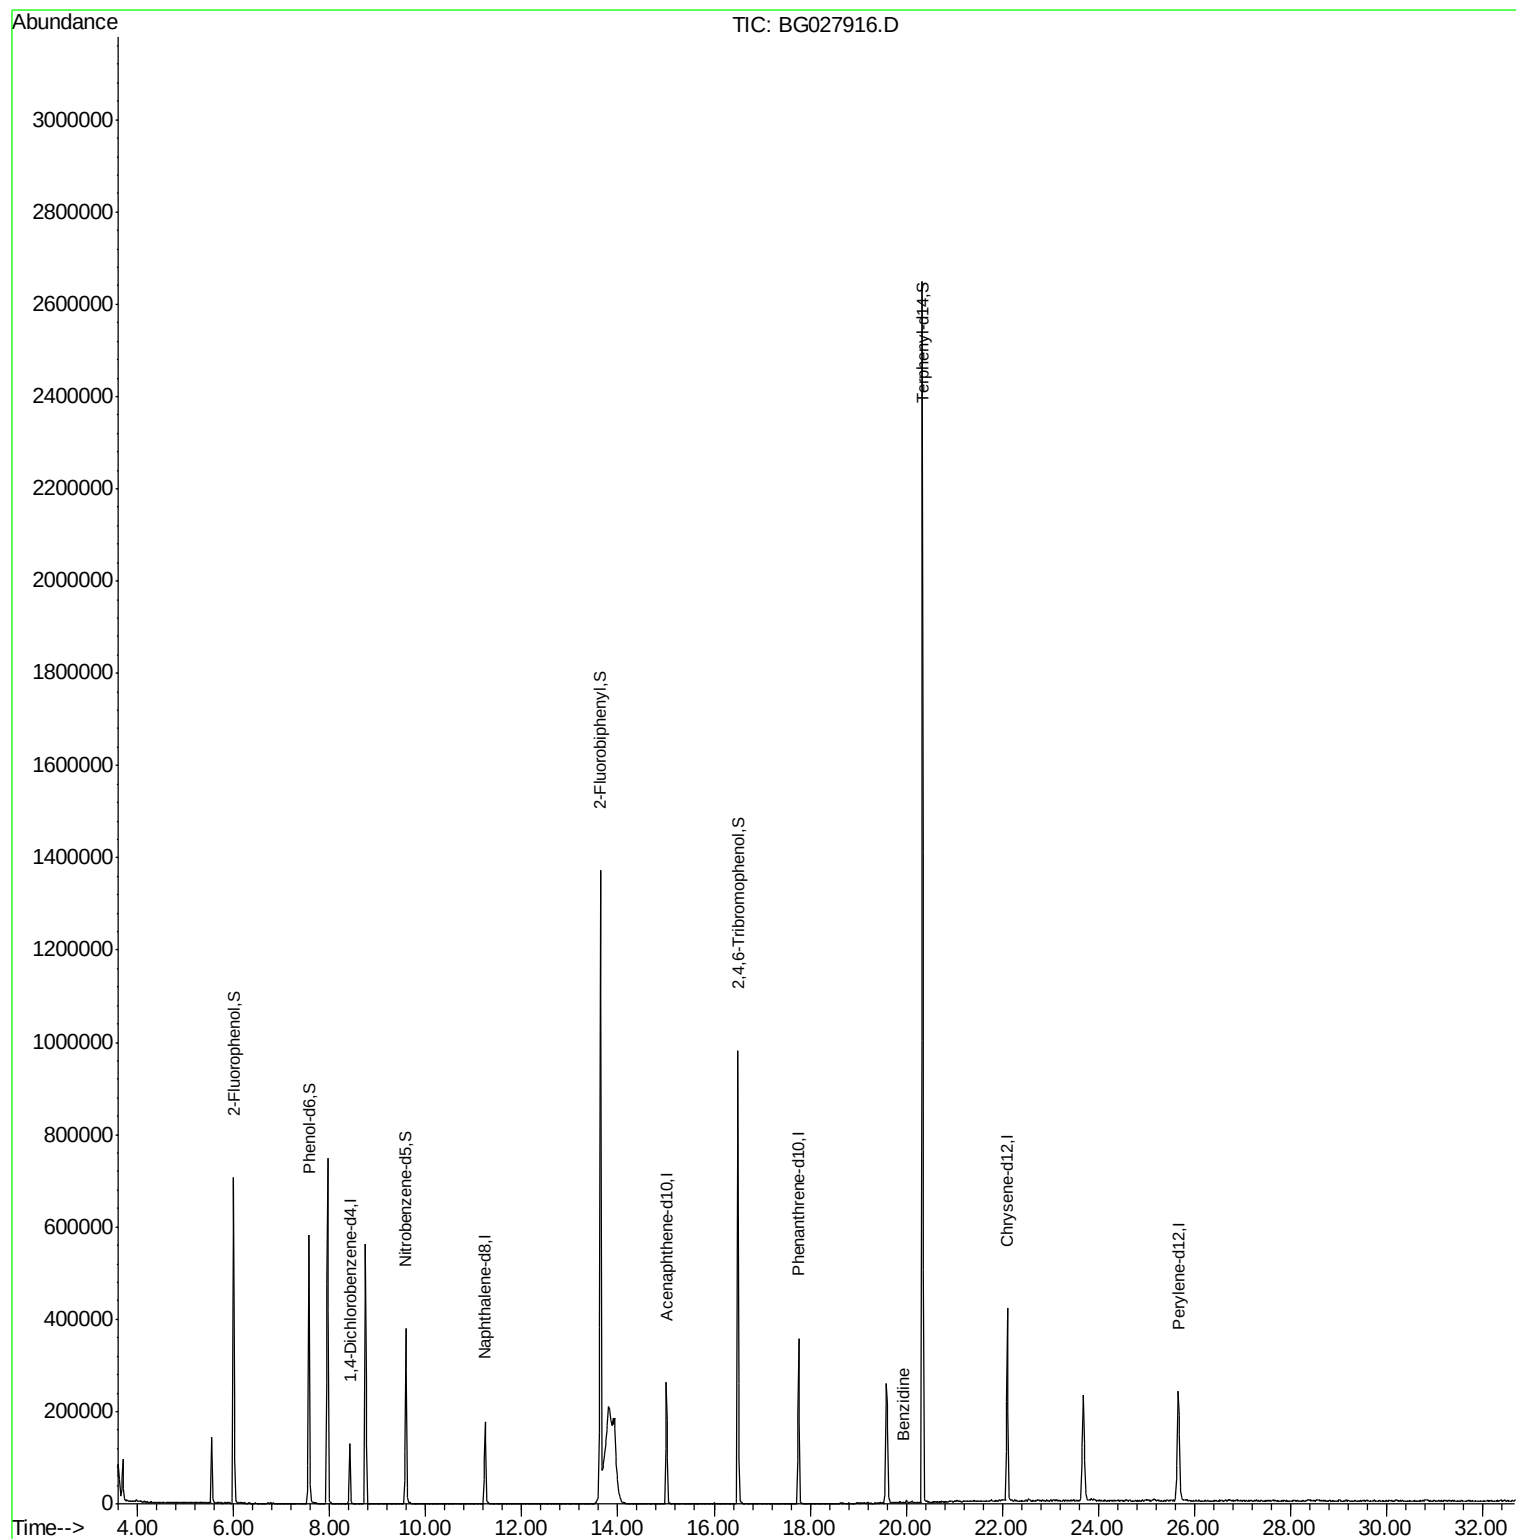


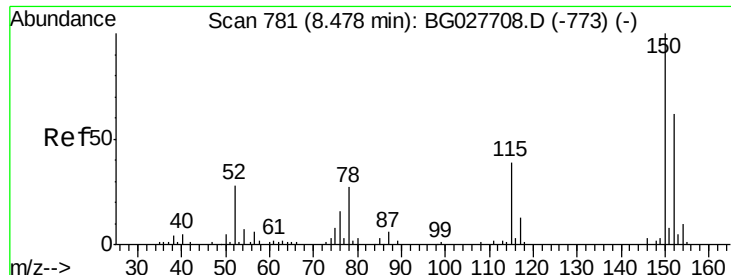

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.42 min Scan# 822
 Delta R.T. -0.01 min
 Lab File: BG027916.D
 Acq: 11 Jul 2017 17:09




Instrument :
 BNA_G
 ClientSampleId :
 CLINTON-AVE-69KV-COMP-(DRUM)


Tgt Ion:152 Resp: 44034
 Ion Ratio Lower Upper
 152 100
 150 155.4 114.0 171.0
 115 58.5 48.1 72.1

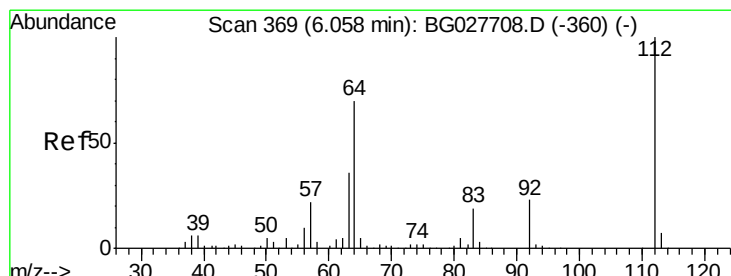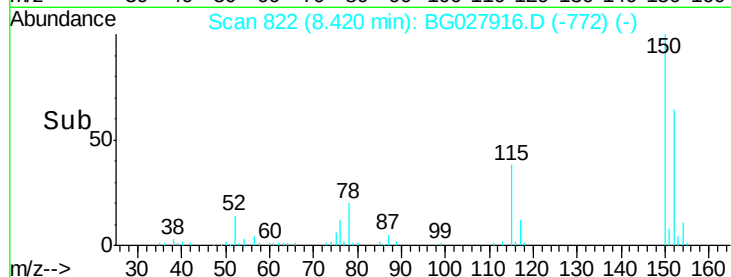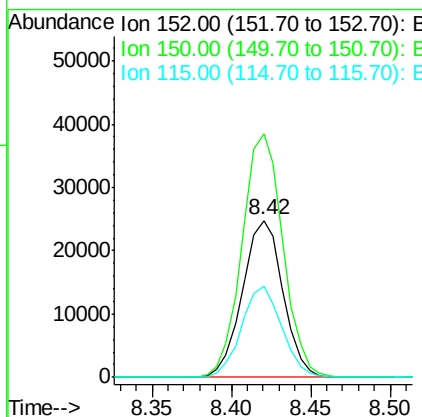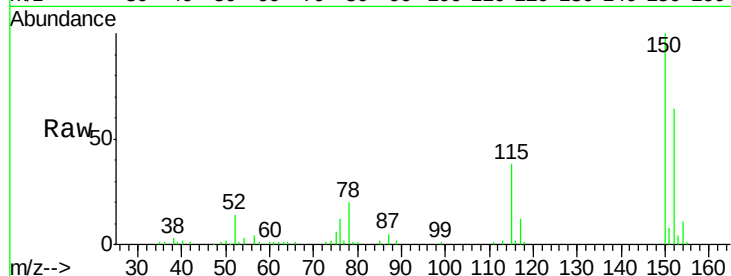

#5
 2-Fluorophenol
 Concen: 139.274 ng
 RT: 6.00 min Scan# 410
 Delta R.T. -0.01 min
 Lab File: BG027916.D
 Acq: 11 Jul 2017 17:09

Tgt Ion:112 Resp: 398256
 Ion Ratio Lower Upper
 112 100
 64 51.0 61.8 92.6#
 63 23.5 37.2 55.8#

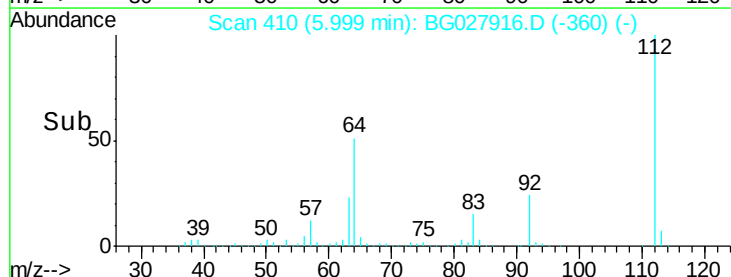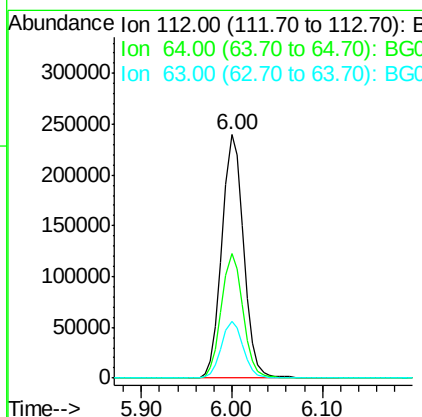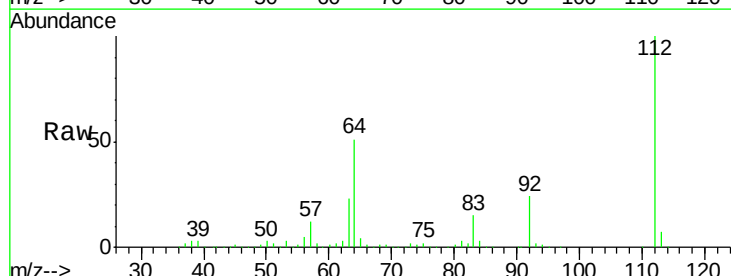

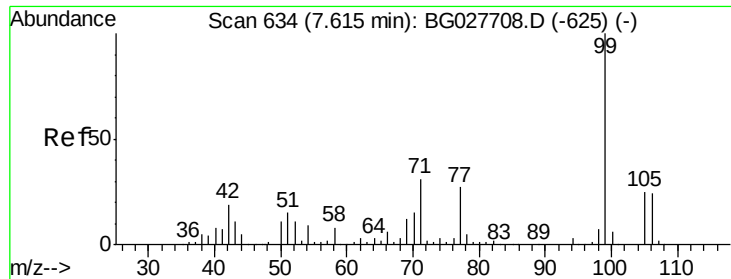

#7

Phenol-d6

Concen: 106.383 ng

RT: 7.57 min Scan# 677

Delta R.T. -0.01 min

Lab File: BG027916.D

Acq: 11 Jul 2017 17:09

Instrument :

BNA_G

ClientSampleId :

CLINTON-AVE-69KV-COMP-(DRUM


Tgt Ion: 99 Resp: 464729

Ion Ratio Lower Upper




99 100

42 10.6 20.5 30.7#

71 24.8 37.6 56.4#

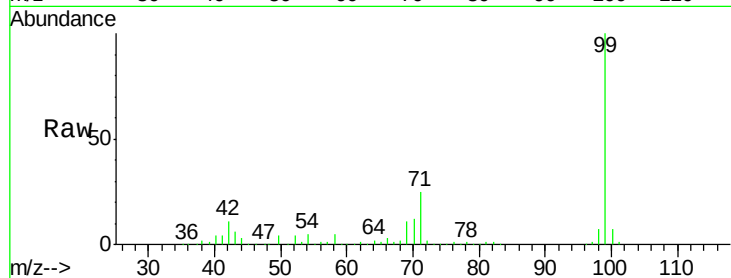

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

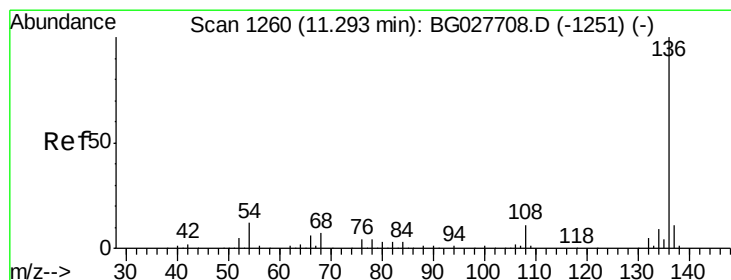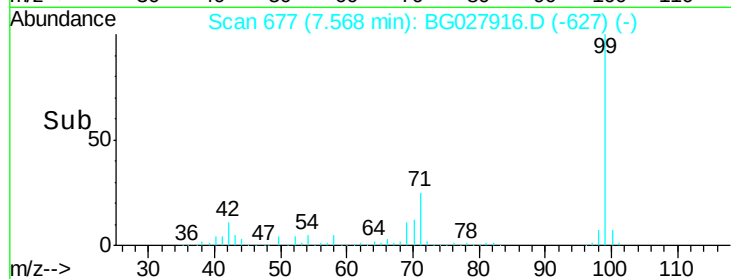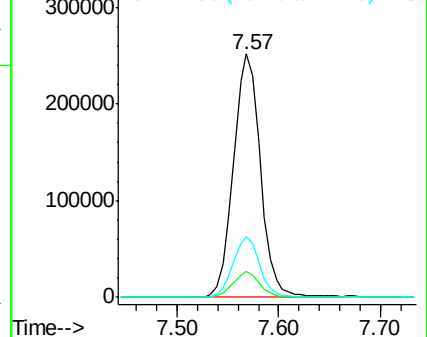

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.23 min Scan# 1301

Delta R.T. -0.01 min

Lab File: BG027916.D

Acq: 11 Jul 2017 17:09

Tgt Ion: 136 Resp: 184218


Ion Ratio Lower Upper

136 100



137 10.9 8.9 13.3


54 7.3 9.3 13.9#

68 6.4 5.1 7.7

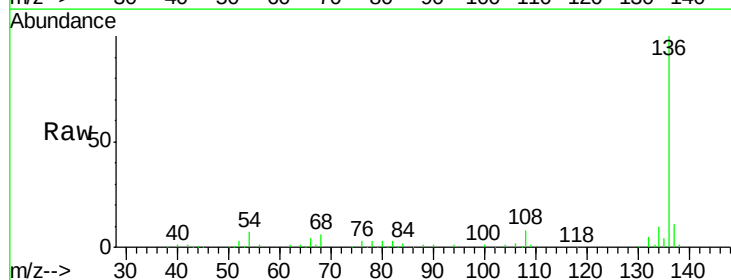

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



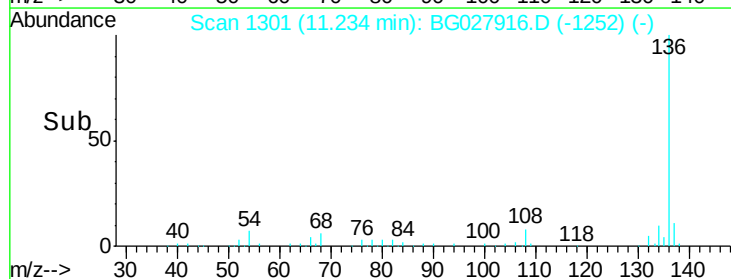
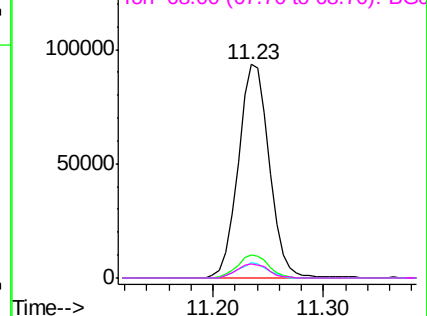


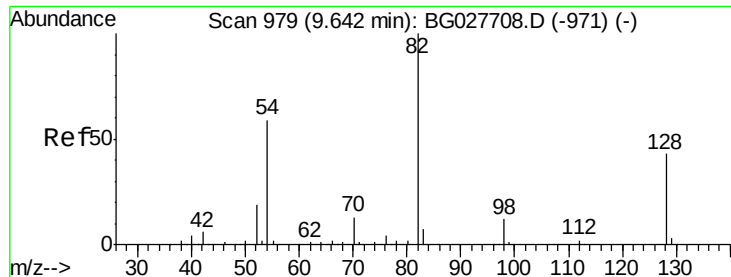

#23
 Nitrobenzene-d5
 Concen: 84.638 ng
 RT: 9.58 min Scan# 1020
 Delta R.T. -0.01 min
 Lab File: BG027916.D
 Acq: 11 Jul 2017 17:09




Instrument :
 BNA_G
 ClientSampleId :
 CLINTON-AVE-69KV-COMP-(DRUM


Tgt Ion: 82 Resp: 279722
 Ion Ratio Lower Upper
 82 100
 128 50.1 26.4 39.6#
 54 37.8 49.4 74.2#

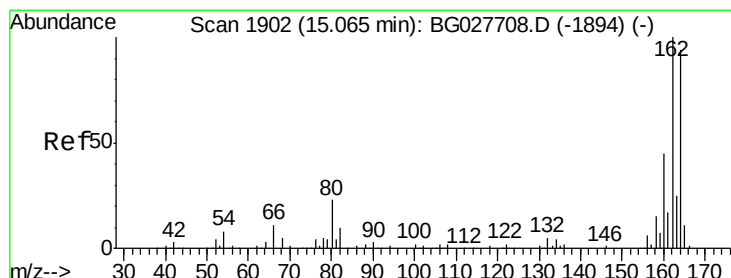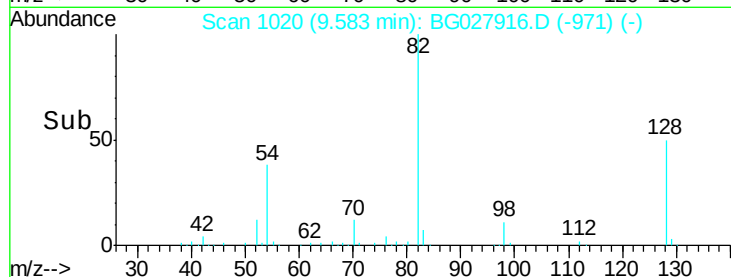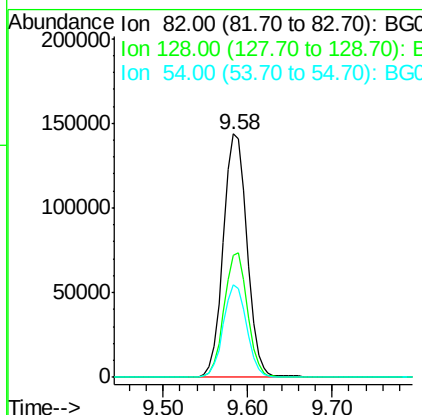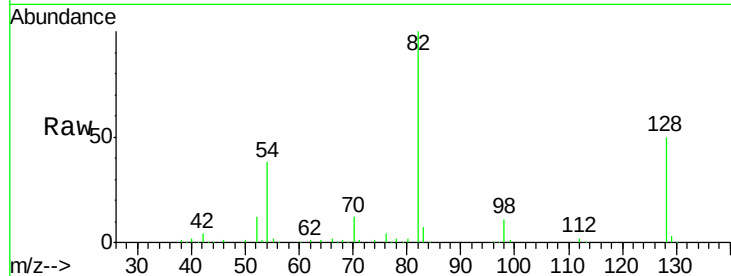

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.01 min Scan# 1944
 Delta R.T. -0.01 min
 Lab File: BG027916.D
 Acq: 11 Jul 2017 17:09

Tgt Ion: 164 Resp: 98684
 Ion Ratio Lower Upper
 164 100
 162 102.8 85.1 127.7
 160 45.0 34.7 52.1

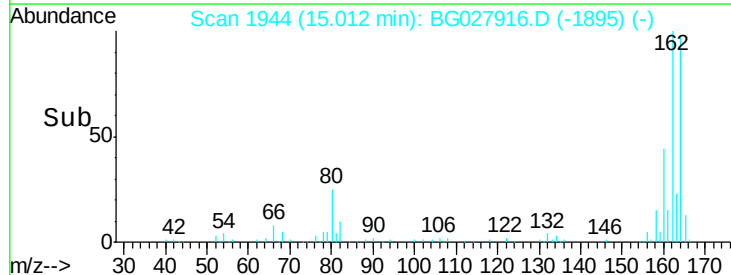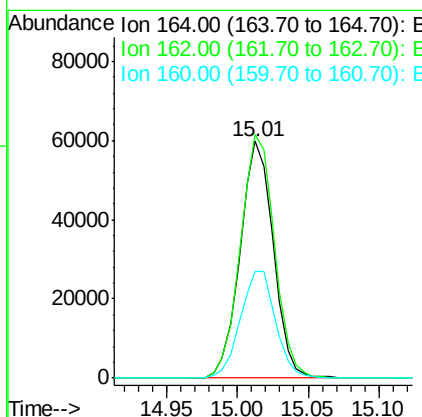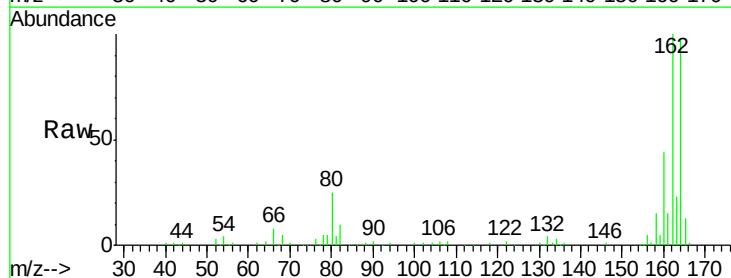


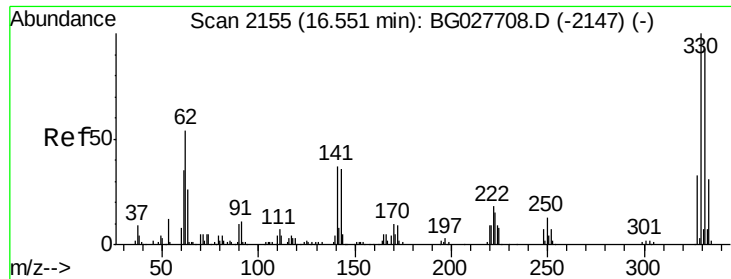




#41
 2,4,6-Tribromophenol
 Concen: 176.663 ng
 RT: 16.50 min Scan# 2197
 Delta R.T. -0.02 min
 Lab File: BG027916.D
 Acq: 11 Jul 2017 17:09

Instrument :
 BNA_G
 ClientSampleId :
 CLINTON-AVE-69KV-COMP-(DRUM

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.8	77.3	115.9
141	26.3	32.1	48.1#

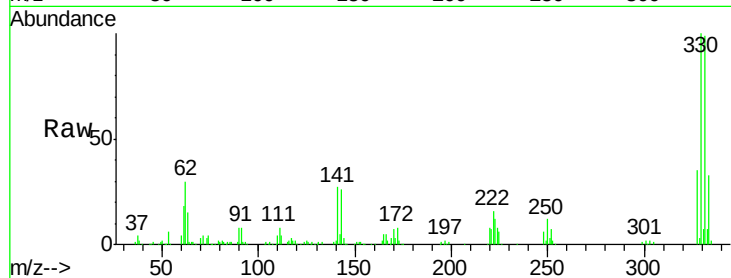


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

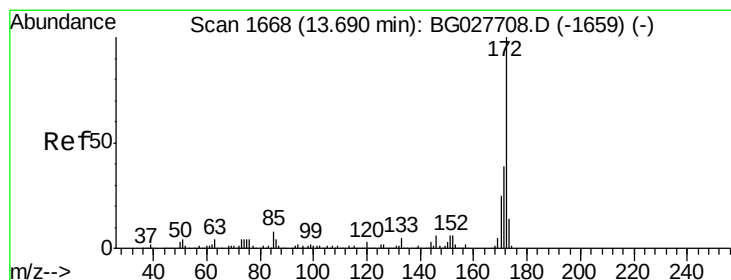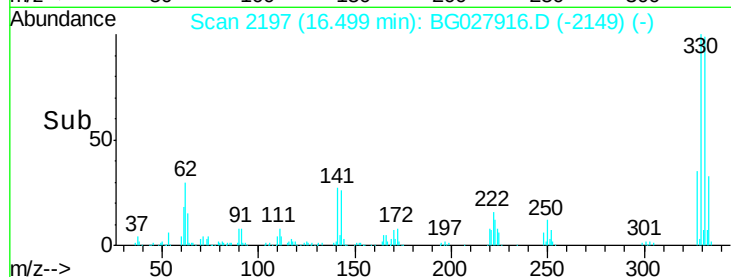
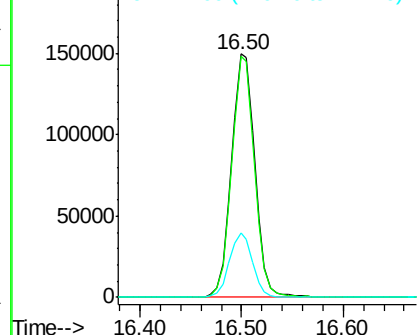



#44
 2-Fluorobiphenyl
 Concen: 106.115 ng
 RT: 13.64 min Scan# 1710
 Delta R.T. -0.01 min
 Lab File: BG027916.D
 Acq: 11 Jul 2017 17:09

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.7	32.2	48.2
170	24.5	21.8	32.6

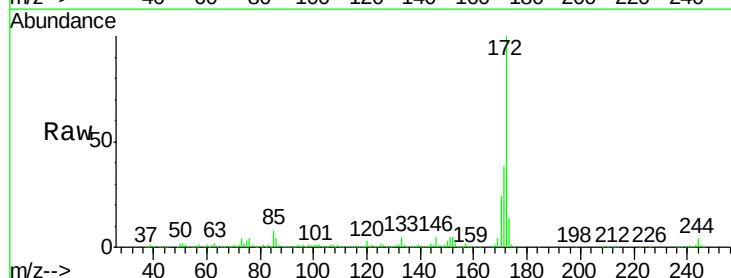

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

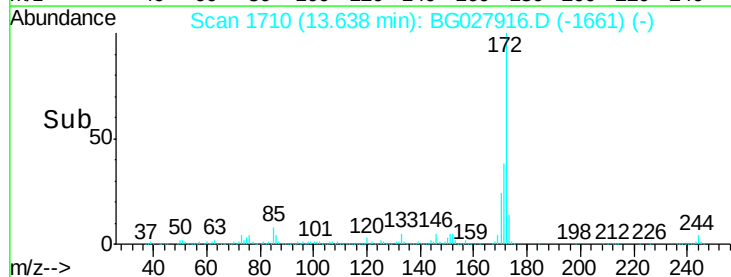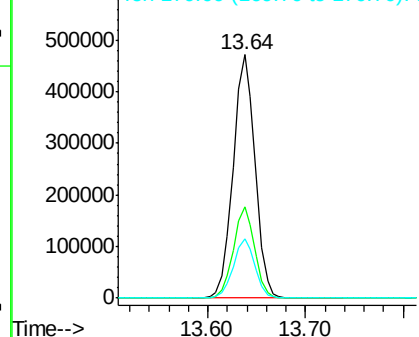


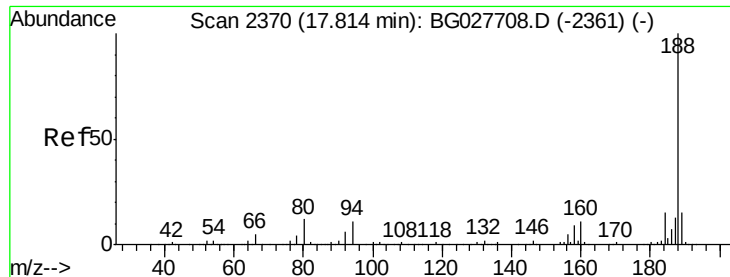




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.76 min Scan# 2412
Delta R.T. -0.01 min
Lab File: BG027916.D
Acq: 11 Jul 2017 17:09

Instrument :
BNA_G
ClientSampleId :
CLINTON-AVE-69KV-COMP-(DRUM

Tgt Ion:188 Resp: 231792
Ion Ratio Lower Upper
188 100
94 11.5 5.8 8.8#
80 12.8 7.5 11.3#

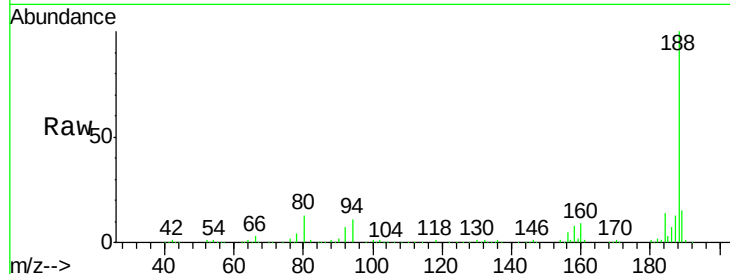


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

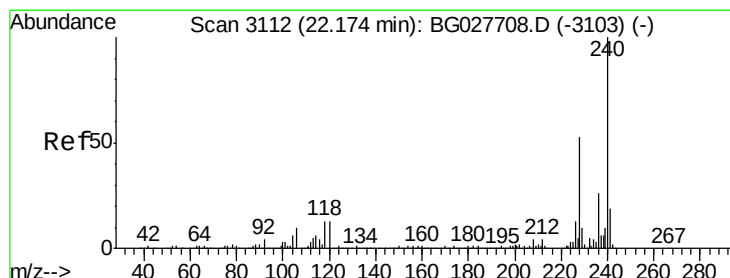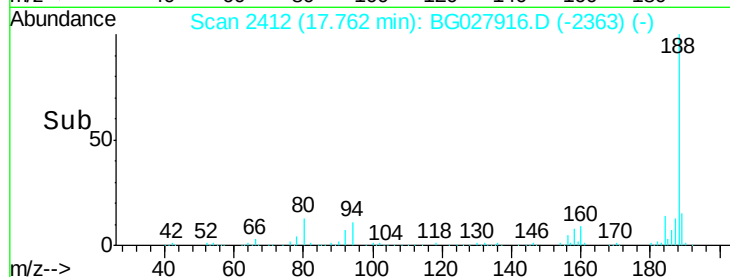
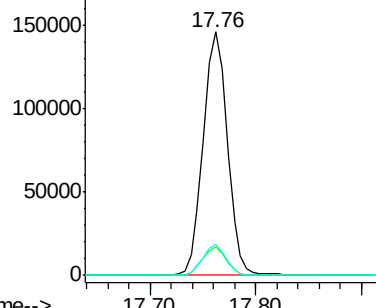



#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.10 min Scan# 3151
Delta R.T. -0.02 min
Lab File: BG027916.D
Acq: 11 Jul 2017 17:09

Tgt Ion:240 Resp: 292494
Ion Ratio Lower Upper
240 100
120 13.9 5.7 8.5#
236 25.4 22.2 33.4

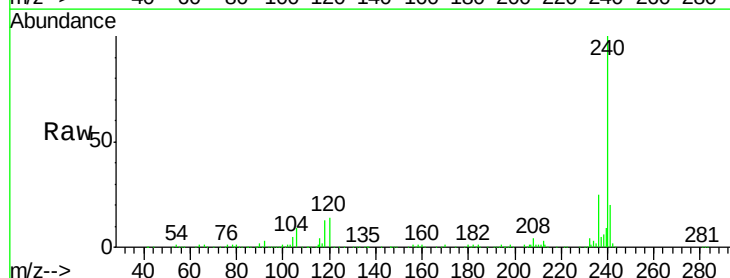

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

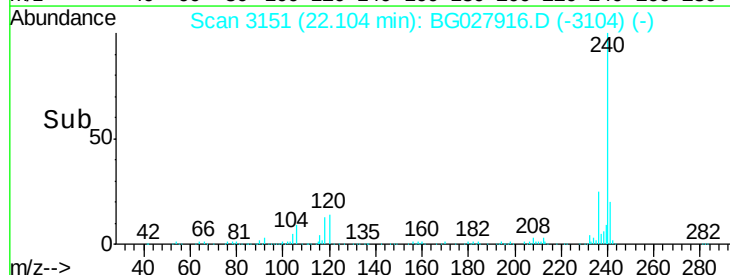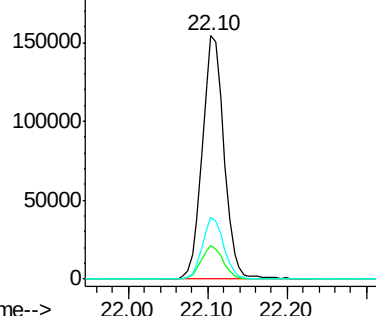

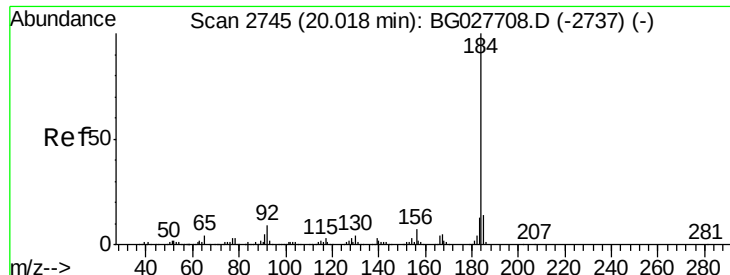

#76

Benzidine

Concen: 3.251 ng

RT: 19.94 min Scan# 2783

Delta R.T. -0.05 min

Lab File: BG027916.D

Acq: 11 Jul 2017 17:09

Instrument :

BNA_G

ClientSampleId :

CLINTON-AVE-69KV-COMP-(DRUM


Tgt Ion:184 Resp: 250

Ion Ratio Lower Upper

184 100

185 0.0 13.0 19.6#




183 0.0 11.0 16.6#

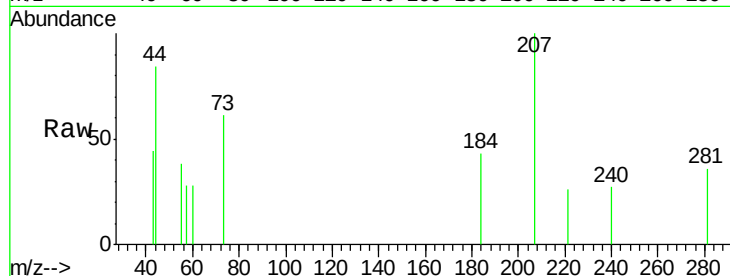

Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

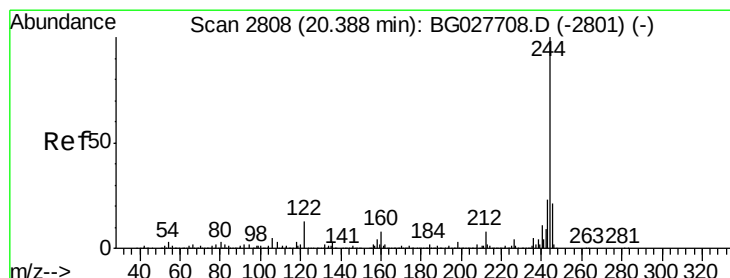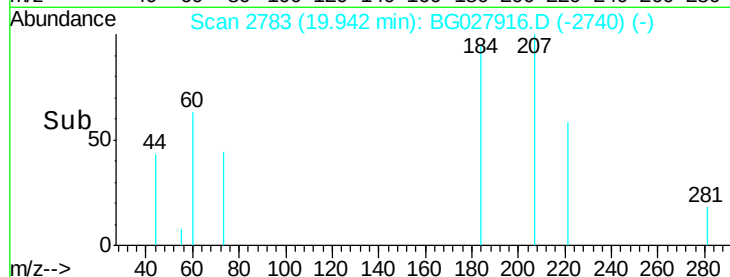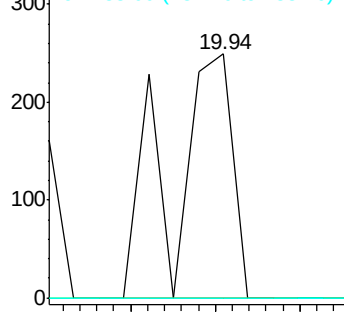

#78

Terphenyl-d14

Concen: 102.189 ng

RT: 20.34 min Scan# 2851

Delta R.T. -0.01 min

Lab File: BG027916.D

Acq: 11 Jul 2017 17:09


Tgt Ion:244 Resp: 1274955

Ion Ratio Lower Upper

244 100

212 6.7 10.0 15.0#



122 13.8 8.6 12.8#



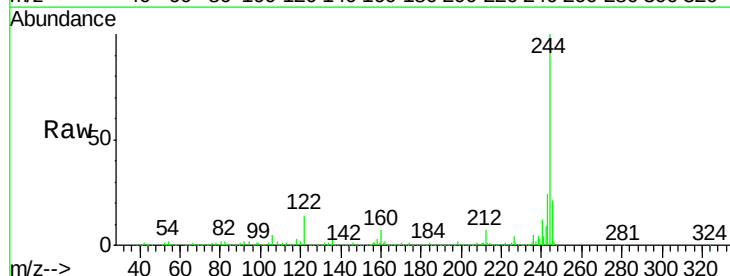


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

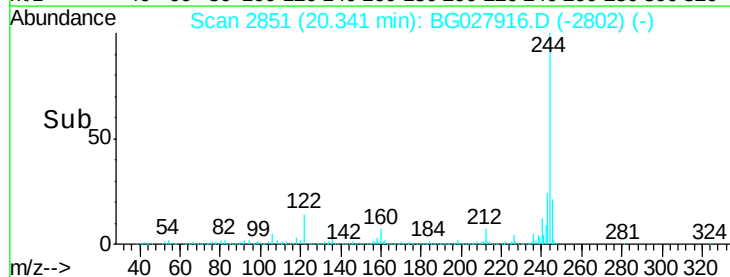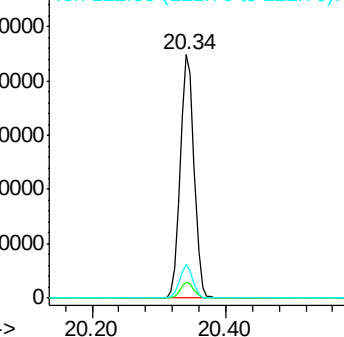

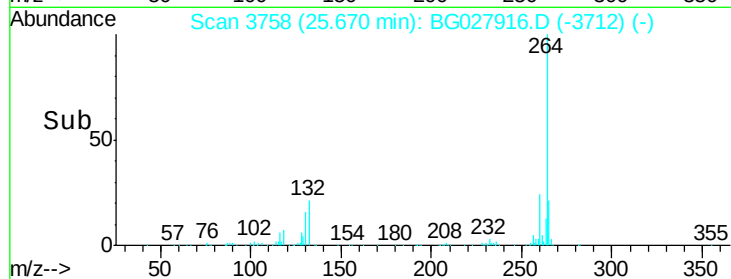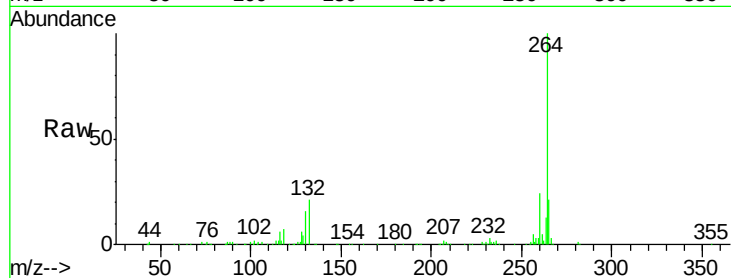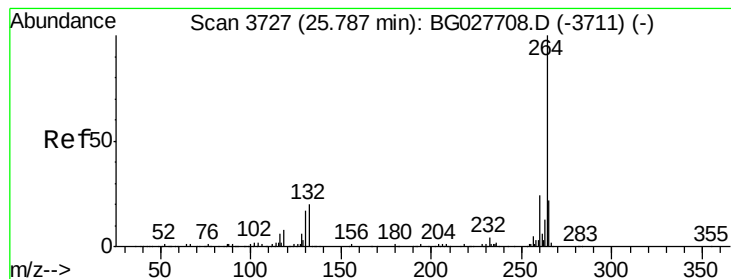

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.67 min Scan# 3758

Delta R.T. -0.03 min

Lab File: BG027916.D

Acq: 11 Jul 2017 17:09

Instrument :

BNA_G

ClientSampleId :

CLINTON-AVE-69KV-COMP-(DRUM

Tgt Ion: 264 Resp: 282202

Ion Ratio Lower Upper

264 100

260 23.8 21.8 32.8

265 21.3 18.2 27.4

