

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071017\
 Data File : BG027898.D
 Acq On : 10 Jul 2017 22:06
 Operator : SJ/JU
 Sample : I4071-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 HR-06-070617-C

Quant Time: Jul 11 07:51:05 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 17:43:21 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.42	152	41336	20.00	ng	0.00
21) Naphthalene-d8	11.23	136	175021	20.00	ng	-0.01
38) Acenaphthene-d10	15.01	164	95595	20.00	ng	-0.01
63) Phenanthrene-d10	17.76	188	249607	20.00	ng	-0.01
75) Chrysene-d12	22.11	240	308255	20.00	ng	-0.02
86) Perylene-d12	25.67	264	300045	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	6.00	112	356839	132.93	ng	0.00
7) Phenol-d6	7.57	99	438218	106.86	ng	0.00
23) Nitrobenzene-d5	9.58	82	258966	82.48	ng	-0.01
41) 2,4,6-Tribromophenol	16.50	330	241654	184.30	ng	-0.01
44) 2-Fluorobiphenyl	13.64	172	662333	98.95	ng	-0.01
78) Terphenyl-d14	20.34	244	1348792	102.58	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071017\
Data File : BG027898.D
Acq On : 10 Jul 2017 22:06
Operator : SJ/JU
Sample : I4071-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
HR-06-070617-C

Quant Time: Jul 11 07:51:05 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 17:43:21 2017
Response via : Initial Calibration

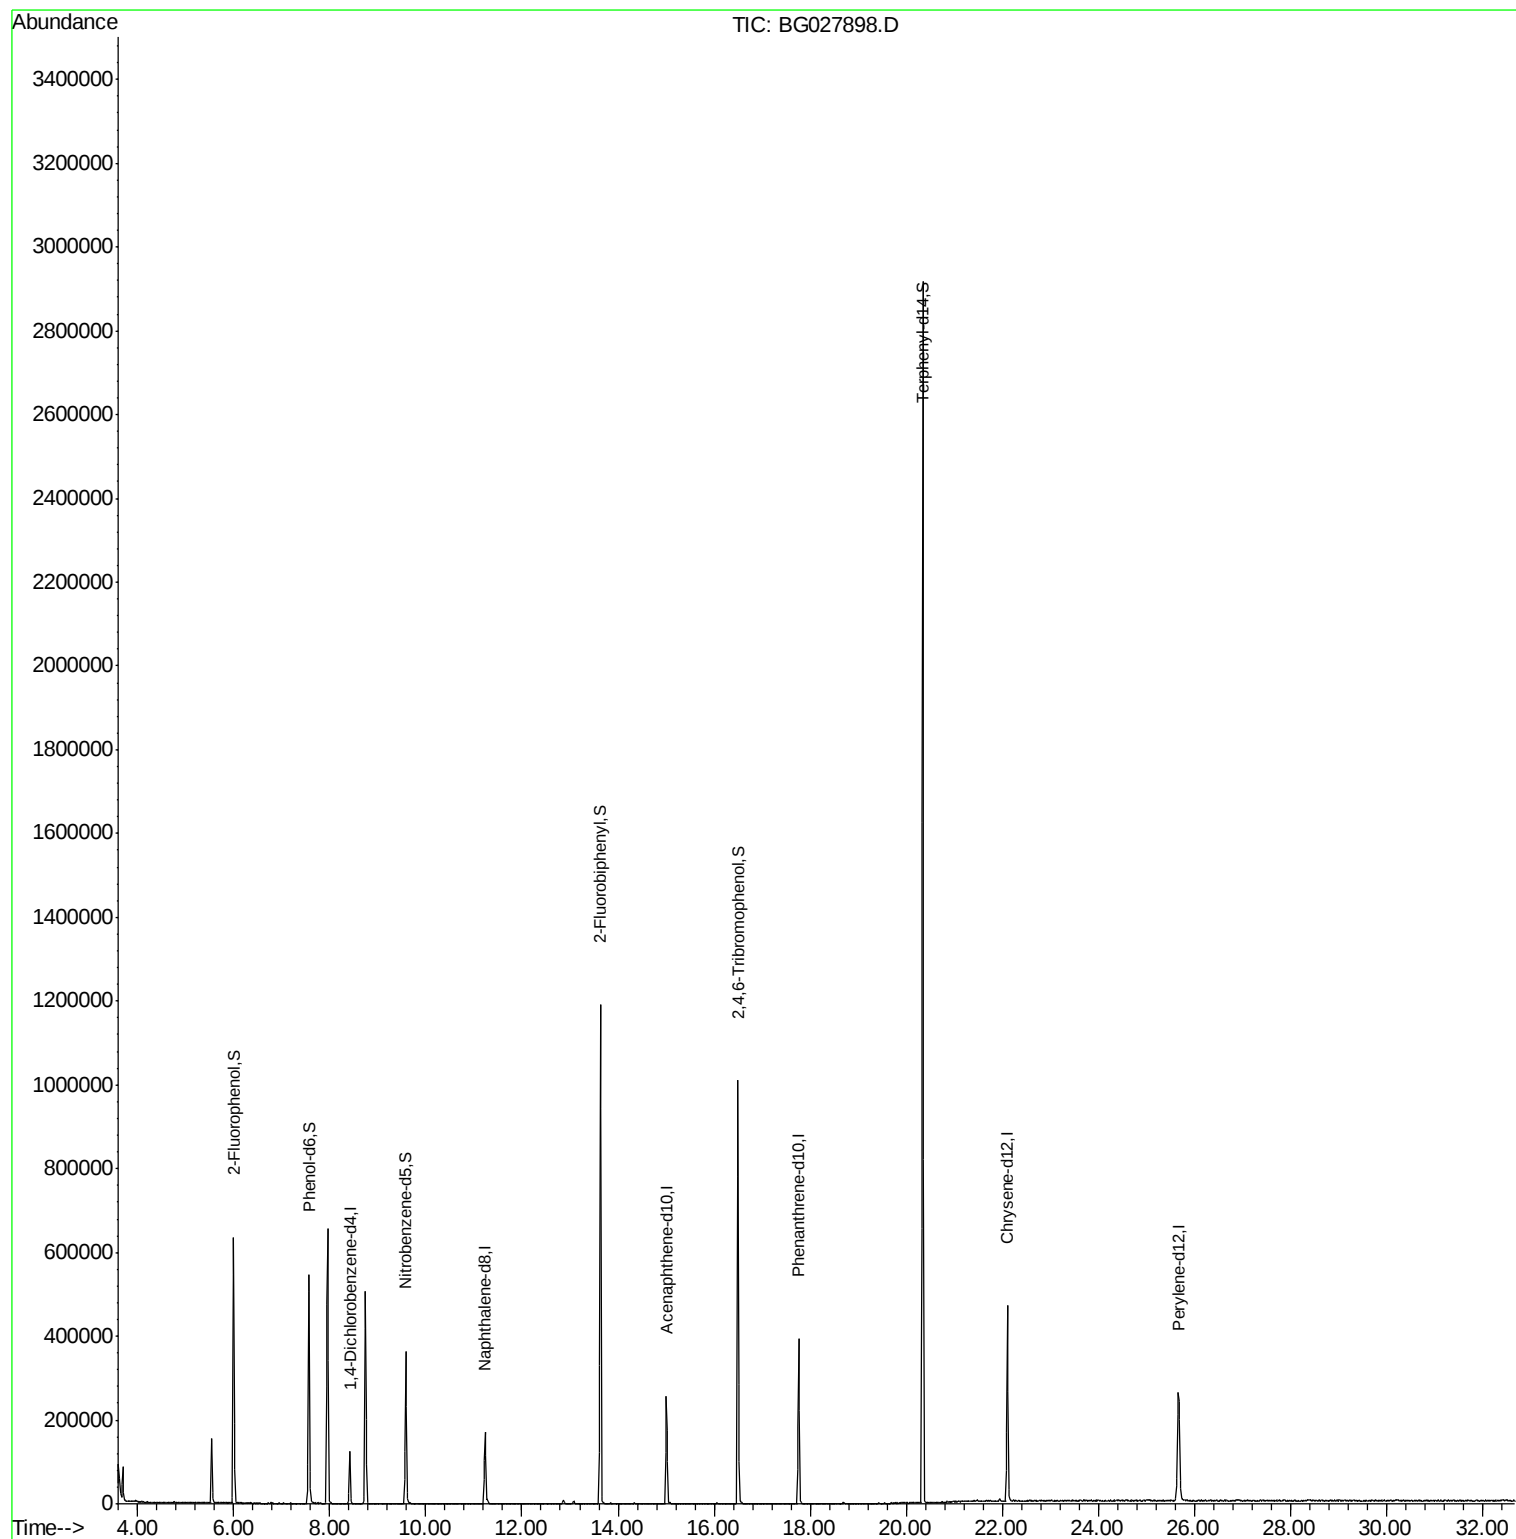

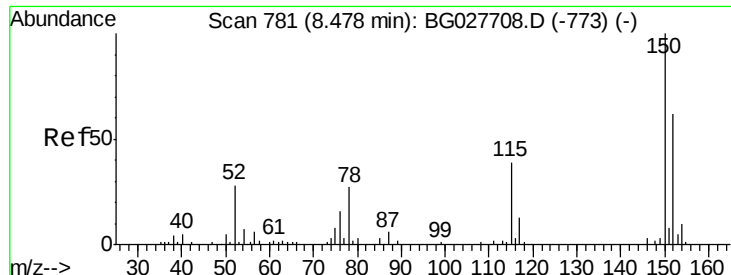


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.42 min Scan# 822
Delta R.T. -0.01 min
Lab File: BG027898.D
Acq: 10 Jul 2017 22:06

Instrument :
BNA_G
ClientSampleId :
HR-06-070617-C

Tgt Ion:152 Resp: 41336
Ion Ratio Lower Upper
152 100
150 156.6 114.0 171.0
115 56.9 48.1 72.1

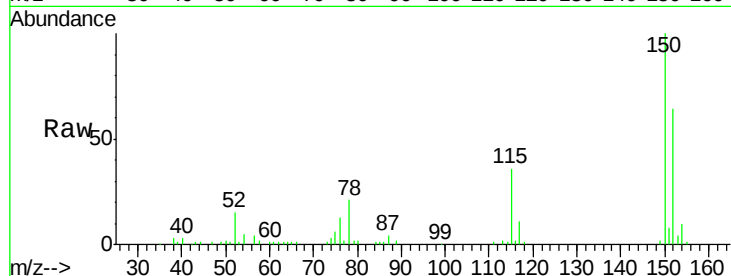


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

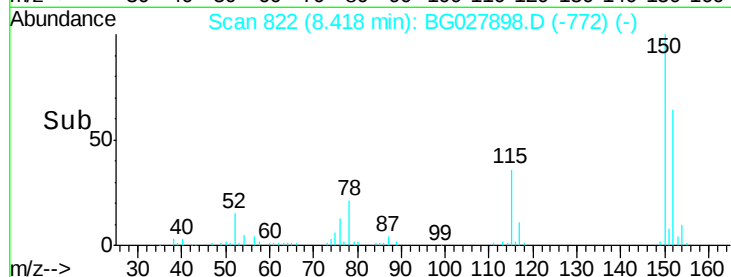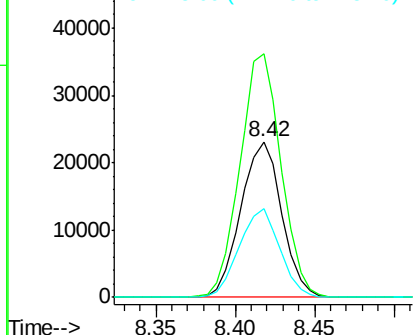



#5

2-Fluorophenol
Concen: 132.935 ng
RT: 6.00 min Scan# 410
Delta R.T. -0.01 min
Lab File: BG027898.D
Acq: 10 Jul 2017 22:06

Tgt Ion:112 Resp: 356839
Ion Ratio Lower Upper
112 100
64 53.1 61.8 92.6#
63 24.6 37.2 55.8#

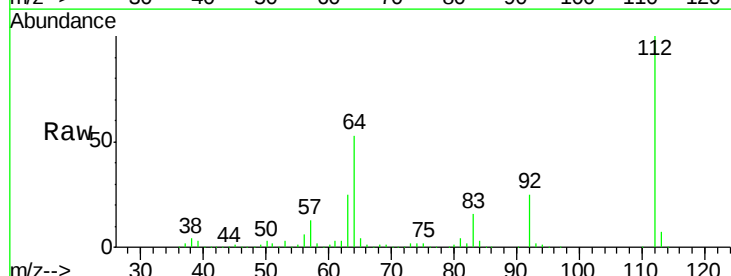

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

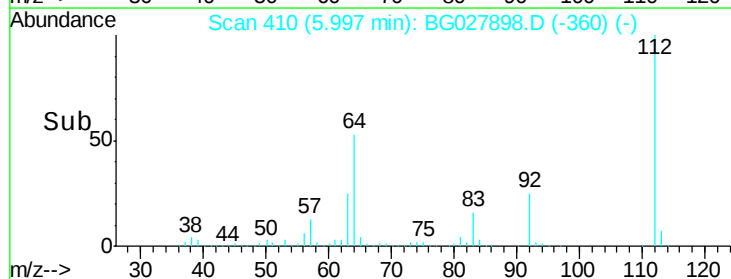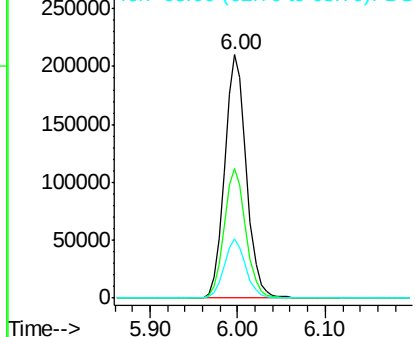



#7

Phenol-d6

Concen: 106.861 ng

RT: 7.57 min Scan# 677

Delta R.T. -0.01 min

Lab File: BG027898.D

Acq: 10 Jul 2017 22:06

Instrument :

BNA_G

ClientSampleId :

HR-06-070617-C


Tgt Ion: 99 Resp: 438218

Ion Ratio Lower Upper




99 100

42 10.0 20.5 30.7#

71 24.1 37.6 56.4#

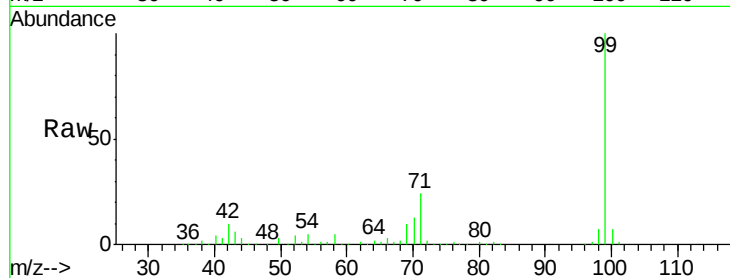

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

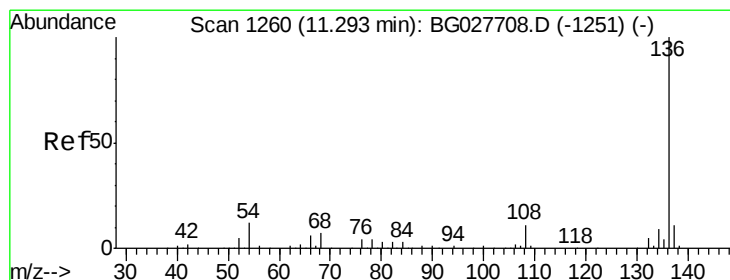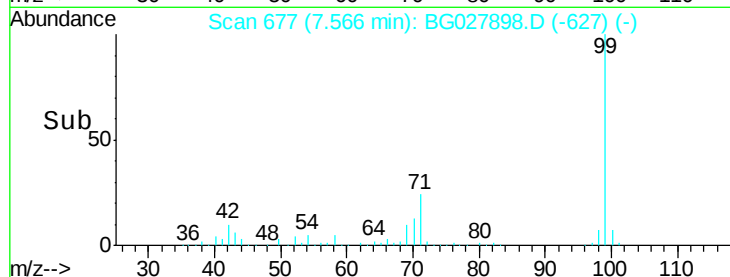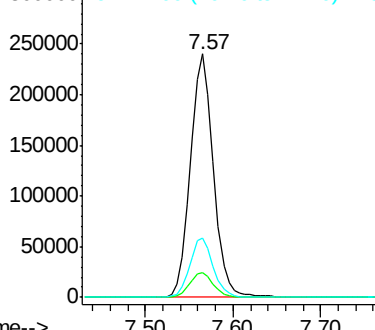

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.23 min Scan# 1301

Delta R.T. -0.01 min

Lab File: BG027898.D

Acq: 10 Jul 2017 22:06

Tgt Ion: 136 Resp: 175021


Ion Ratio Lower Upper

136 100



137 11.0 8.9 13.3

54 7.6 9.3 13.9#

68 7.0 5.1 7.7

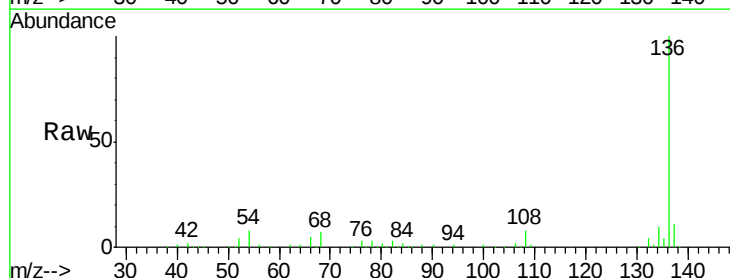

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

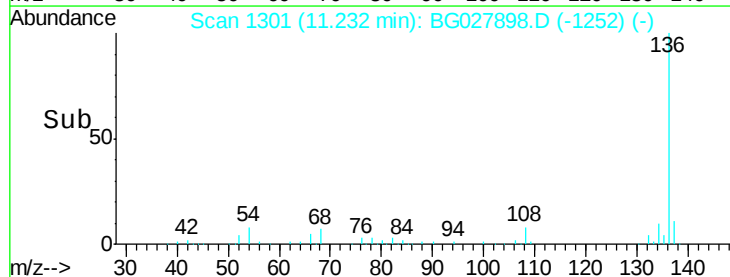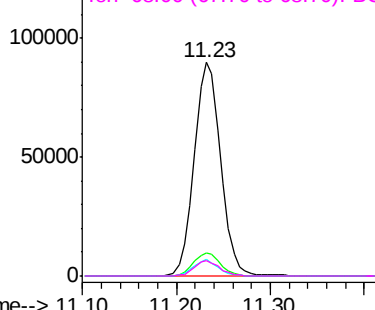







#23
 Nitrobenzene-d5
 Concen: 82.476 ng
 RT: 9.58 min Scan# 1020
 Delta R.T. -0.01 min
 Lab File: BG027898.D
 Acq: 10 Jul 2017 22:06

Instrument :
 BNA_G
 ClientSampleId :
 HR-06-070617-C

Tgt Ion: 82 Resp: 258966
 Ion Ratio Lower Upper
 82 100
 128 49.5 26.4 39.6#
 54 37.8 49.4 74.2#

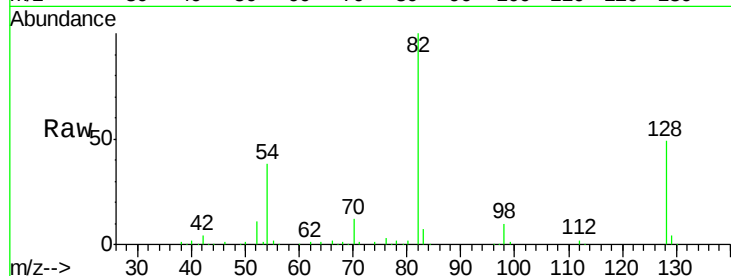


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

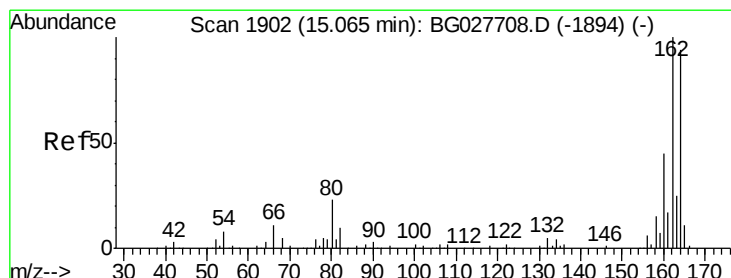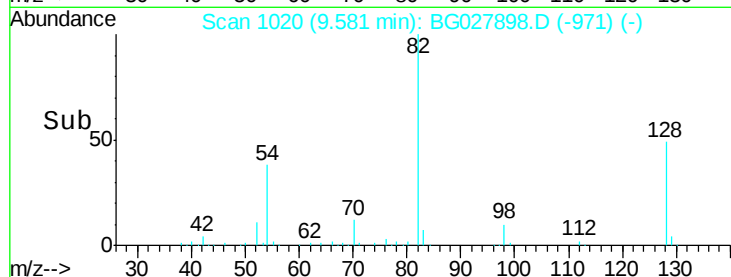
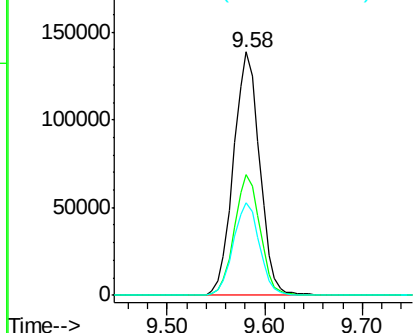



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.01 min Scan# 1944
 Delta R.T. -0.01 min
 Lab File: BG027898.D
 Acq: 10 Jul 2017 22:06

Tgt Ion: 164 Resp: 95595
 Ion Ratio Lower Upper
 164 100
 162 103.7 85.1 127.7
 160 46.1 34.7 52.1

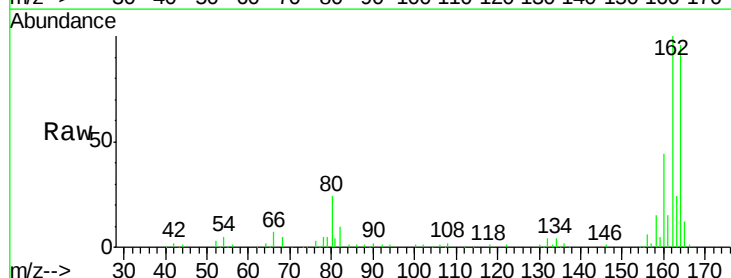

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

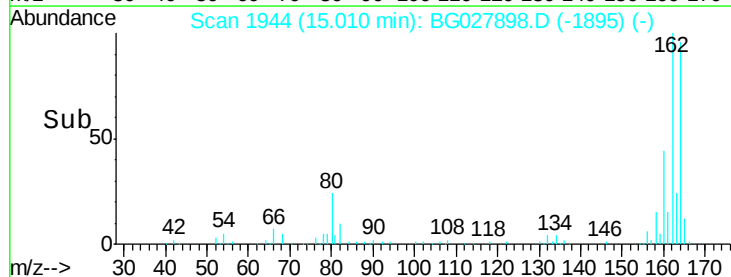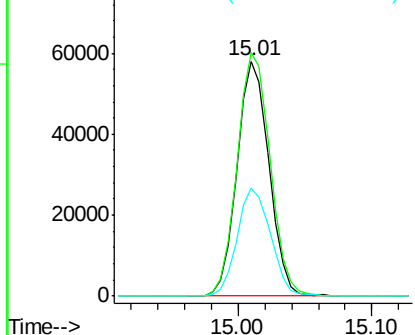


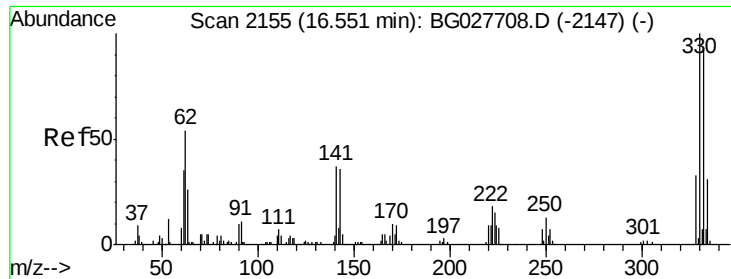




#41
 2,4,6-Tribromophenol
 Concen: 184.301 ng
 RT: 16.50 min Scan# 2198
 Delta R.T. -0.01 min
 Lab File: BG027898.D
 Acq: 10 Jul 2017 22:06

Instrument :
 BNA_G
 ClientSampleId :
 HR-06-070617-C

Tgt Ion	Ratio	Lower	Upper
330	100		
332	97.3	77.3	115.9
141	27.6	32.1	48.1#

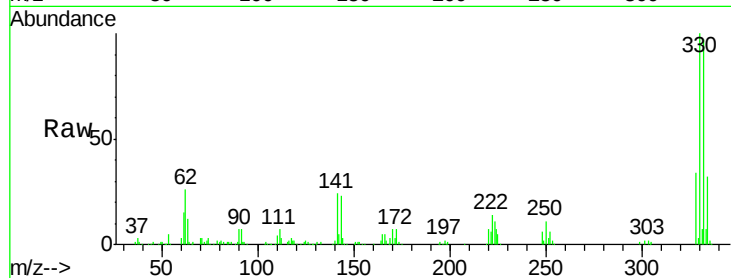


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

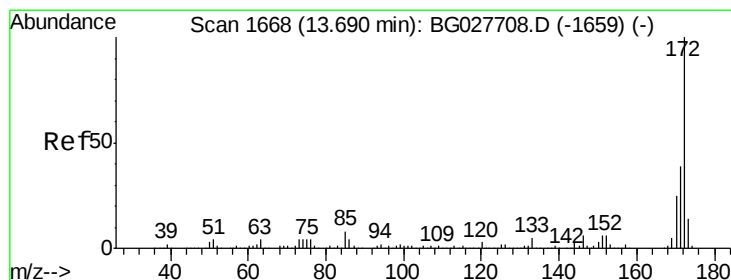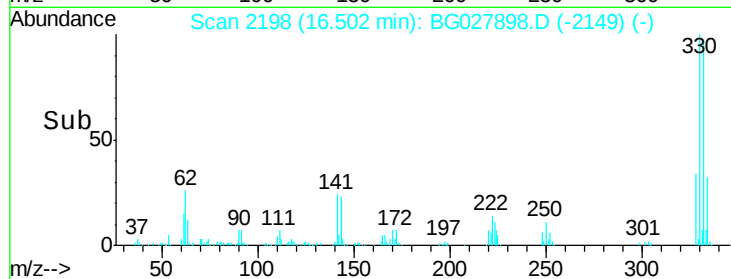
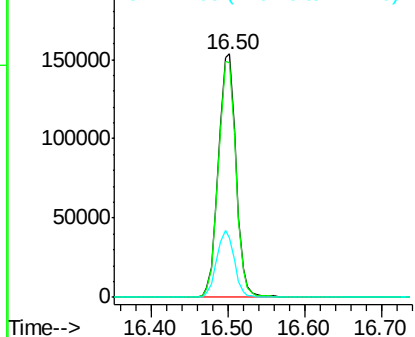



#44
 2-Fluorobiphenyl
 Concen: 98.951 ng
 RT: 13.64 min Scan# 1710
 Delta R.T. -0.01 min
 Lab File: BG027898.D
 Acq: 10 Jul 2017 22:06

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.2	32.2	48.2
170	24.2	21.8	32.6

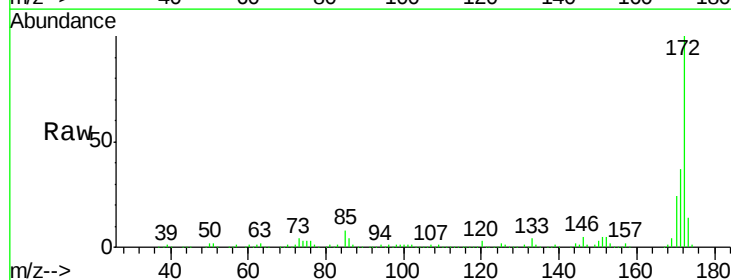

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

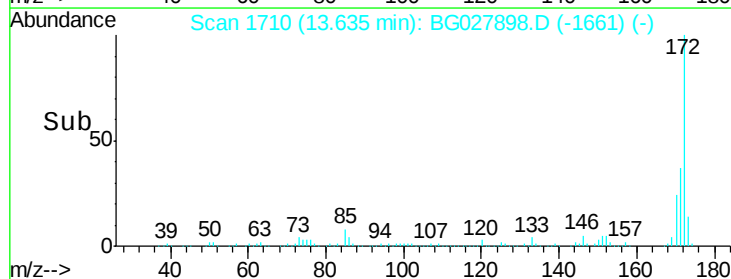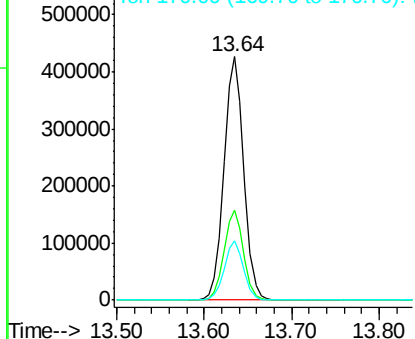

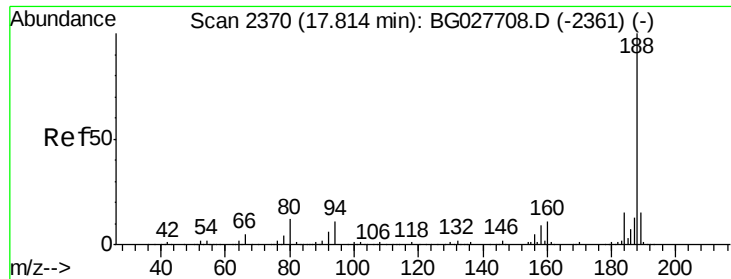

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.76 min Scan# 2412

Delta R.T. -0.01 min

Lab File: BG027898.D

Acq: 10 Jul 2017 22:06

Instrument :

BNA_G

ClientSampleId :

HR-06-070617-C


Tgt Ion:188 Resp: 249607

Ion Ratio Lower Upper

188 100

94 12.2 5.8 8.8#




80 13.2 7.5 11.3#

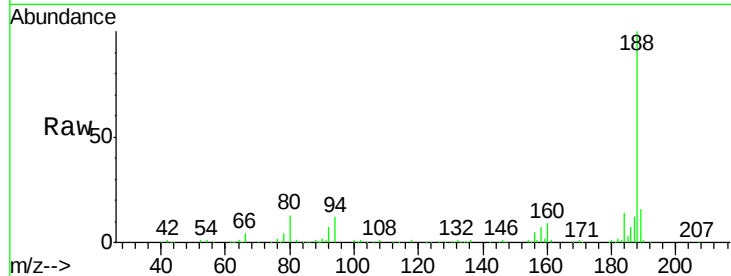

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

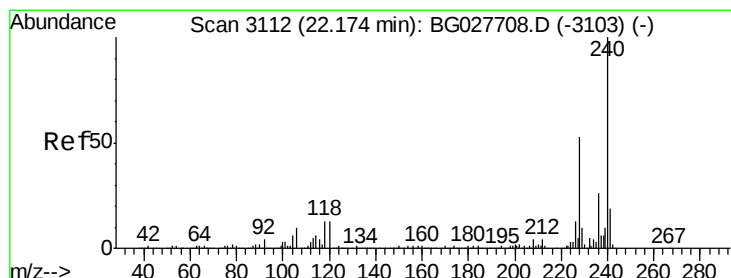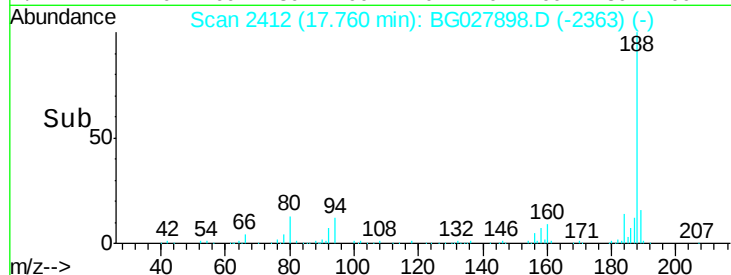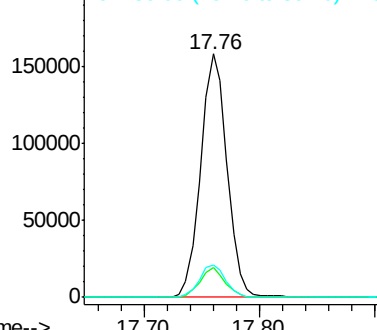

#75

Chrysene-d12

Concen: 20.000 ng

RT: 22.11 min Scan# 3152

Delta R.T. -0.02 min

Lab File: BG027898.D

Acq: 10 Jul 2017 22:06


Tgt Ion:240 Resp: 308255

Ion Ratio Lower Upper

240 100

120 14.3 5.7 8.5#



236 24.6 22.2 33.4

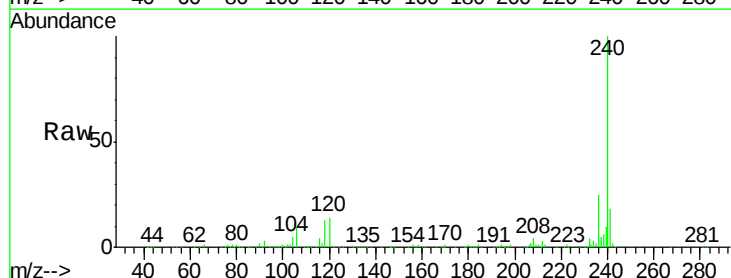

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

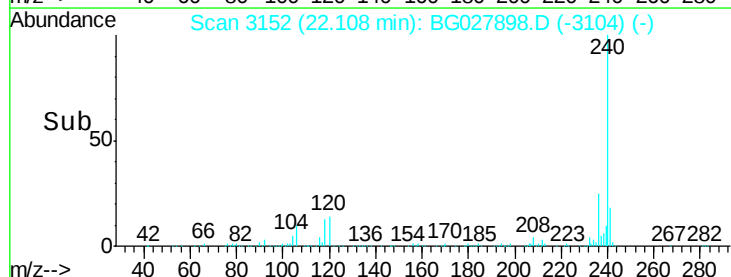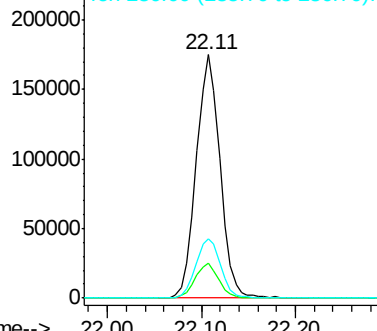



#78

Terphenyl-d14

Concen: 102.580 ng

RT: 20.34 min Scan# 2852

Delta R.T. -0.01 min

Lab File: BG027898.D

Acq: 10 Jul 2017 22:06

Instrument :

BNA_G

ClientSampleId :

HR-06-070617-C


Tgt Ion:244 Resp: 1348792

Ion Ratio Lower Upper

244 100

212 6.4 10.0 15.0#



122 13.2 8.6 12.8#

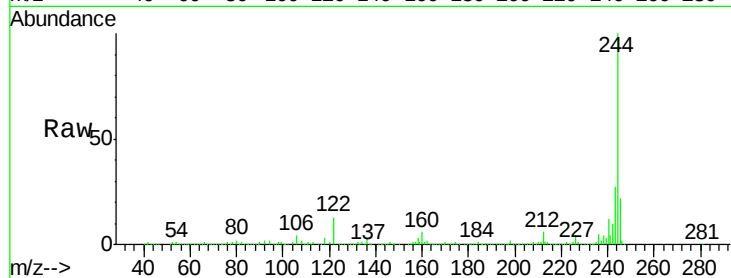

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

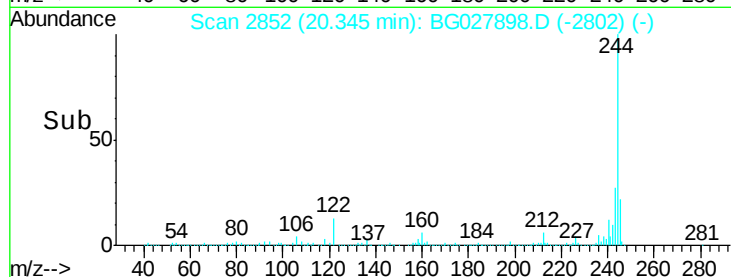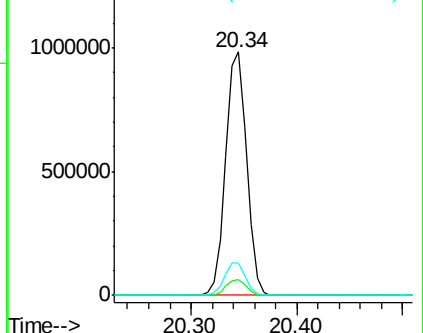

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.67 min Scan# 3758

Delta R.T. -0.03 min

Lab File: BG027898.D

Acq: 10 Jul 2017 22:06


Tgt Ion:264 Resp: 300045

Ion Ratio Lower Upper

264 100

260 23.9 21.8 32.8

265 22.7 18.2 27.4

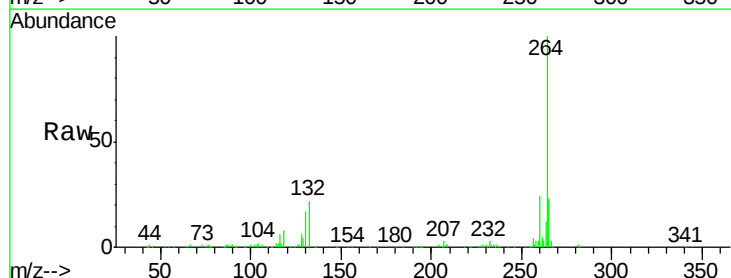

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

