

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071017\
 Data File : BG027907.D
 Acq On : 11 Jul 2017 4:02
 Operator : SJ/JU
 Sample : I4078-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 VNJ-211

Quant Time: Jul 11 08:09:17 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 17:43:21 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.42	152	25554	20.00	ng	0.00
21) Naphthalene-d8	11.24	136	112551	20.00	ng	0.00
38) Acenaphthene-d10	15.01	164	66951	20.00	ng	-0.02
63) Phenanthrene-d10	17.76	188	222242	20.00	ng	-0.02
75) Chrysene-d12	22.11	240	282790	20.00	ng	-0.02
86) Perylene-d12	25.67	264	276764	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	6.00	112	221005	133.18	ng	0.00
7) Phenol-d6	7.56	99	279397	110.21	ng	0.00
23) Nitrobenzene-d5	9.58	82	158052	78.28	ng	-0.02
41) 2,4,6-Tribromophenol	16.50	330	203609	221.72	ng	-0.02
44) 2-Fluorobiphenyl	13.63	172	409188	87.29	ng	-0.02
78) Terphenyl-d14	20.34	244	1507639	124.99	ng	-0.01


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071017\
Data File : BG027907.D
Acq On : 11 Jul 2017 4:02
Operator : SJ/JU
Sample : I4078-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
VNJ-211

Quant Time: Jul 11 08:09:17 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 17:43:21 2017
Response via : Initial Calibration

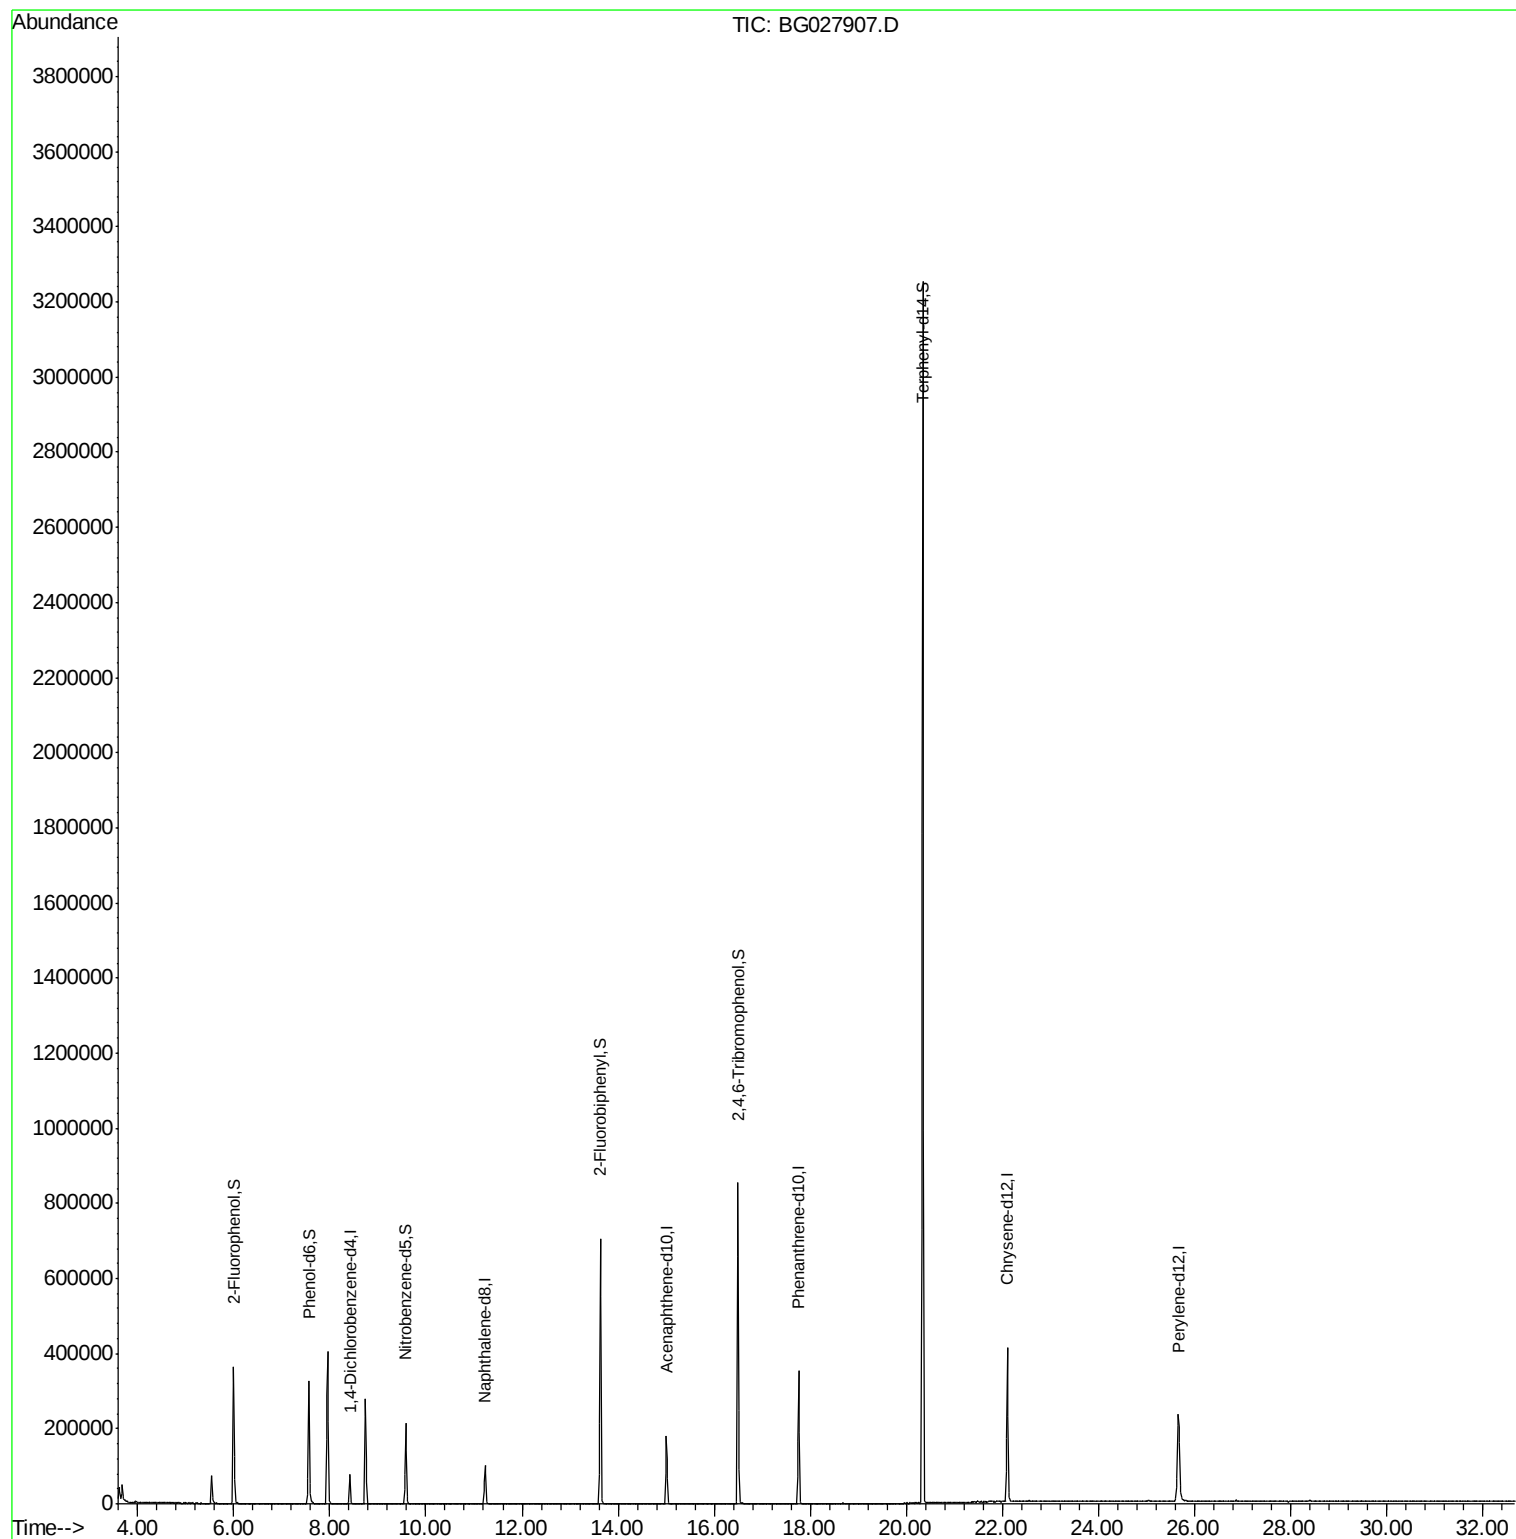




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.42 min Scan# 822
 Delta R.T. -0.01 min
 Lab File: BG027907.D
 Acq: 11 Jul 2017 4:02

Instrument :
 BNA_G
 ClientSampleId :
 VNJ-211

Tgt Ion:152 Resp: 25554
 Ion Ratio Lower Upper
 152 100
 150 151.4 114.0 171.0
 115 54.9 48.1 72.1

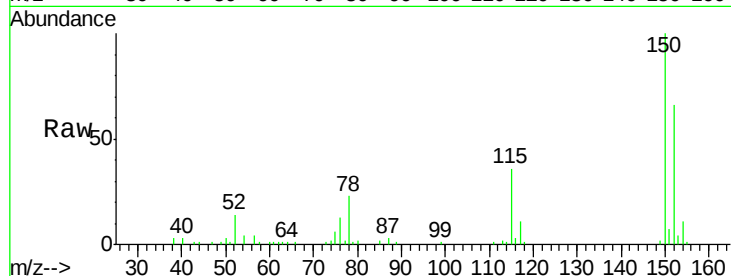


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

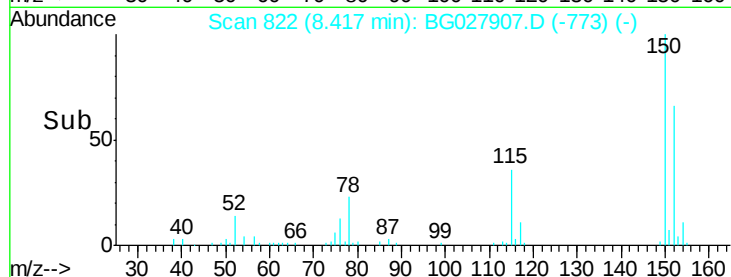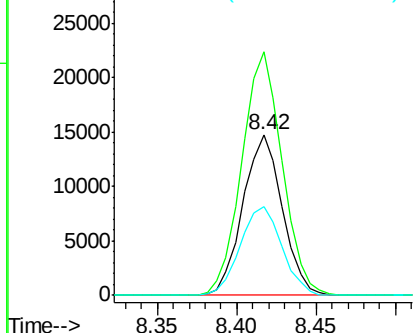



#5

2-Fluorophenol
 Concen: 133.180 ng
 RT: 6.00 min Scan# 410
 Delta R.T. -0.01 min
 Lab File: BG027907.D
 Acq: 11 Jul 2017 4:02

Tgt Ion:112 Resp: 221005
 Ion Ratio Lower Upper
 112 100
 64 51.5 61.8 92.6#
 63 24.0 37.2 55.8#

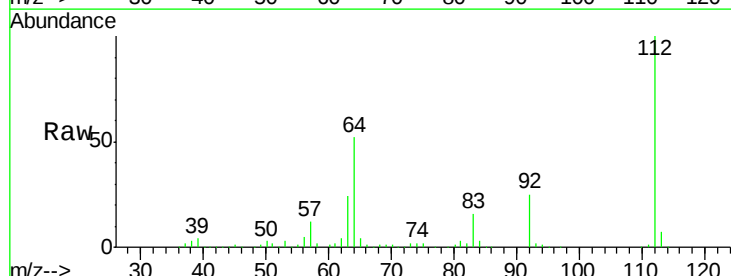

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BGC
 Ion 63.00 (62.70 to 63.70): BGC

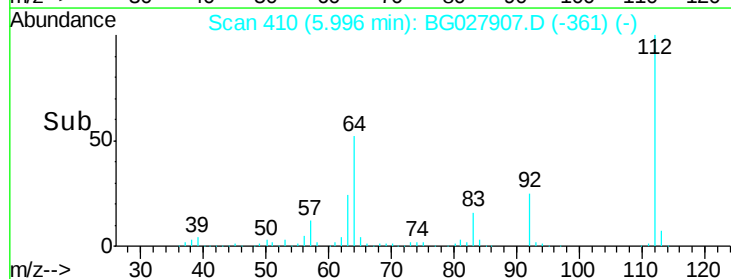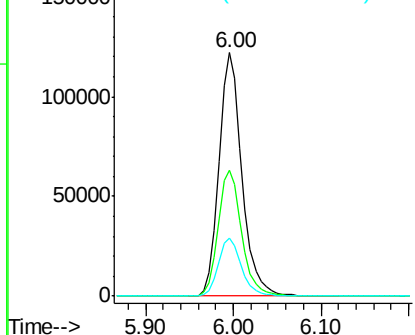



#7

Phenol-d6

Concen: 110.210 ng

RT: 7.56 min Scan# 677

Delta R.T. -0.01 min

Lab File: BG027907.D

Acq: 11 Jul 2017 4:02

Instrument :

BNA_G

ClientSampleId :

VNJ-211


Tgt Ion: 99 Resp: 279397

Ion Ratio Lower Upper




99 100

42 10.1 20.5 30.7#

71 24.2 37.6 56.4#

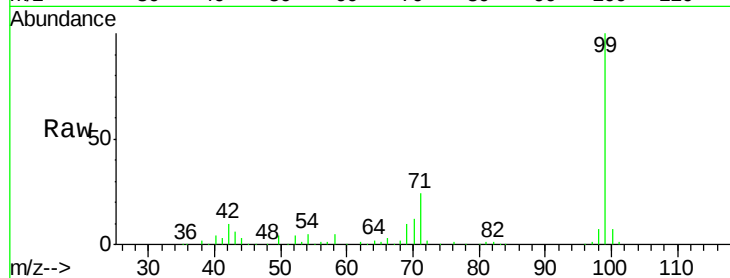

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

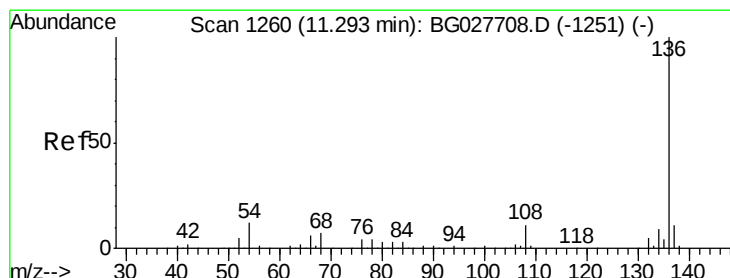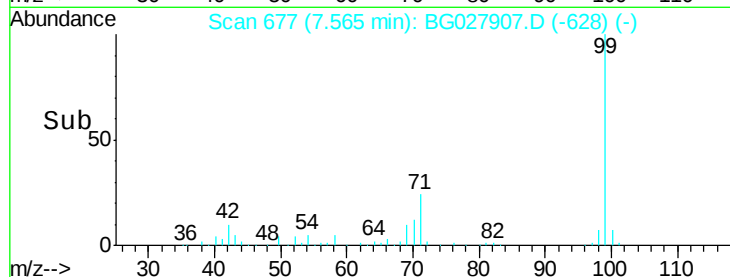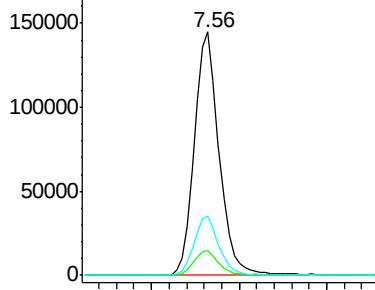

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.24 min Scan# 1302

Delta R.T. -0.01 min

Lab File: BG027907.D

Acq: 11 Jul 2017 4:02

Tgt Ion: 136 Resp: 112551


Ion Ratio Lower Upper

136 100



137 11.0 8.9 13.3


54 6.7 9.3 13.9#

68 6.9 5.1 7.7

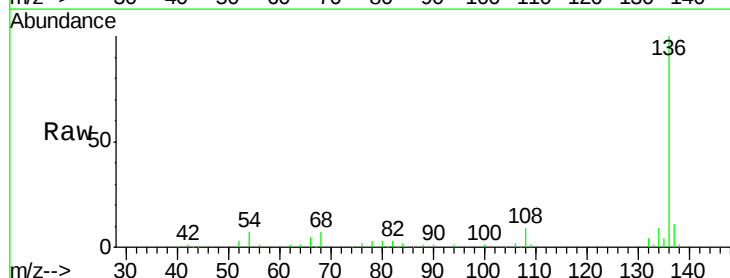

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



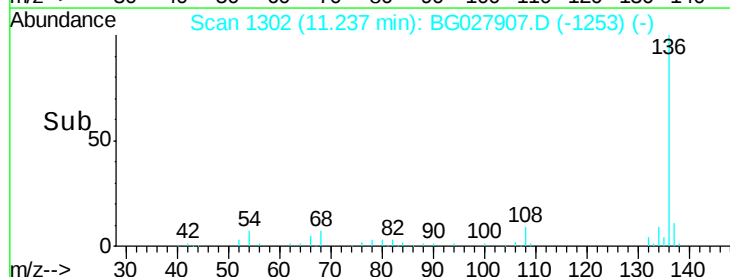
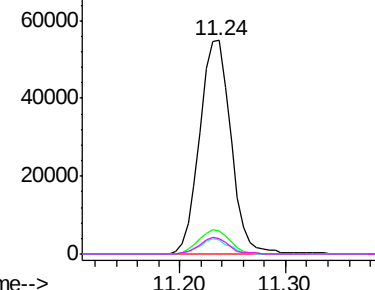


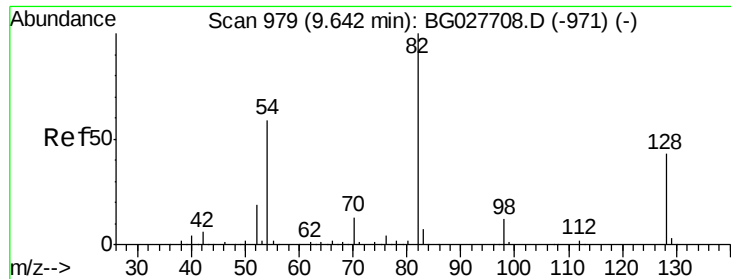

#23
 Nitrobenzene-d5
 Concen: 78.275 ng
 RT: 9.58 min Scan# 1020
 Delta R.T. -0.02 min
 Lab File: BG027907.D
 Acq: 11 Jul 2017 4:02




Instrument :
 BNA_G
 ClientSampleId :
 VNJ-211


Tgt Ion: 82 Resp: 158052
 Ion Ratio Lower Upper
 82 100
 128 49.1 26.4 39.6#
 54 37.1 49.4 74.2#

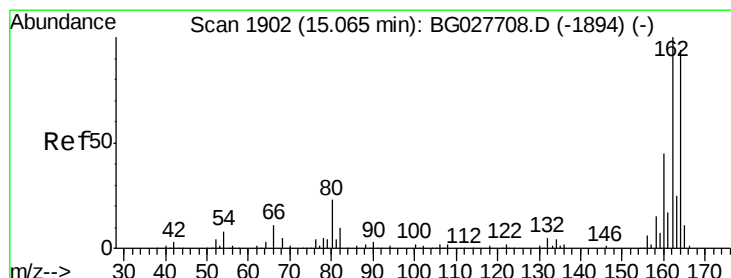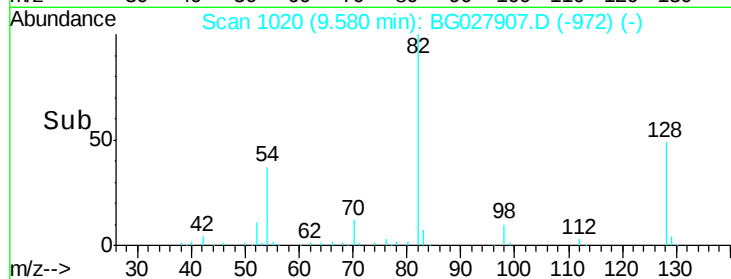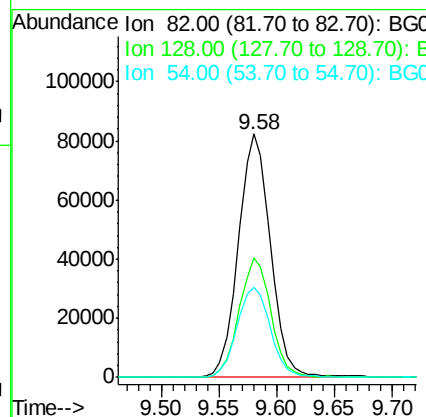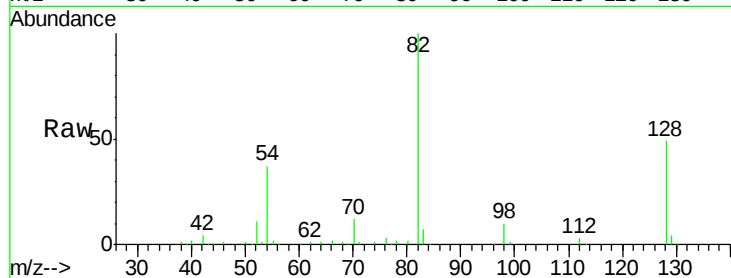

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.01 min Scan# 1944
 Delta R.T. -0.02 min
 Lab File: BG027907.D
 Acq: 11 Jul 2017 4:02

Tgt Ion: 164 Resp: 66951
 Ion Ratio Lower Upper
 164 100
 162 106.6 85.1 127.7
 160 45.2 34.7 52.1


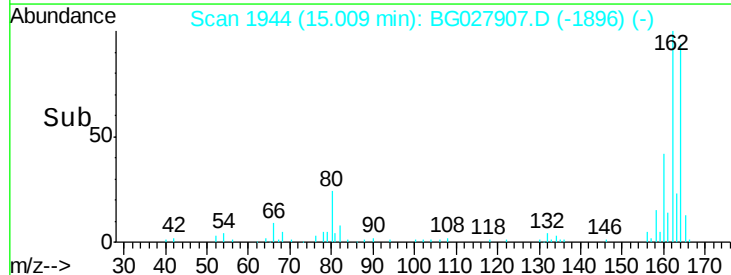
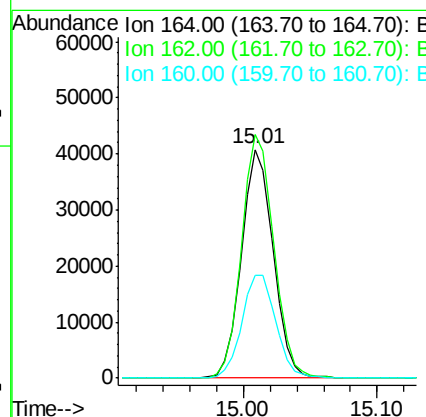
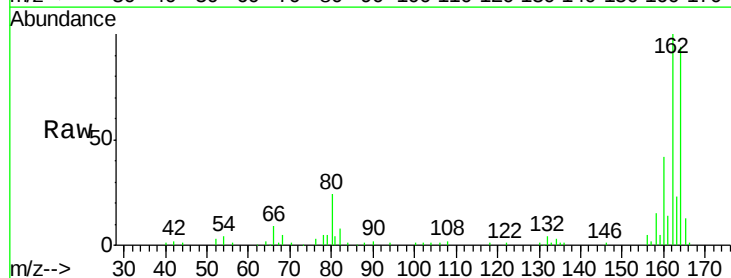


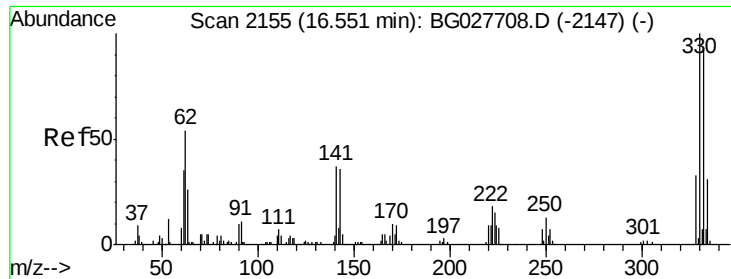

#41
 2,4,6-Tribromophenol
 Concen: 221.722 ng
 RT: 16.50 min Scan# 2197
 Delta R.T. -0.02 min
 Lab File: BG027907.D
 Acq: 11 Jul 2017 4:02




Instrument :
 BNA_G
 ClientSampleId :
 VNJ-211

Tgt Ion	Ratio	Lower	Upper
330	100		
332	97.0	77.3	115.9
141	27.5	32.1	48.1#

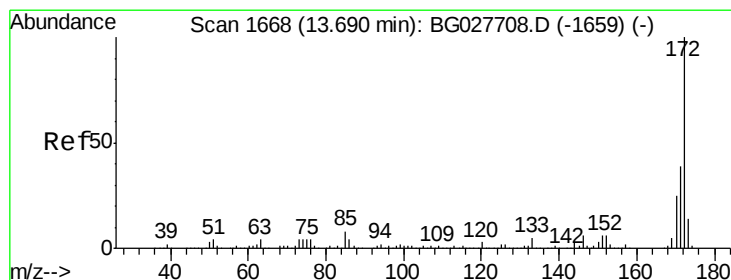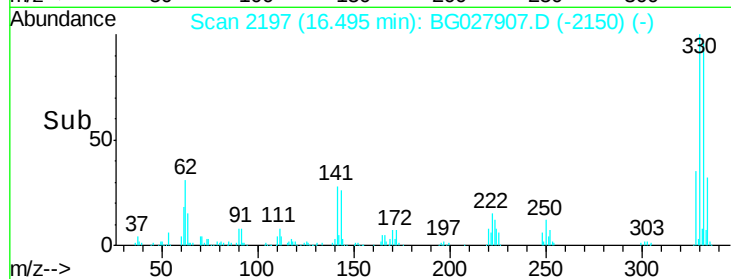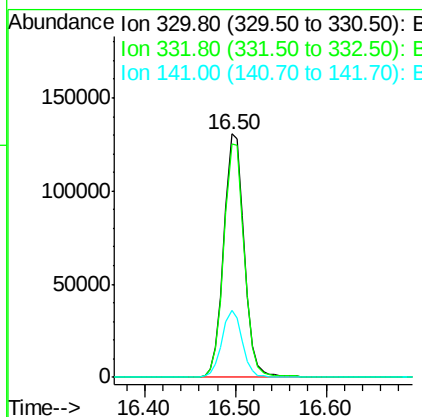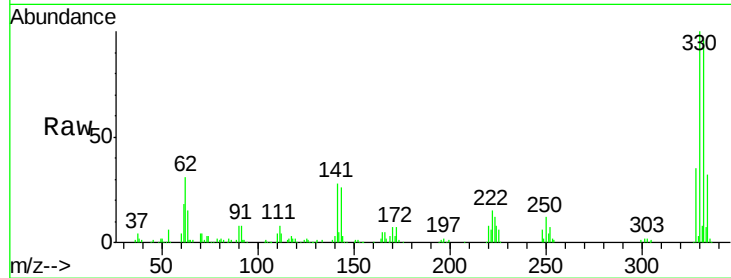

#44
 2-Fluorobiphenyl
 Concen: 87.286 ng
 RT: 13.63 min Scan# 1710
 Delta R.T. -0.02 min
 Lab File: BG027907.D
 Acq: 11 Jul 2017 4:02

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.6	32.2	48.2
170	23.3	21.8	32.6


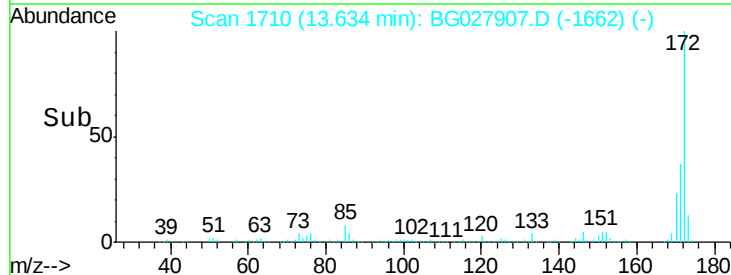
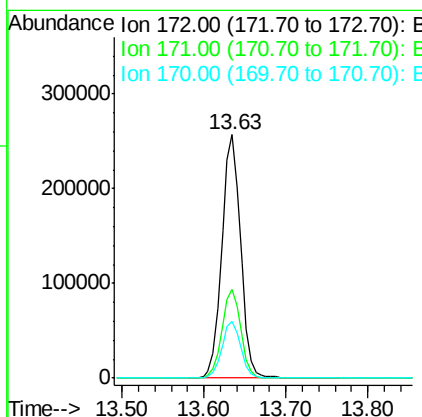
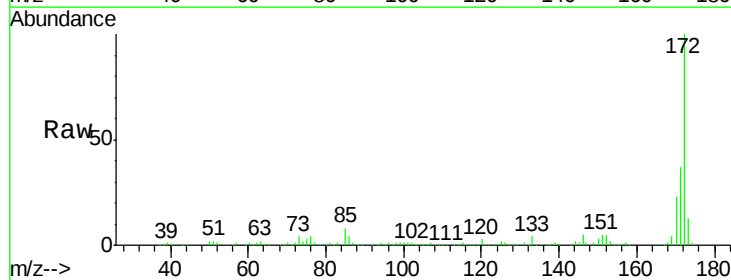




#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.76 min Scan# 2412
 Delta R.T. -0.02 min
 Lab File: BG027907.D
 Acq: 11 Jul 2017 4:02




Instrument :
 BNA_G
 ClientSampleId :
 VNJ-211

Tgt Ion:188 Resp: 222242
 Ion Ratio Lower Upper
 188 100
 94 11.4 5.8 8.8#
 80 13.1 7.5 11.3#

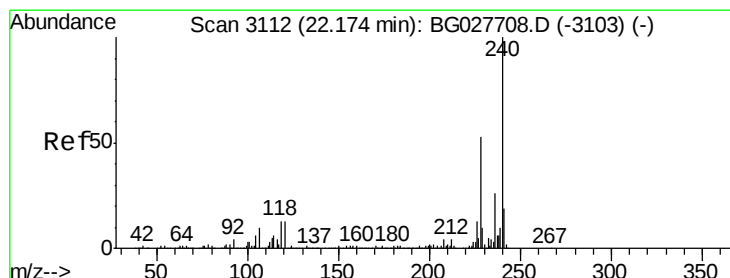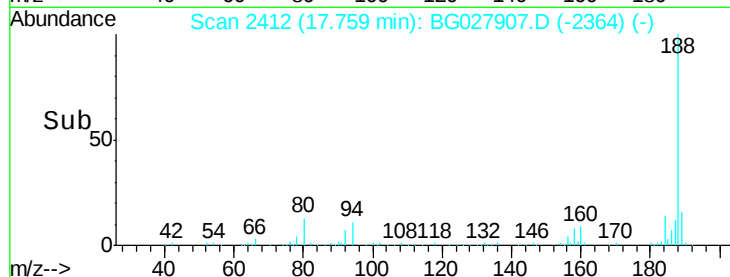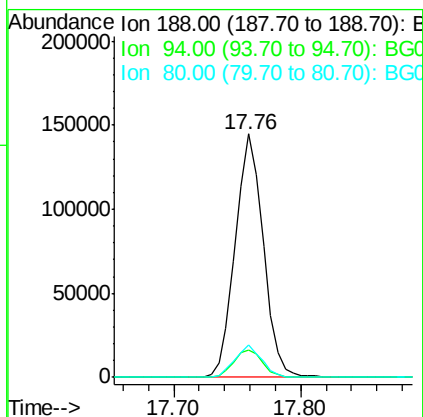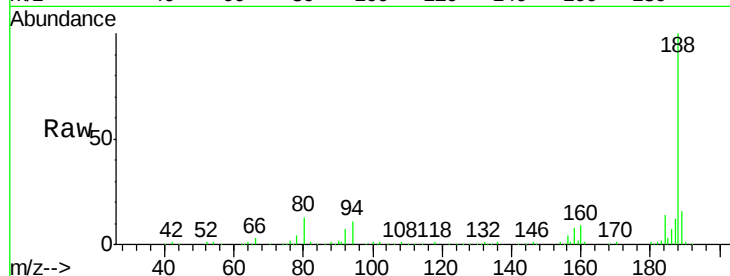

#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 22.11 min Scan# 3152
 Delta R.T. -0.02 min
 Lab File: BG027907.D
 Acq: 11 Jul 2017 4:02

Tgt Ion:240 Resp: 282790
 Ion Ratio Lower Upper
 240 100
 120 13.8 5.7 8.5#
 236 25.5 22.2 33.4

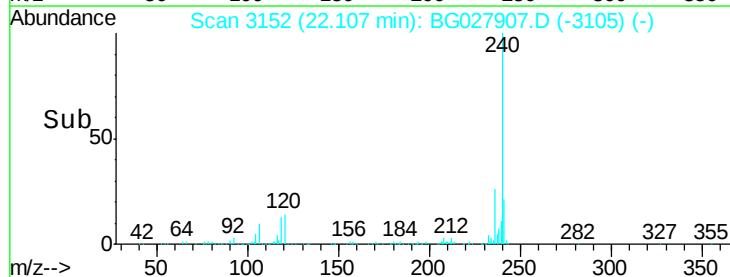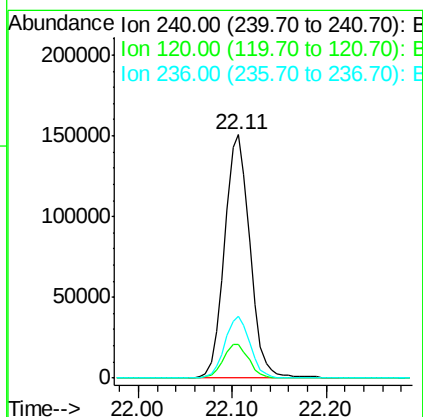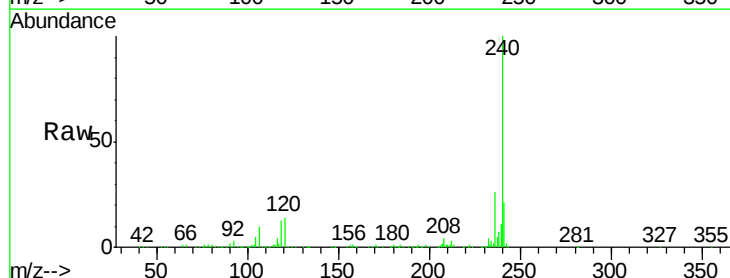



#78

Terphenyl-d14

Concen: 124.985 ng

RT: 20.34 min Scan# 2852

Delta R.T. -0.01 min

Lab File: BG027907.D

Acq: 11 Jul 2017 4:02

Instrument :

BNA_G

ClientSampleId :

VNJ-211


Tgt Ion:244 Resp: 1507639

Ion Ratio Lower Upper




244 100

212 6.8 10.0 15.0#

122 13.6 8.6 12.8#

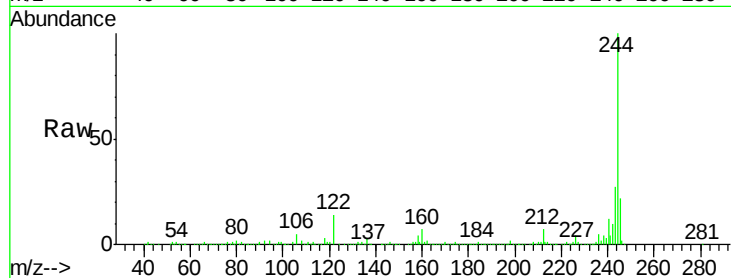

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

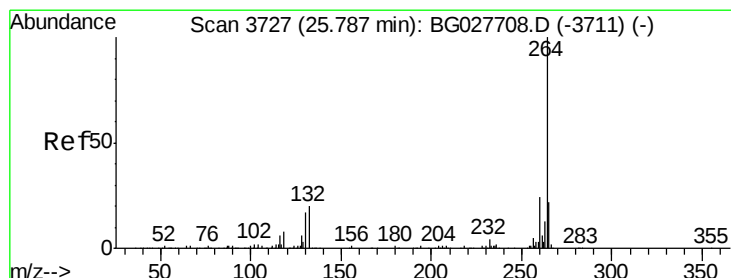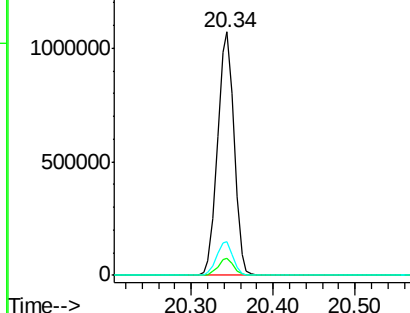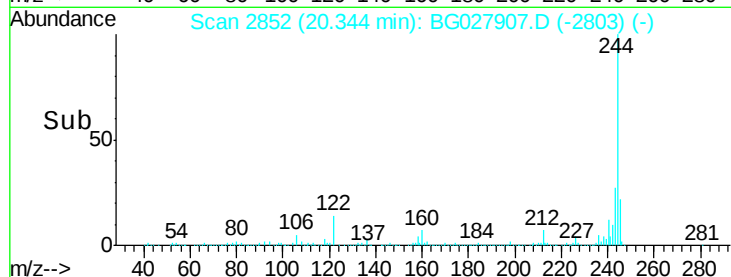

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.67 min Scan# 3758

Delta R.T. -0.03 min

Lab File: BG027907.D

Acq: 11 Jul 2017 4:02


Tgt Ion:264 Resp: 276764

Ion Ratio Lower Upper

264 100

260 24.2 21.8 32.8

265 21.9 18.2 27.4

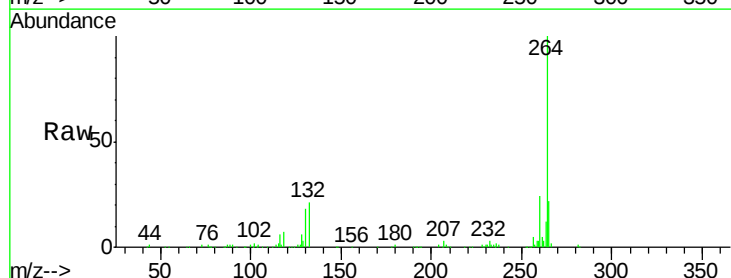

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

