


Data Path : Z:\HPCHEM1\BNA_G\Data\BG071017\
 Data File : BG027889.D
 Acq On : 10 Jul 2017 16:11
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 11 15:32:18 2017

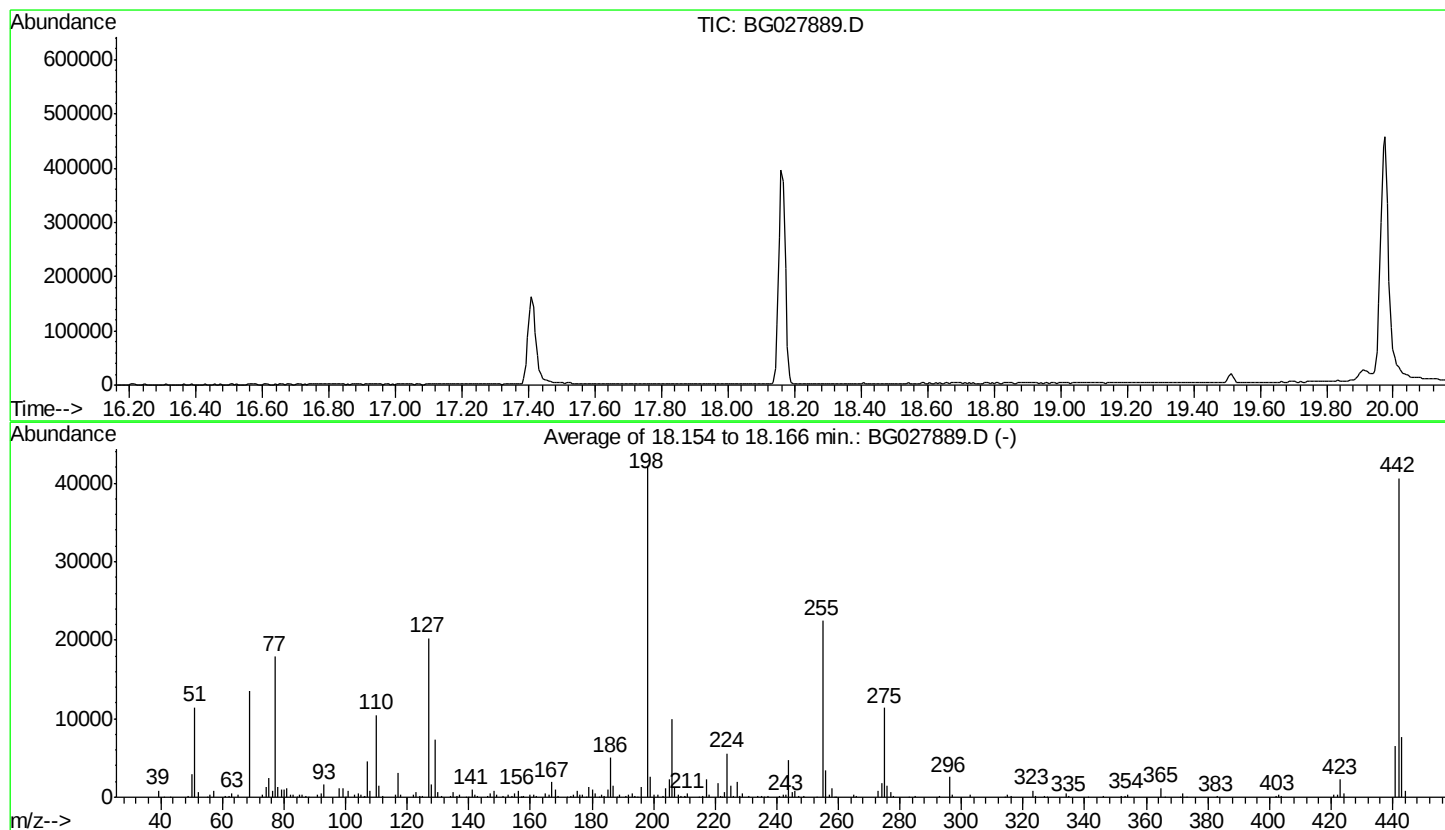

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	11442	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.2	13577	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.0	20250	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42226	PASS
199	198	5	9	6.4	2695	PASS
275	198	10	60	26.9	11347	PASS
365	198	1	100	2.9	1208	PASS
441	442	0.01	24	16.2	6581	PASS
442	198	50	100	96.2	40640	PASS
443	442	15	24	19.0	7736	PASS