
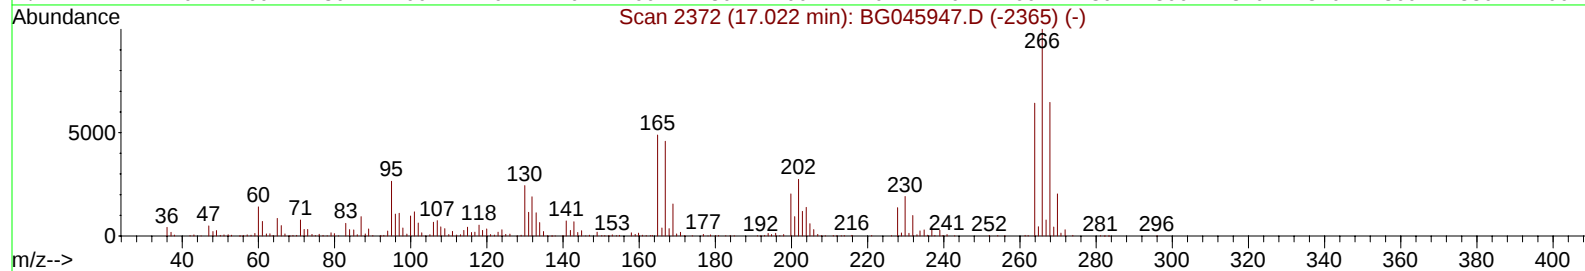
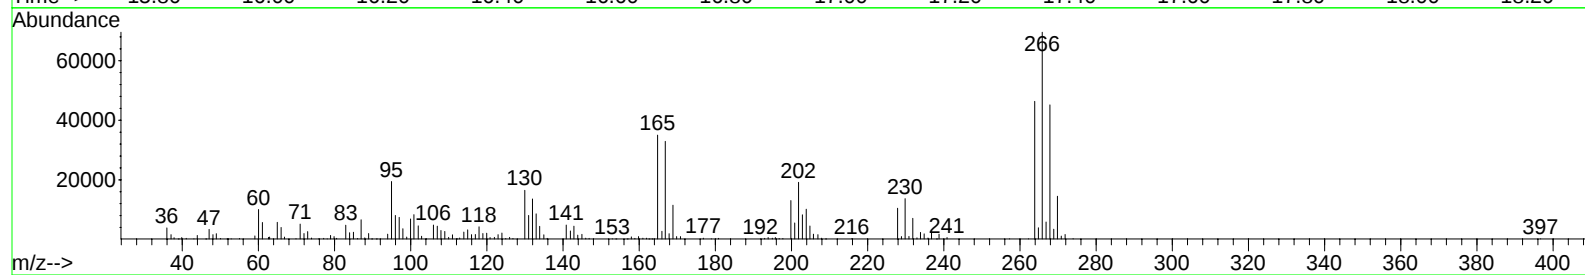


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071020\
 Data File : BG045997.D
 Acq On : 10 Jul 2020 8:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 18:08:15 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG070620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 07 09:58:42 2020
 Response via : Initial Calibration

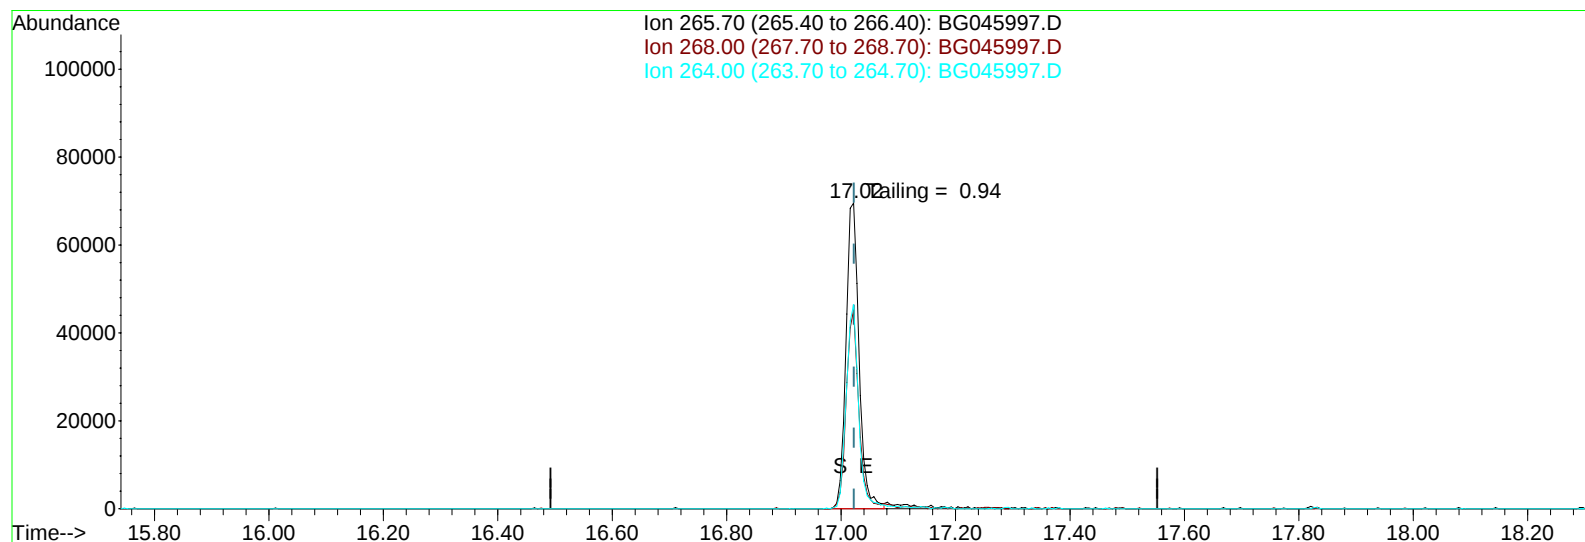

TIC: BG045997.D

(70) Pentachlorophenol (C)




17.022min (-0.000) 223125.46ng

response 111227

Ion	Exp%	Act%
265.70	100	100
268.00	64.80	64.97
264.00	64.20	66.67
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071020\
 Data File : BG045997.D
 Acq On : 10 Jul 2020 8:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 18:08:15 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG070620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 07 09:58:42 2020
 Response via : Initial Calibration

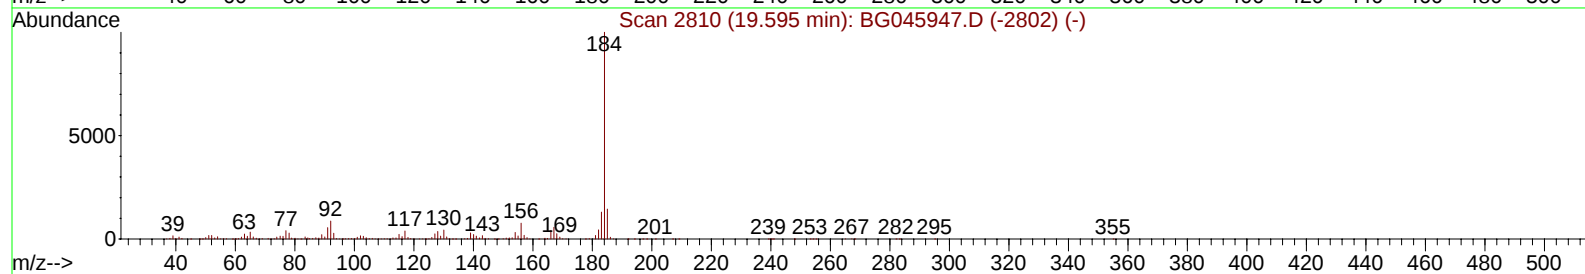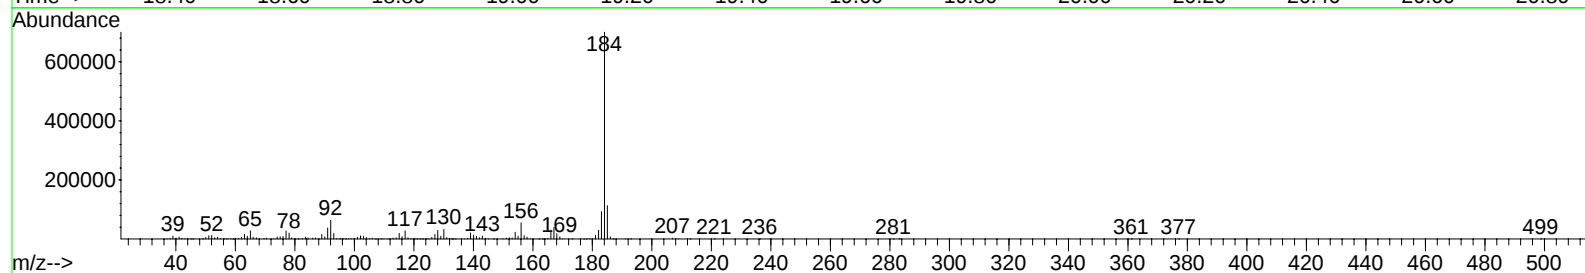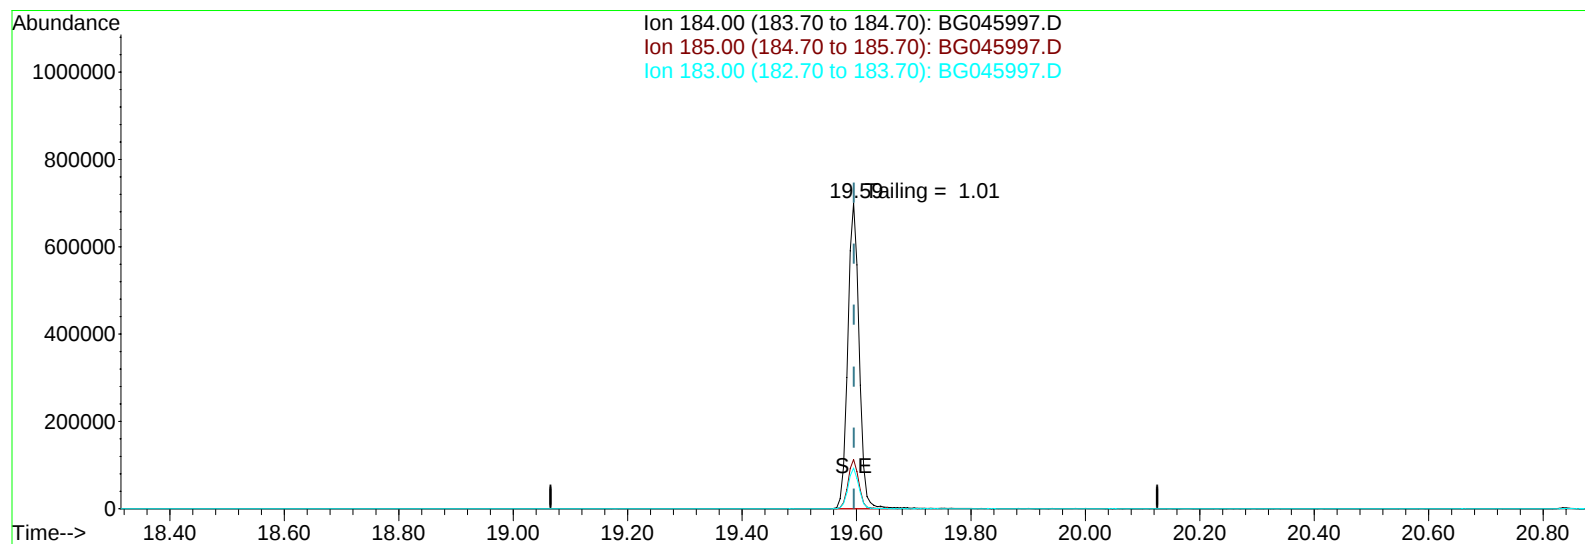

TIC: BG045997.D

(77) Benzidine

19.595min (-0.000) 11509.59ng

response 967192

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	16.13
183.00	13.00	13.30
0.00	0.00	0.00