

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071020\  
 Data File : BG046003.D  
 Acq On : 10 Jul 2020 12:20  
 Operator : CG/JU  
 Sample : PB130070BL  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB130070BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG070620.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.141       | 5             | 9           | 20           | rBV3     | 78387          | 203065        | 2.05%           | 0.400%        |
| 2         | 4.222       | 187           | 193         | 202          | rVB      | 167058         | 271592        | 2.75%           | 0.535%        |
| 3         | 5.585       | 417           | 425         | 439          | rBV      | 2863427        | 4666630       | 47.22%          | 9.188%        |
| 4         | 7.165       | 685           | 694         | 702          | rBV      | 2920249        | 5043981       | 51.04%          | 9.931%        |
| 5         | 8.005       | 829           | 837         | 845          | rVB      | 634547         | 1035037       | 10.47%          | 2.038%        |
| 6         | 8.328       | 884           | 892         | 900          | rBV      | 2406301        | 4191114       | 42.41%          | 8.252%        |
| 7         | 9.156       | 1025          | 1033        | 1044         | rBV      | 1894625        | 3405142       | 34.46%          | 6.704%        |
| 8         | 10.801      | 1305          | 1313        | 1320         | rBV      | 823301         | 1451905       | 14.69%          | 2.859%        |
| 9         | 13.257      | 1722          | 1731        | 1738         | rBV      | 4624957        | 7239682       | 73.26%          | 14.254%       |
| 10        | 14.625      | 1957          | 1964        | 1974         | rVB2     | 1235007        | 1916411       | 19.39%          | 3.773%        |
| 11        | 16.112      | 2209          | 2217        | 2237         | rBV      | 3274416        | 4825263       | 48.83%          | 9.500%        |
| 12        | 17.369      | 2424          | 2431        | 2439         | rBV      | 1429418        | 2166937       | 21.93%          | 4.266%        |
| 13        | 19.983      | 2870          | 2876        | 2882         | rBV      | 6996402        | 9882450       | 100.00%         | 19.458%       |
| 14        | 21.622      | 3148          | 3155        | 3167         | rVB2     | 1430995        | 2283260       | 23.10%          | 4.496%        |
| 15        | 24.776      | 3682          | 3692        | 3704         | rVB2     | 788113         | 2207329       | 22.34%          | 4.346%        |


Sum of corrected areas: 50789798

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071020\  
Data File : BG046003.D  
Acq On : 10 Jul 2020 12:20  
Operator : CG/JU  
Sample : PB130070BL  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB130070BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG070620.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

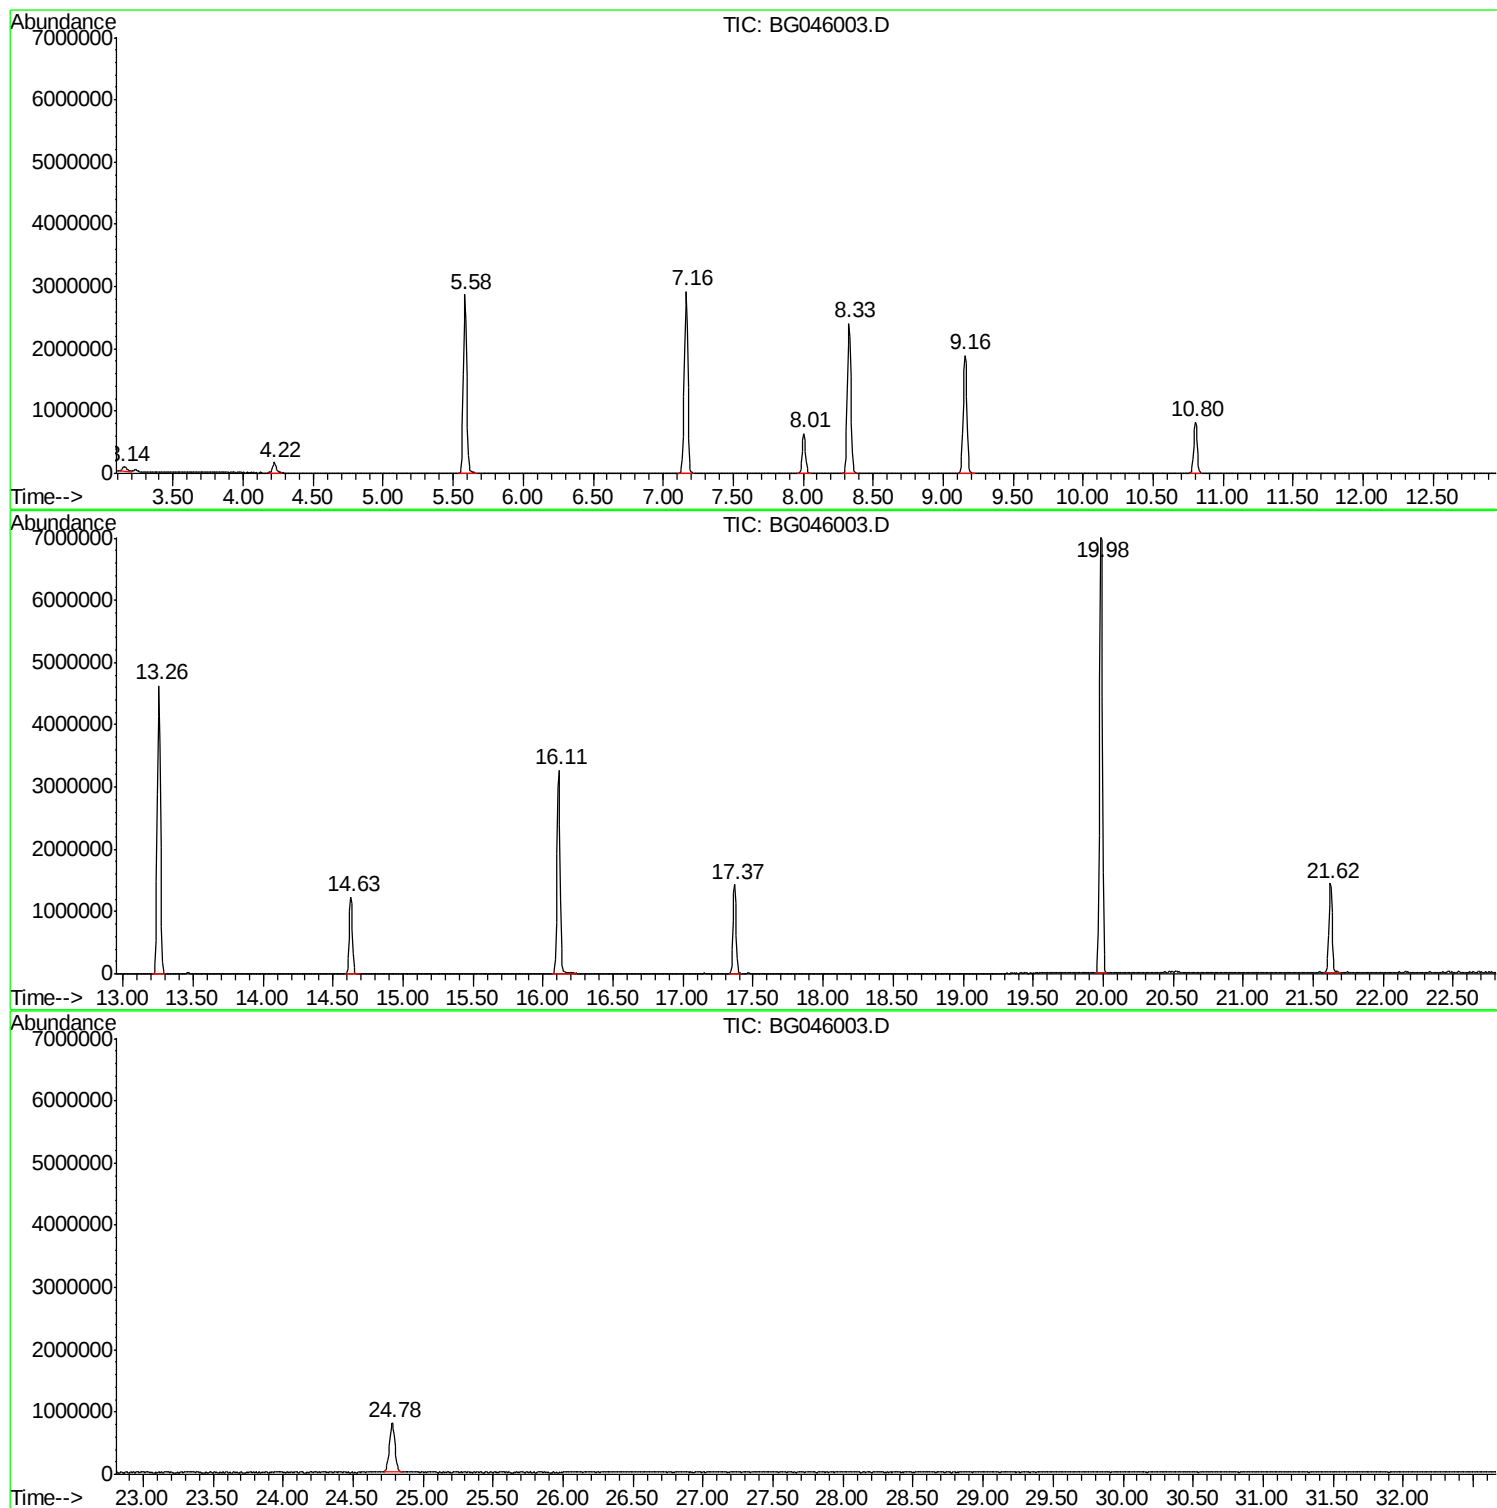

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG071020\  
Data File : BG046003.D  
Acq On : 10 Jul 2020 12:20  
Operator : CG/JU  
Sample : PB130070BL  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB130070BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG070620.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG071020\  
Data File : BG046003.D  
Acq On : 10 Jul 2020 12:20  
Operator : CG/JU  
Sample : PB130070BL  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB130070BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG070620.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |