


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071020\
 Data File : BG045997.D
 Acq On : 10 Jul 2020 8:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG070620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 07 09:58:42 2020

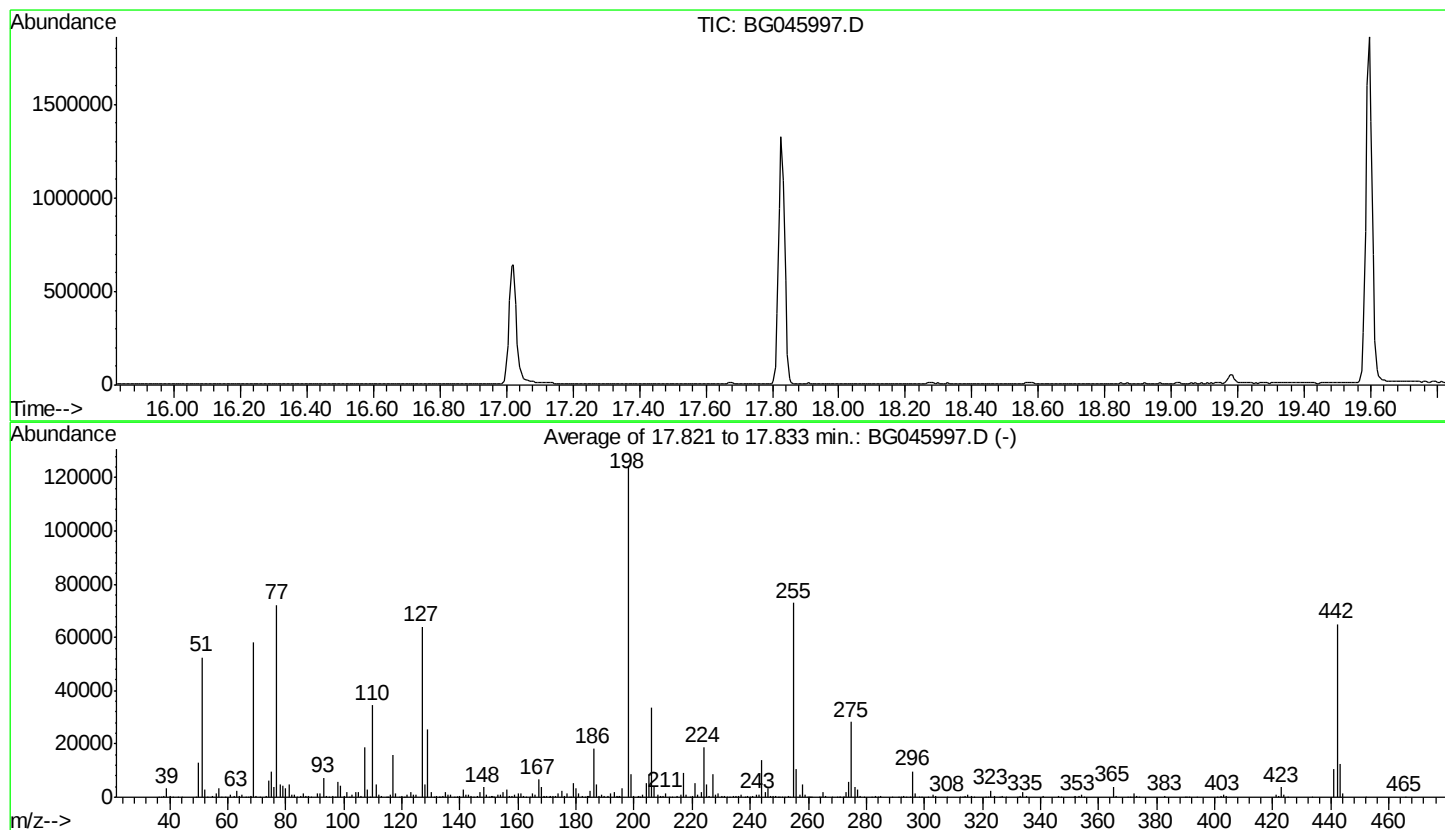

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	52485	PASS
68	69	0.00	2	0.8	463	PASS
69	198	0.00	100	46.8	58221	PASS
70	69	0.00	2	0.5	287	PASS
127	198	10	80	51.5	64154	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	124514	PASS
199	198	5	9	7.1	8836	PASS
275	198	10	60	22.7	28309	PASS
365	198	1	100	3.1	3876	PASS
441	198	0.01	100	8.6	10669	PASS
442	198	50	100	52.1	64898	PASS
443	442	15	24	19.1	12415	PASS