




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071024\
 Data File : BG061996.D
 Acq On : 10 Jul 2024 13:12
 Operator : MA/JU
 Sample : P3109-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 H0HC4

Manual IntegrationsAPPROVED

Quant Time: Jul 10 13:45:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 02:38:46 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2024
 Supervised By :mohammad ahmed 07/11/2024

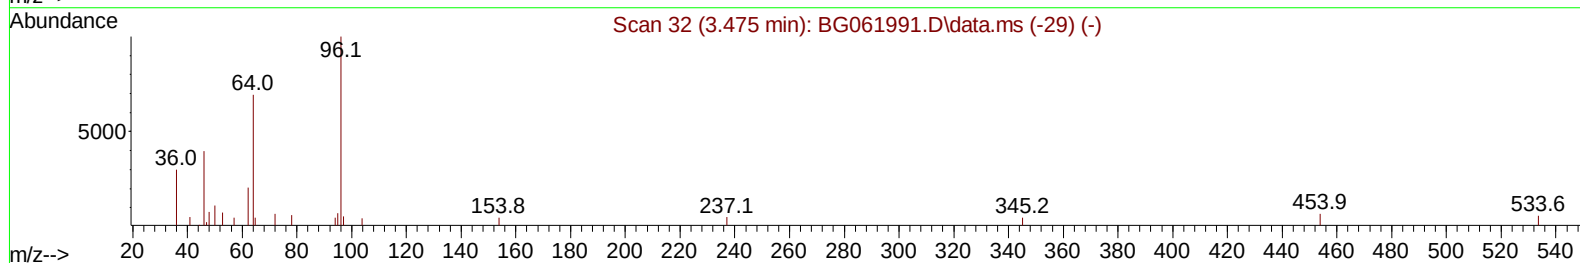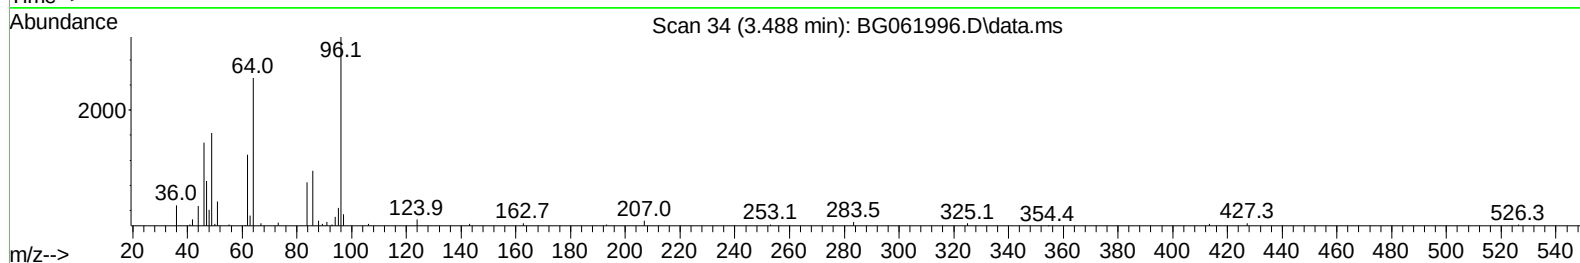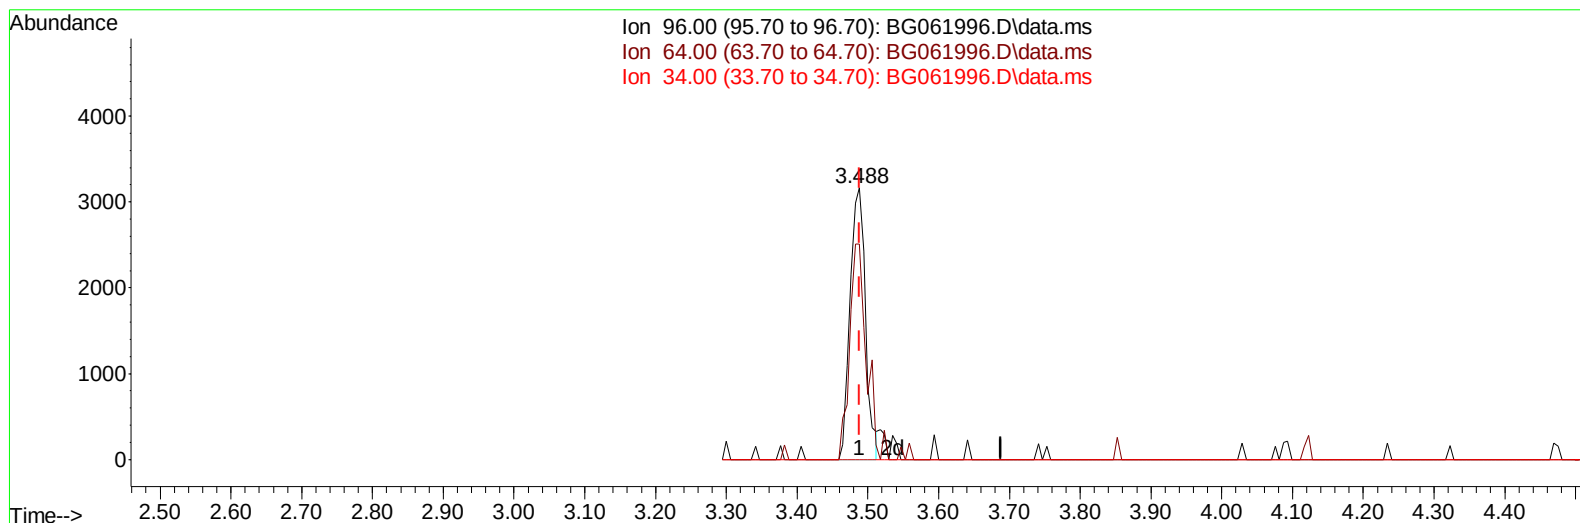

TIC: BG061996.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.488min (+ 0.000) 3.82 ng/uL

response 4780

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	104.80	79.32#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071024\
Data File : BG061996.D
Acq On : 10 Jul 2024 13:12
Operator : MA/JU
Sample : P3109-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
H0HC4

Manual IntegrationsAPPROVED

Quant Time: Jul 10 13:45:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 02:38:46 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2024
Supervised By :mohammad ahmed 07/11/2024

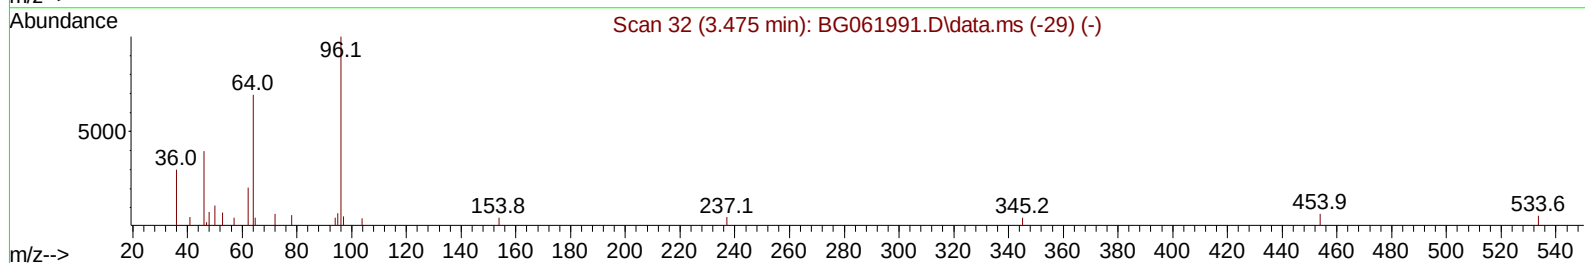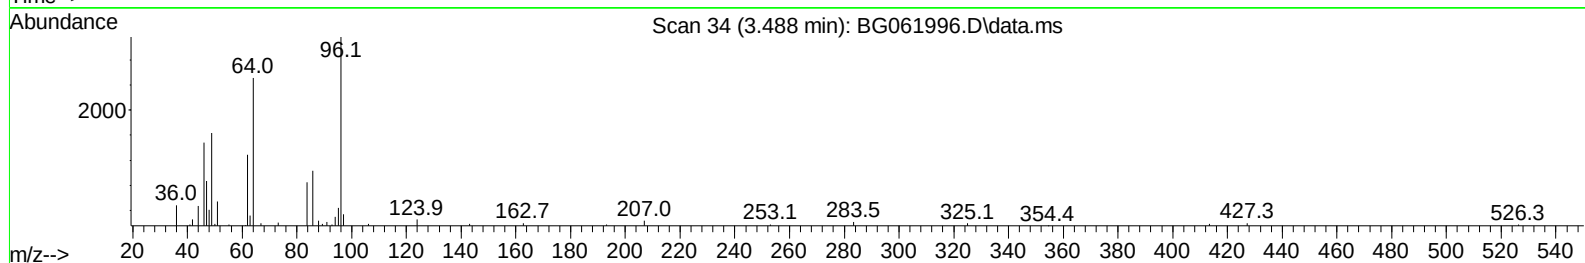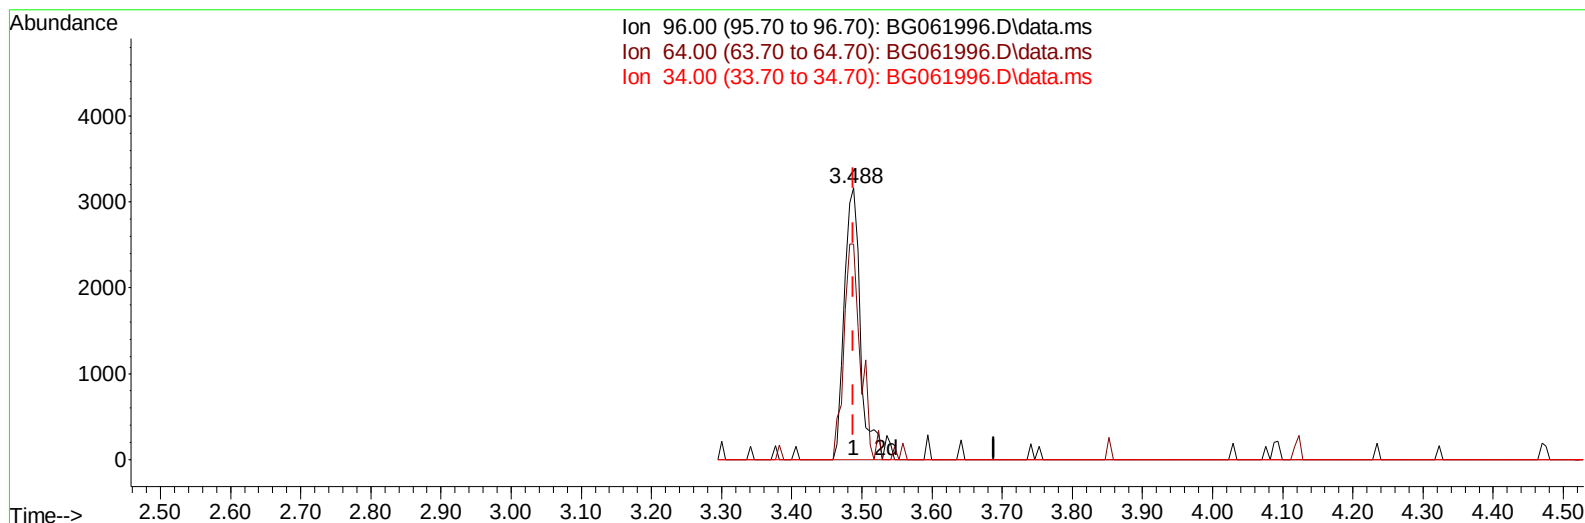

TIC: BG061996.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.488min (+ 0.000) 4.00 ng/uL m

response 5006

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	104.80	79.32#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071024\
 Data File : BG061996.D
 Acq On : 10 Jul 2024 13:12
 Operator : MA/JU
 Sample : P3109-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 H0HC4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/11/2024
 Supervised By :mohammad ahmed 07/11/2024

Quant Time: Jul 11 00:52:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 03 02:38:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.095	152	46997	20.000	ng/ul	0.00
20) Naphthalene-d8	10.909	136	240870	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.716	164	175784	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.460	188	396276	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.720	240	352888	20.000	ng/ul	# 0.00
88) Perylene-d12	24.957	264	425793	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.488	96	5006m	4.003	ng/uL	0.00
4) Pyridine-d5	3.905	84	28385	7.381	ng/ul	0.00
7) Phenol-d5	7.248	99	55803	10.850	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.419	67	80938	24.850	ng/ul	0.00
11) 2-Chlorophenol-d4	7.625	132	96630	27.390	ng/ul	0.00
15) 4-Methylphenol-d8	8.800	113	92591	22.865	ng/ul	0.00
21) Nitrobenzene-d5	9.270	128	54097	29.531	ng/ul	0.00
24) 2-Nitrophenol-d4	9.986	143	68157	32.580	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.527	165	127696	31.646	ng/ul	0.00
31) 4-Chloroaniline-d4	11.038	131	113874	19.438	ng/ul	0.00
46) Dimethylphthalate-d6	14.117	166	458206	31.706	ng/ul	0.00
49) Acenaphthylene-d8	14.417	160	479411	31.725	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	26988	11.694	ng/ul	0.00
60) Fluorene-d10	15.709	176	395142	32.479	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.821	200	74148	35.628	ng/ul	0.00
73) Anthracene-d10	17.560	188	641856	34.692	ng/ul	0.00
81) Pyrene-d10	19.840	212	733327	35.330	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.734	264	786037	37.223	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071024\
Data File : BG061996.D
Acq On : 10 Jul 2024 13:12
Operator : MA/JU
Sample : P3109-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
H0HC4

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:52:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 03 02:38:46 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2024
Supervised By :mohammad ahmed 07/11/2024

