

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071024\
 Data File : BG061992.D
 Acq On : 10 Jul 2024 10:25
 Operator : MA/JU
 Sample : PB161916BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK916

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061992.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.482	30	33	38	rVB6	11283	15926	0.91%	0.080%
2	3.699	67	70	73	rBV4	2158	3216	0.18%	0.016%
3	3.758	79	80	83	rVB2	3420	3069	0.17%	0.015%
4	3.840	92	94	98	rVB4	2534	3055	0.17%	0.015%
5	3.899	100	104	114	rBV	182411	309797	17.66%	1.555%
6	4.234	159	161	167	rBV	3207	6163	0.35%	0.031%
7	4.392	184	188	190	rBV3	2170	3070	0.17%	0.015%
8	4.768	247	252	258	rVB5	3289	7170	0.41%	0.036%
9	4.815	258	260	263	rBV3	3048	3452	0.20%	0.017%
10	5.985	456	459	462	rBV3	2309	3149	0.18%	0.016%
11	6.161	486	489	491	rBV3	2610	2954	0.17%	0.015%
12	6.531	551	552	557	rVB	2493	2809	0.16%	0.014%
13	6.760	589	591	596	rVB	2963	2888	0.16%	0.014%
14	6.848	603	606	608	rBV2	2099	2671	0.15%	0.013%
15	6.925	614	619	620	rBV	2183	2933	0.17%	0.015%
16	7.142	653	656	659	rBV	2175	2951	0.17%	0.015%
17	7.201	664	666	667	rVV	4386	2481	0.14%	0.012%
18	7.248	667	674	684	rVB	263801	480403	27.38%	2.411%
19	7.412	695	702	709	rBV	172389	291544	16.62%	1.463%
20	7.624	731	738	748	rBV	236284	421950	24.05%	2.117%
21	8.094	811	818	828	rBV	235651	404731	23.07%	2.031%
22	8.159	828	829	835	rVB3	2072	2706	0.15%	0.014%
23	8.229	839	841	845	rBV	2411	3078	0.18%	0.015%
24	8.429	873	875	879	rVB	2557	2926	0.17%	0.015%
25	8.793	929	937	949	rBV2	340027	577479	32.91%	2.898%
26	9.093	986	988	991	rBV	2894	2753	0.16%	0.014%
27	9.257	1008	1016	1025	rBV	257010	471076	26.85%	2.364%
28	9.663	1083	1085	1088	rBV	1713	2588	0.15%	0.013%
29	9.980	1132	1139	1149	rVB2	259380	453917	25.87%	2.278%
30	10.409	1209	1212	1216	rVV	1658	2479	0.14%	0.012%
31	10.520	1222	1231	1238	rBV	351162	638350	36.38%	3.203%
32	10.597	1243	1244	1248	rVB	2941	2462	0.14%	0.012%
33	10.691	1257	1260	1262	rVB	2427	2891	0.16%	0.015%
34	10.720	1262	1265	1267	rBV	2779	2874	0.16%	0.014%
35	10.908	1288	1297	1308	rVB	364971	670309	38.21%	3.364%
36	11.037	1312	1319	1329	rVV2	303441	551986	31.46%	2.770%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071024\
Data File : BG061992.D
Acq On : 10 Jul 2024 10:25
Operator : MA/JU
Sample : PB161916BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK916

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Title : SVOA CALIBRATION

37	11.114	1331	1332	1338	rBV2	2833	4162	0.24%	0.021%
38	11.296	1358	1363	1366	rBV	1384	3012	0.17%	0.015%
39	11.889	1462	1464	1469	rBV	1615	2710	0.15%	0.014%
40	12.312	1533	1536	1538	rBV	2329	2820	0.16%	0.014%
41	12.483	1560	1565	1570	rVB2	7149	12505	0.71%	0.063%
42	12.583	1579	1582	1585	rBV	2245	2695	0.15%	0.014%
43	12.947	1641	1644	1648	rVB	2381	3160	0.18%	0.016%
44	13.382	1714	1718	1722	rBV	2152	3077	0.18%	0.015%
45	13.517	1738	1741	1745	rBV	2201	3926	0.22%	0.020%
46	13.640	1758	1762	1763	rBV2	2447	2644	0.15%	0.013%
47	14.116	1835	1843	1851	rVB	678722	966931	55.11%	4.852%
48	14.410	1886	1893	1902	rVB	663358	1076981	61.39%	5.404%
49	14.716	1939	1945	1952	rVB	642038	978037	55.75%	4.908%
50	14.815	1961	1962	1965	rVB	3372	2589	0.15%	0.013%
51	14.904	1971	1977	1986	rBV	332803	543252	30.96%	2.726%
52	15.609	2095	2097	2102	rVB2	2562	3708	0.21%	0.019%
53	15.703	2105	2113	2120	rVB	893717	1349784	76.93%	6.773%
54	15.814	2126	2132	2143	rBV	364107	533914	30.43%	2.679%
55	15.932	2150	2152	2153	rBV2	2784	2579	0.15%	0.013%
56	16.043	2169	2171	2173	rBV	2559	2994	0.17%	0.015%
57	16.167	2189	2192	2193	rBV2	3889	3174	0.18%	0.016%
58	16.226	2200	2202	2206	rVB	3852	2673	0.15%	0.013%
59	16.267	2206	2209	2212	rBV3	2825	3212	0.18%	0.016%
60	16.290	2212	2213	2219	rVB2	2865	3789	0.22%	0.019%
61	16.484	2244	2246	2253	rVB4	3248	5057	0.29%	0.025%
62	16.637	2270	2272	2277	rVB	2609	3120	0.18%	0.016%
63	16.948	2323	2325	2327	rBV	3517	2697	0.15%	0.014%
64	16.972	2327	2329	2333	rVB	3243	3665	0.21%	0.018%
65	17.459	2405	2412	2419	rVB	770329	1215335	69.27%	6.098%
66	17.553	2421	2428	2437	rVB	969437	1470695	83.83%	7.380%
67	17.653	2444	2445	2448	rBV	2395	2473	0.14%	0.012%
68	17.794	2467	2469	2472	rVB	2584	2632	0.15%	0.013%
69	17.935	2491	2493	2497	rBV	2025	2907	0.17%	0.015%
70	18.112	2520	2523	2528	rVB3	7381	7922	0.45%	0.040%
71	18.264	2547	2549	2553	rVB	2980	3318	0.19%	0.017%
72	18.358	2563	2565	2568	rVB2	2892	2789	0.16%	0.014%
73	18.399	2568	2572	2576	rBV4	5442	8283	0.47%	0.042%
74	18.670	2614	2618	2619	rBV2	3137	3131	0.18%	0.016%
75	18.711	2623	2625	2628	rBV	2473	3356	0.19%	0.017%
76	18.875	2651	2653	2655	rBV	2903	2760	0.16%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071024\
 Data File : BG061992.D
 Acq On : 10 Jul 2024 10:25
 Operator : MA/JU
 Sample : PB161916BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK916

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

77	19.005	2673	2675	2676	rVB2	4054	2626	0.15%	0.013%
78	19.022	2676	2678	2680	rBV2	3583	3469	0.20%	0.017%
79	19.234	2712	2714	2718	rBV	3041	3869	0.22%	0.019%
80	19.398	2739	2742	2748	rVB4	14820	20629	1.18%	0.104%
81	19.469	2750	2754	2757	rVV2	10375	13160	0.75%	0.066%
82	19.539	2762	2766	2767	rBV	2780	3340	0.19%	0.017%
83	19.627	2780	2781	2783	rBV2	3245	2555	0.15%	0.013%
84	19.739	2797	2800	2803	rVB3	9693	10628	0.61%	0.053%
85	19.833	2808	2816	2826	rBV	1133987	1648200	93.94%	8.271%
86	20.344	2901	2903	2906	rBV3	4824	4782	0.27%	0.024%
87	20.385	2909	2910	2913	rBV	7196	4799	0.27%	0.024%
88	20.415	2913	2915	2917	rBV3	4351	4717	0.27%	0.024%
89	20.503	2928	2930	2931	rVB2	5239	3063	0.17%	0.015%
90	21.713	3129	3136	3142	rBV2	759994	1262974	71.99%	6.338%
91	22.313	3236	3238	3239	rBV	6006	3042	0.17%	0.015%
92	22.506	3269	3271	3276	rVB5	10456	14798	0.84%	0.074%
93	23.917	3509	3511	3514	rVB4	9520	6485	0.37%	0.033%
94	24.727	3639	3649	3660	rBV2	626354	1754456	100.00%	8.804%
95	24.956	3676	3688	3701	rBV	513376	1492584	85.07%	7.490%
96	28.294	4253	4256	4257	rBV2	8469	7869	0.45%	0.039%
97	29.504	4460	4462	4466	rBV5	8325	7673	0.44%	0.039%
98	30.826	4685	4687	4689	rBV3	6908	7104	0.40%	0.036%
99	31.073	4726	4729	4732	rBV5	13085	22960	1.31%	0.115%
100	32.401	4953	4955	4956	rBV2	7039	3994	0.23%	0.020%




Sum of corrected areas: 19928500

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071024\
Data File : BG061992.D
Acq On : 10 Jul 2024 10:25
Operator : MA/JU
Sample : PB161916BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK916

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

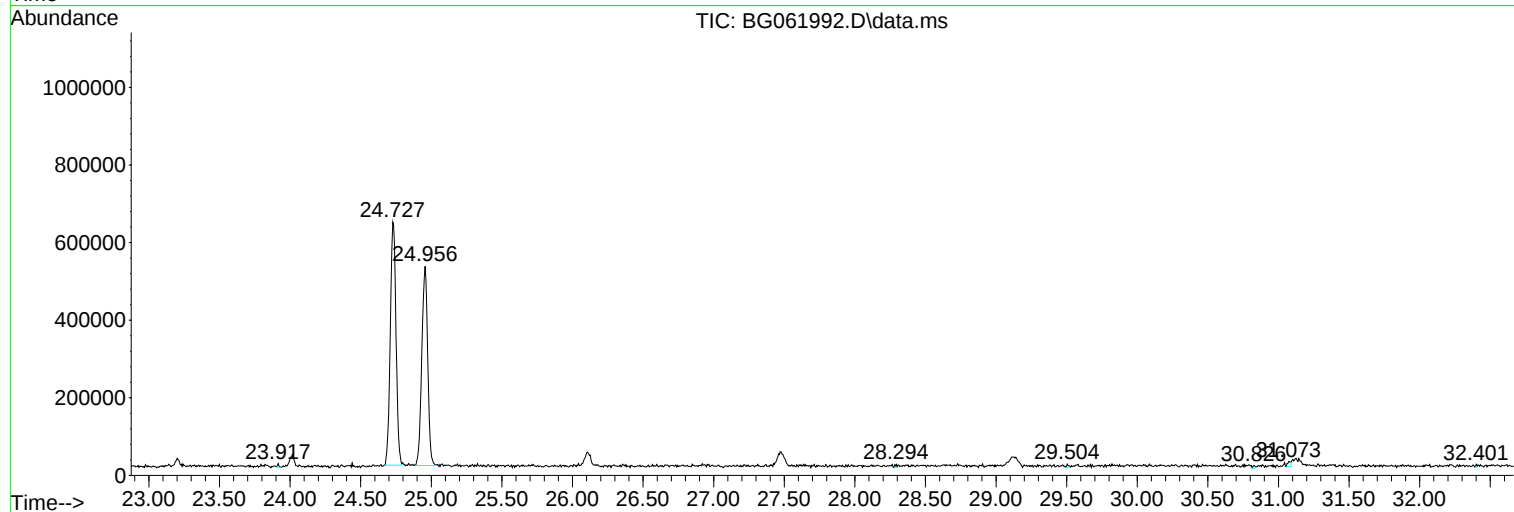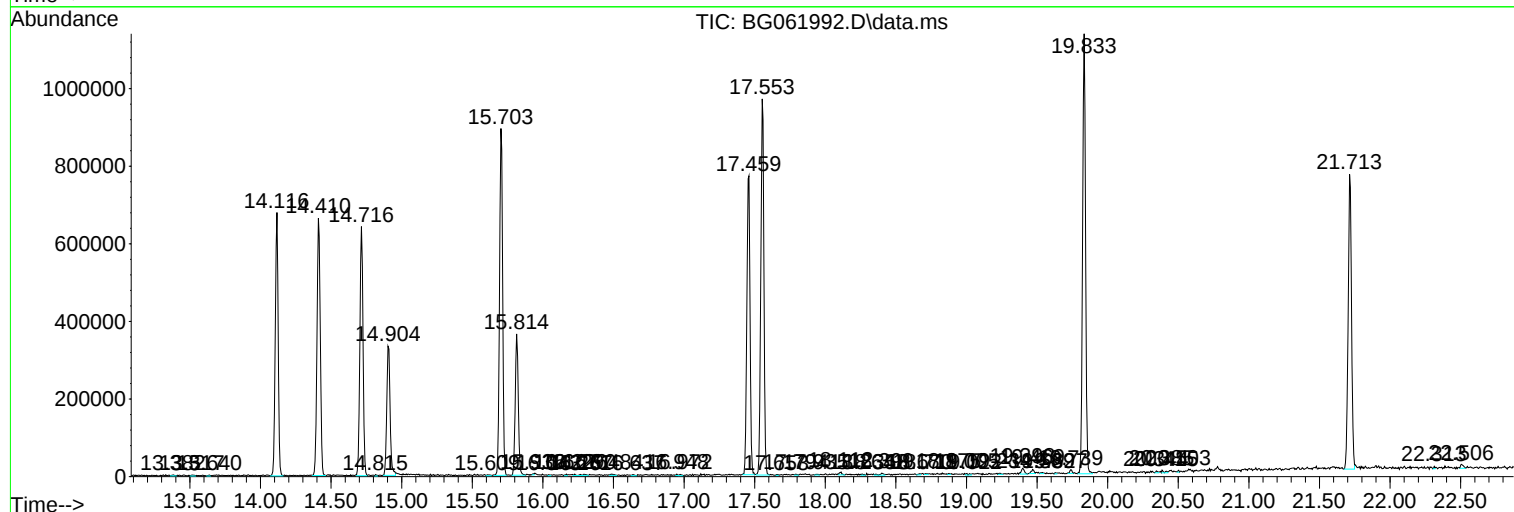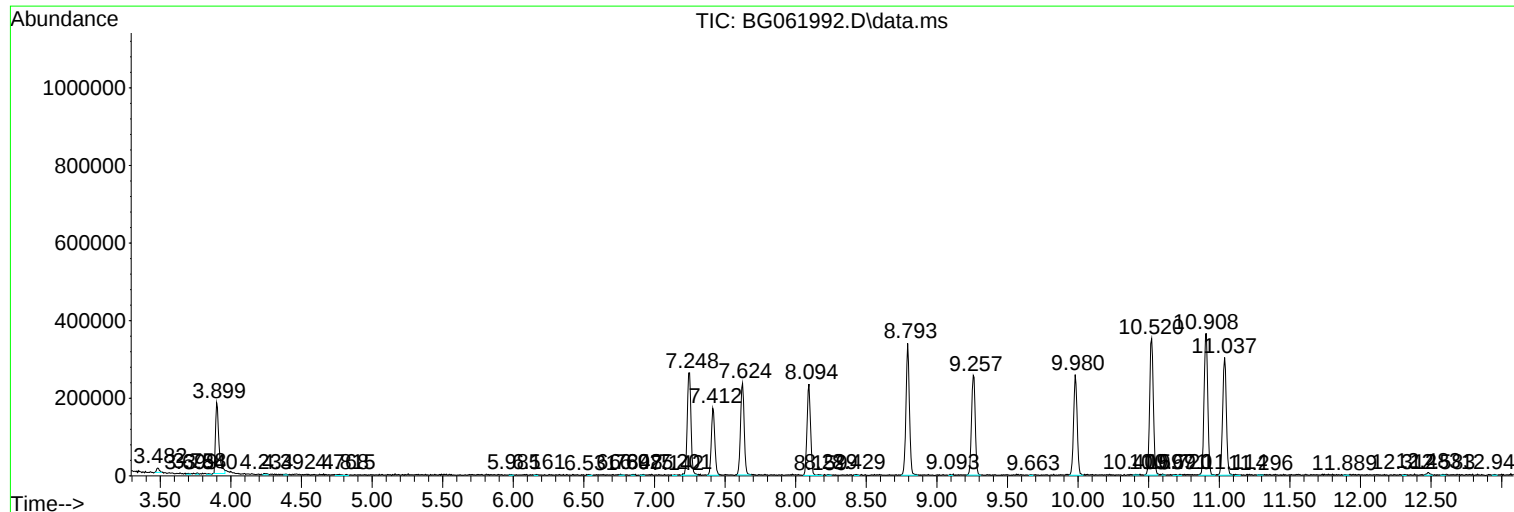

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071024\
Data File : BG061992.D
Acq On : 10 Jul 2024 10:25
Operator : MA/JU
Sample : PB161916BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK916

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071024\
Data File : BG061992.D
Acq On : 10 Jul 2024 10:25
Operator : MA/JU
Sample : PB161916BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK916

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------