
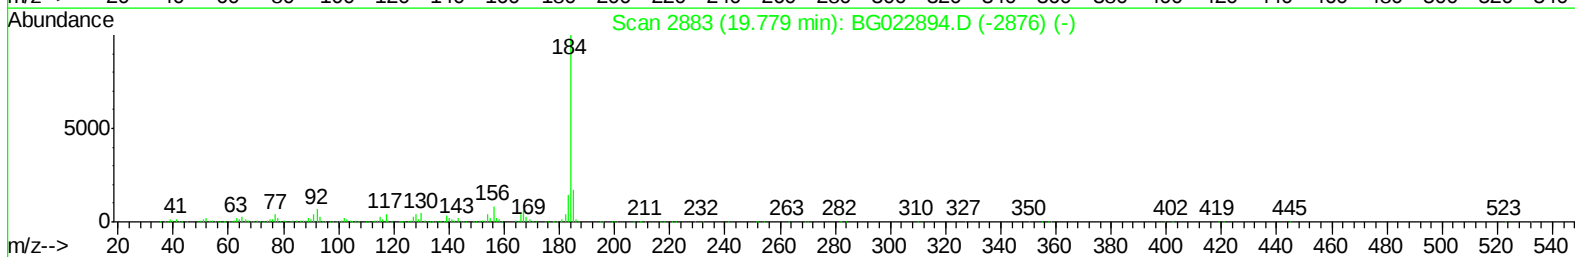
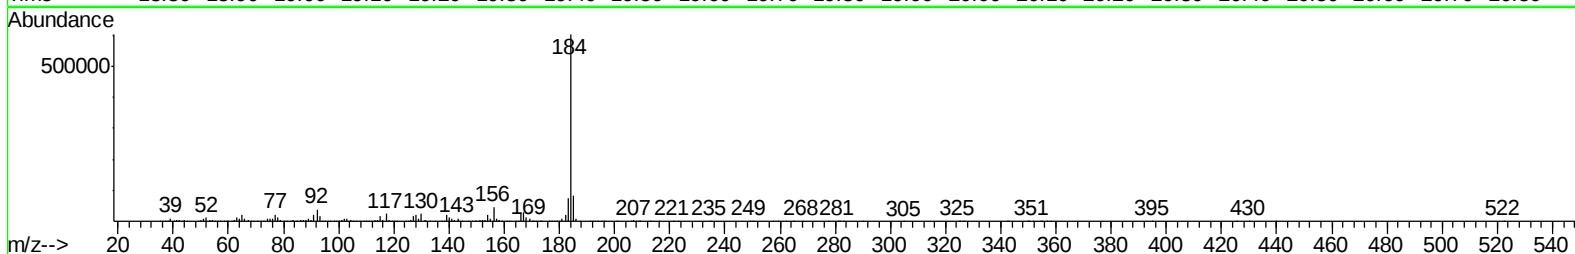


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071116\
Data File : BG023000.D
Acq On : 11 Jul 2016 9:38
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 07:43:23 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 16:51:07 2016
Response via : Initial Calibration

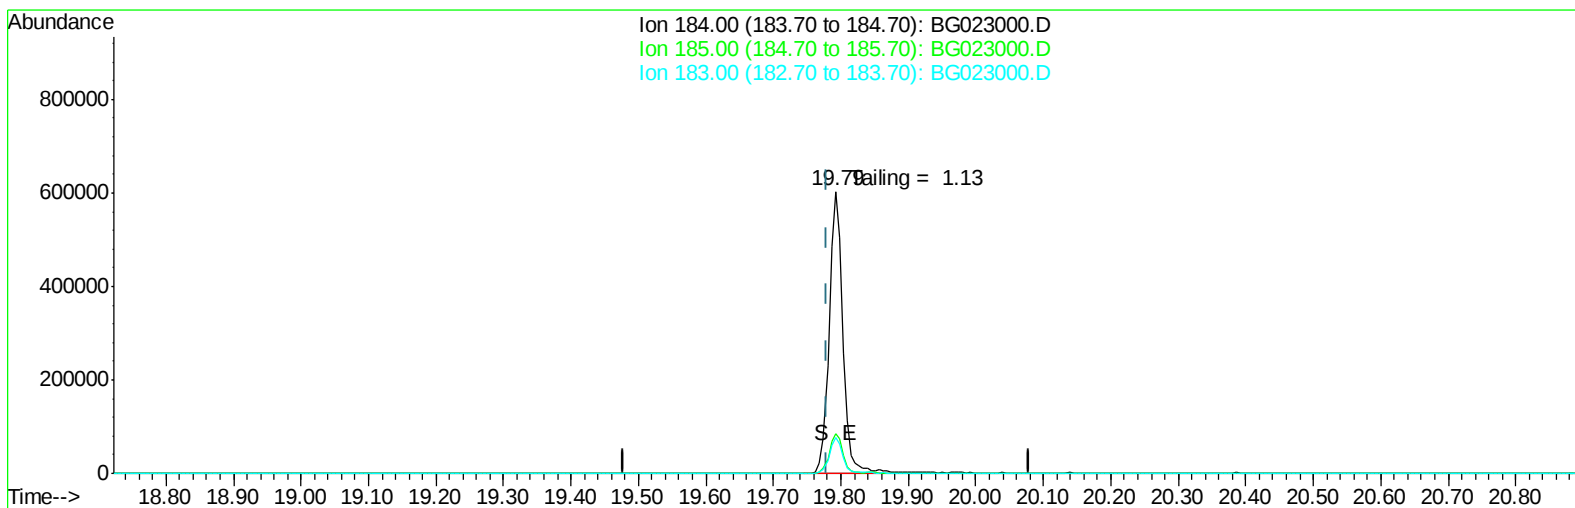

TIC: BG023000.D

(76) Benzidine




19.792min (+0.013) 175612.87ng

response 855878

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.01
183.00	13.40	12.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071116\
Data File : BG023000.D
Acq On : 11 Jul 2016 9:38
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 07:43:23 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 16:51:07 2016
Response via : Initial Calibration

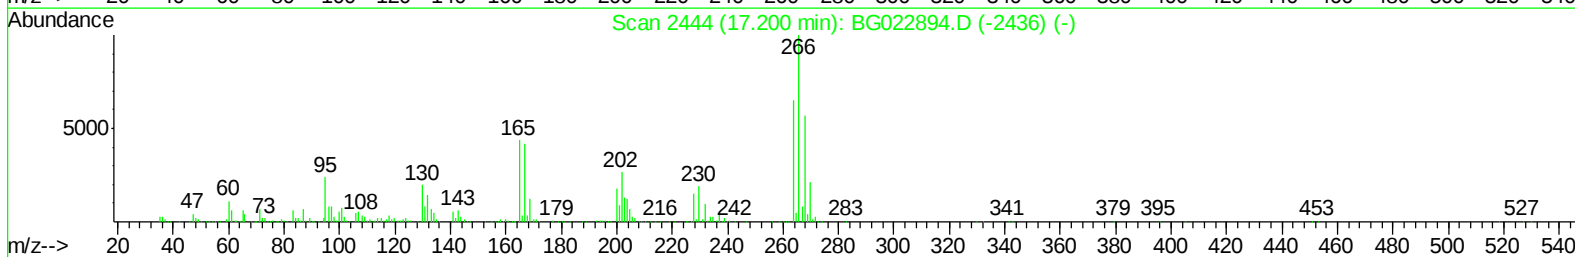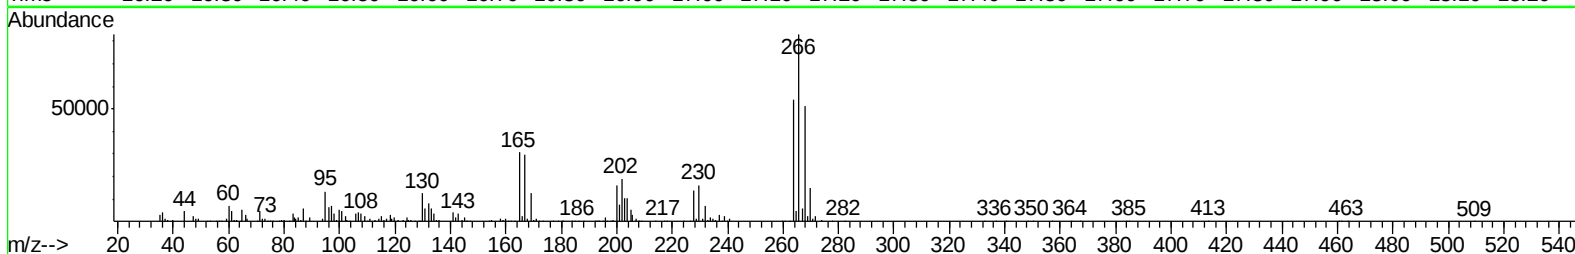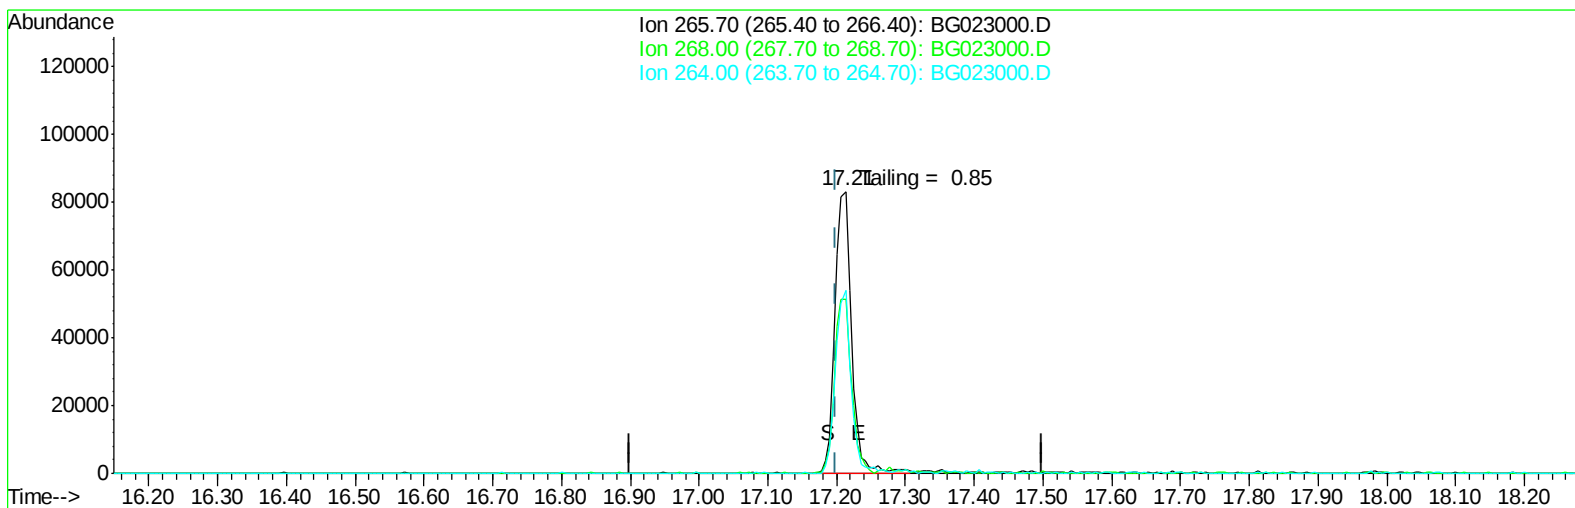

TIC: BG023000.D

(69) Pentachlorophenol (C)

17.213min (+0.013) 23435.79ng

response 136760

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	62.03
264.00	63.20	64.95
0.00	0.00	0.00