
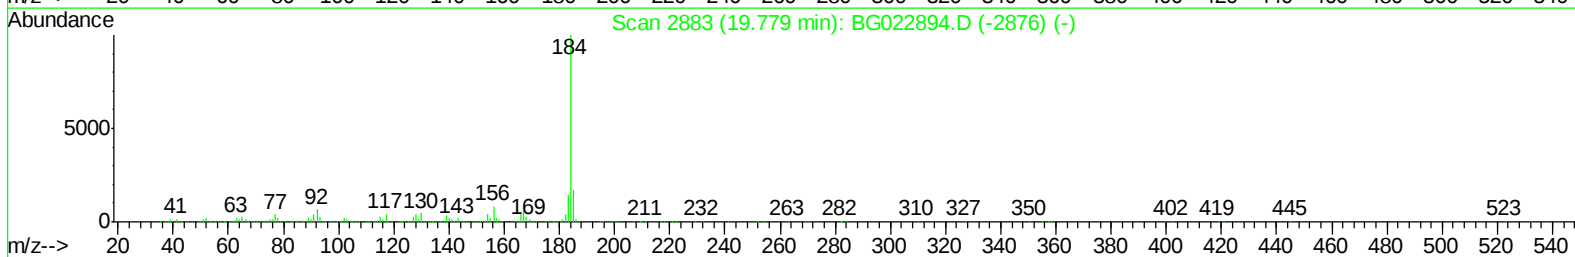
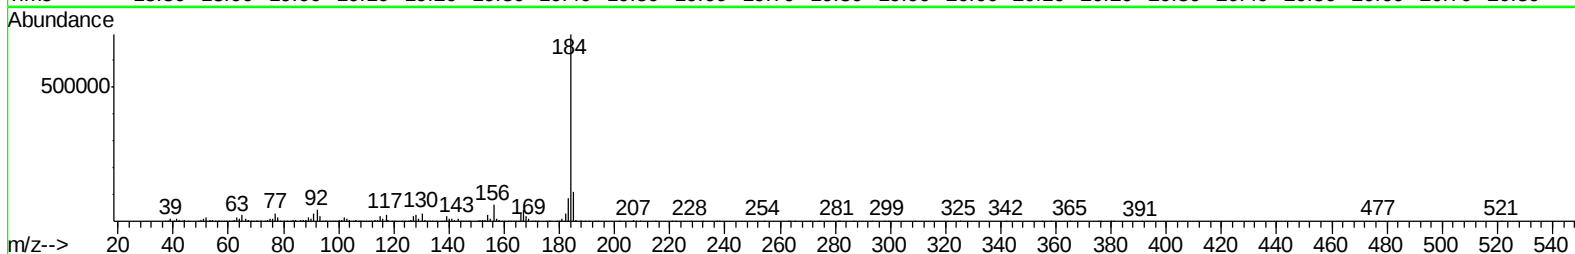


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071116\
Data File : BG023003.D
Acq On : 11 Jul 2016 15:54
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 07:44:19 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 16:51:07 2016
Response via : Initial Calibration

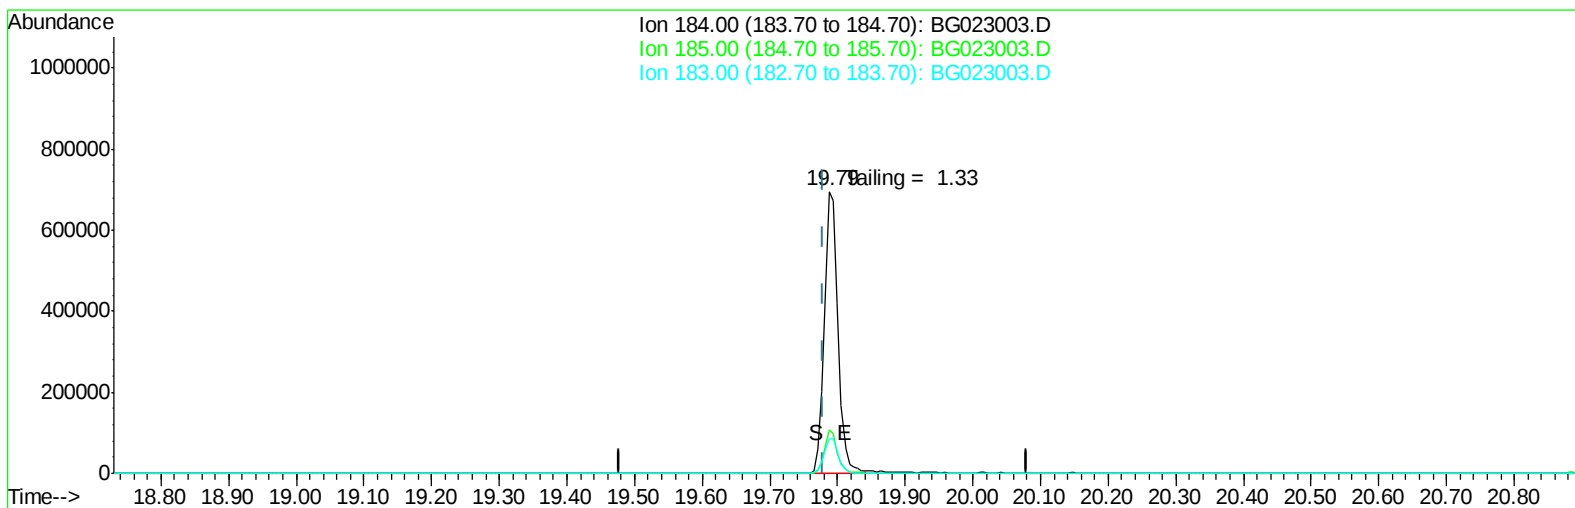

TIC: BG023003.D

(76) Benzidine




19.788min (+0.009) 59080.01ng

response 1002695

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.56
183.00	13.40	12.24
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071116\
Data File : BG023003.D
Acq On : 11 Jul 2016 15:54
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 07:44:19 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 16:51:07 2016
Response via : Initial Calibration

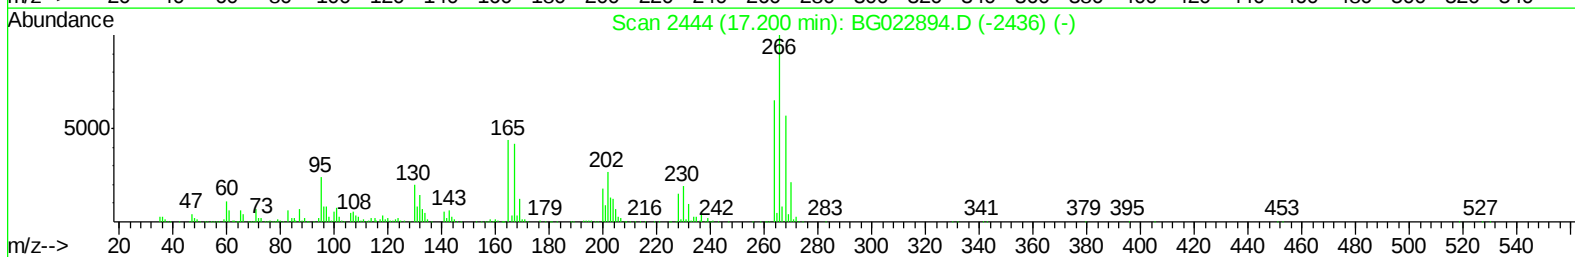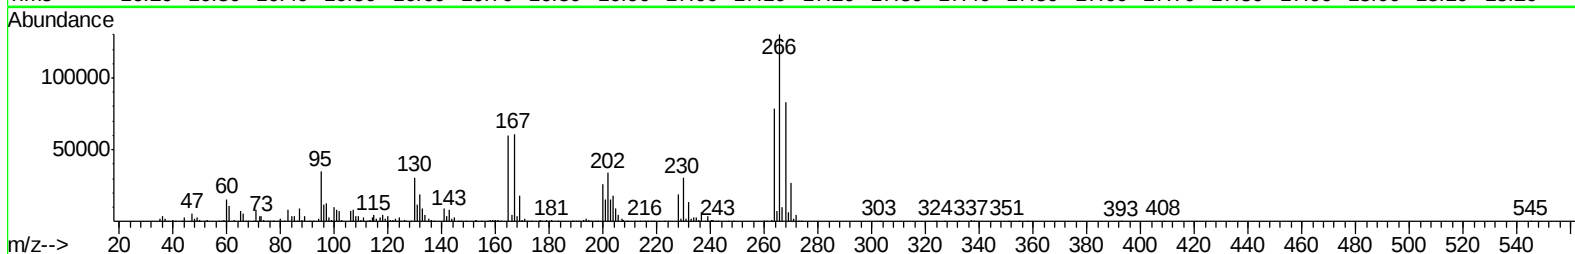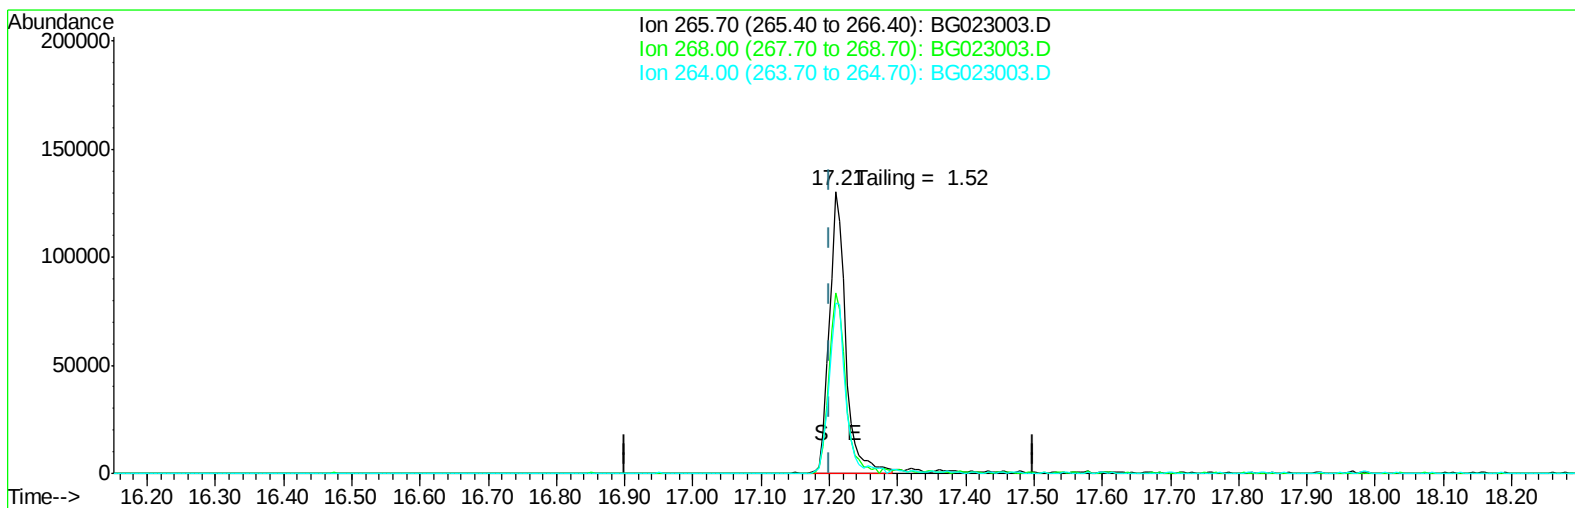

TIC: BG023003.D

(69) Pentachlorophenol (C)

17.209min (+0.009) 13703.42ng

response 218182

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	63.97
264.00	63.20	60.45
0.00	0.00	0.00