


Data Path : Z:\HPCHEM1\BNA G\DATA\BG071116\
Data File : BG023000.D
Acq On : 11 Jul 2016 9:38
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 07 16:51:07 2016

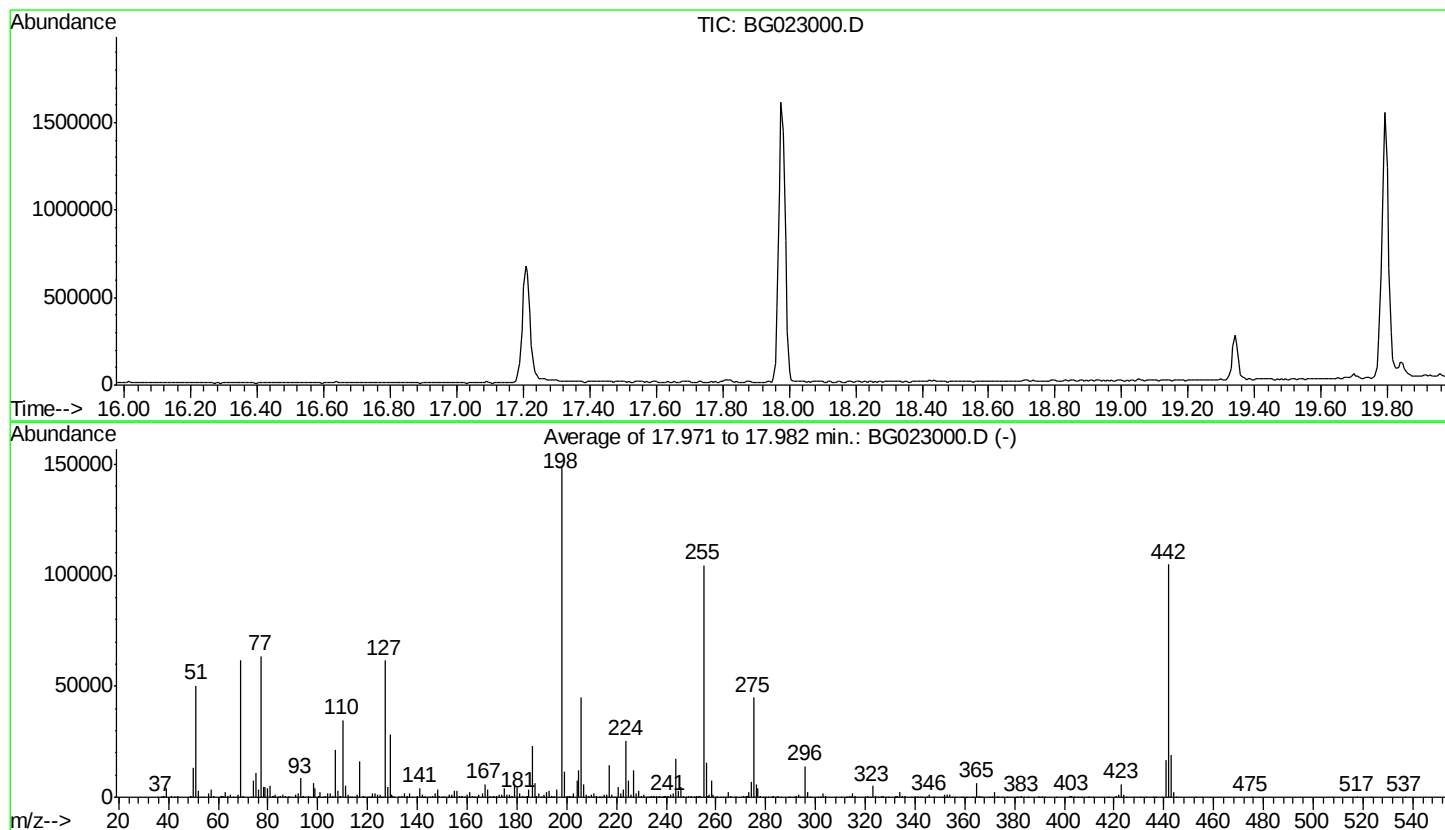

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	50304	PASS
68	69	0.00	2	1.5	921	PASS
69	198	0.00	100	41.5	61927	PASS
70	69	0.00	2	0.9	585	PASS
127	198	10	80	41.2	61445	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	149296	PASS
199	198	5	9	7.7	11461	PASS
275	198	10	60	29.9	44698	PASS
365	198	1	100	4.3	6446	PASS
441	442	0.01	24	16.1	16859	PASS
442	198	50	100	70.1	104672	PASS
443	442	15	24	18.3	19147	PASS