


Data Path : Z:\HPCHEM1\BNA G\DATA\BG071116\
 Data File : BG023003.D
 Acq On : 11 Jul 2016 15:54
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 07 16:51:07 2016

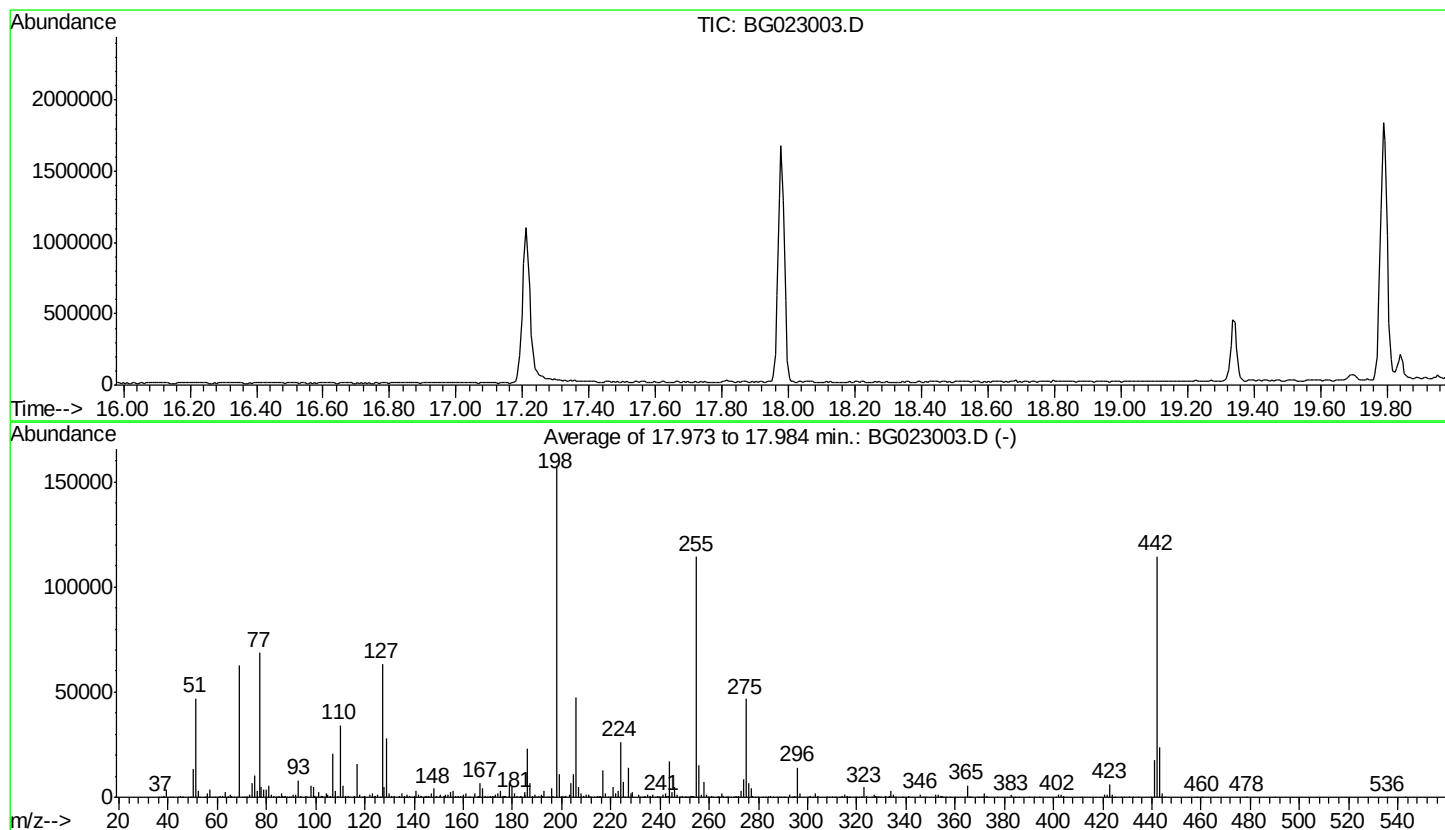

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	47080	PASS
68	69	0.00	2	0.4	234	PASS
69	198	0.00	100	39.9	62904	PASS
70	69	0.00	2	0.4	238	PASS
127	198	10	80	40.3	63490	PASS
197	198	0.00	2	0.3	460	PASS
198	198	100	100	100.0	157717	PASS
199	198	5	9	7.0	11007	PASS
275	198	10	60	29.6	46746	PASS
365	198	1	100	3.6	5691	PASS
441	442	0.01	24	15.7	17953	PASS
442	198	50	100	72.6	114498	PASS
443	442	15	24	20.6	23533	PASS