

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071124\
 Data File : BG062009.D
 Acq On : 11 Jul 2024 14:13
 Operator : MA/JU
 Sample : PB161824BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK824

Quant Time: Jul 12 00:06:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 11 12:11:32 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.041	152	35558	20.000	ng/ul	0.00
20) Naphthalene-d8	10.850	136	187050	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.669	164	151557	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.413	188	353295	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.673	240	332815	20.000	ng/ul	0.00
88) Perylene-d12	24.875	264	373811	20.000	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.441	96	5563	5.879	ng/uL	0.00
4) Pyridine-d5	3.858	84	71259	24.492	ng/ul	0.00
7) Phenol-d5	7.195	99	96788	24.873	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.360	67	61376	24.907	ng/ul	0.00
11) 2-Chlorophenol-d4	7.566	132	75459	28.270	ng/ul	0.00
15) 4-Methylphenol-d8	8.741	113	78179	25.517	ng/ul	0.00
21) Nitrobenzene-d5	9.205	128	35491	24.948	ng/ul	0.00
24) 2-Nitrophenol-d4	9.927	143	45140	27.786	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.468	165	89201	28.467	ng/ul	0.00
31) 4-Chloroaniline-d4	10.985	131	91082	20.021	ng/ul	0.00
46) Dimethylphthalate-d6	14.070	166	345810	27.754	ng/ul	0.00
49) Acenaphthylene-d8	14.363	160	351522	26.980	ng/ul	0.00
54) 4-Nitrophenol-d4	14.869	143	50708	25.484	ng/ul	0.00
60) Fluorene-d10	15.662	176	294233	28.051	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.774	200	38456	20.726	ng/ul	0.00
73) Anthracene-d10	17.513	188	443887	26.911	ng/ul	0.00
81) Pyrene-d10	19.798	212	529416	27.044	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.663	264	540155	29.136	ng/ul	0.00
Target Compounds						
17) N-Nitroso-di-n-propyla...	8.746	70	2855	1.008	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071124\
Data File : BG062009.D
Acq On : 11 Jul 2024 14:13
Operator : MA/JU
Sample : PB161824BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK824


Quant Time: Jul 12 00:06:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 11 12:11:32 2024
Response via : Initial Calibration

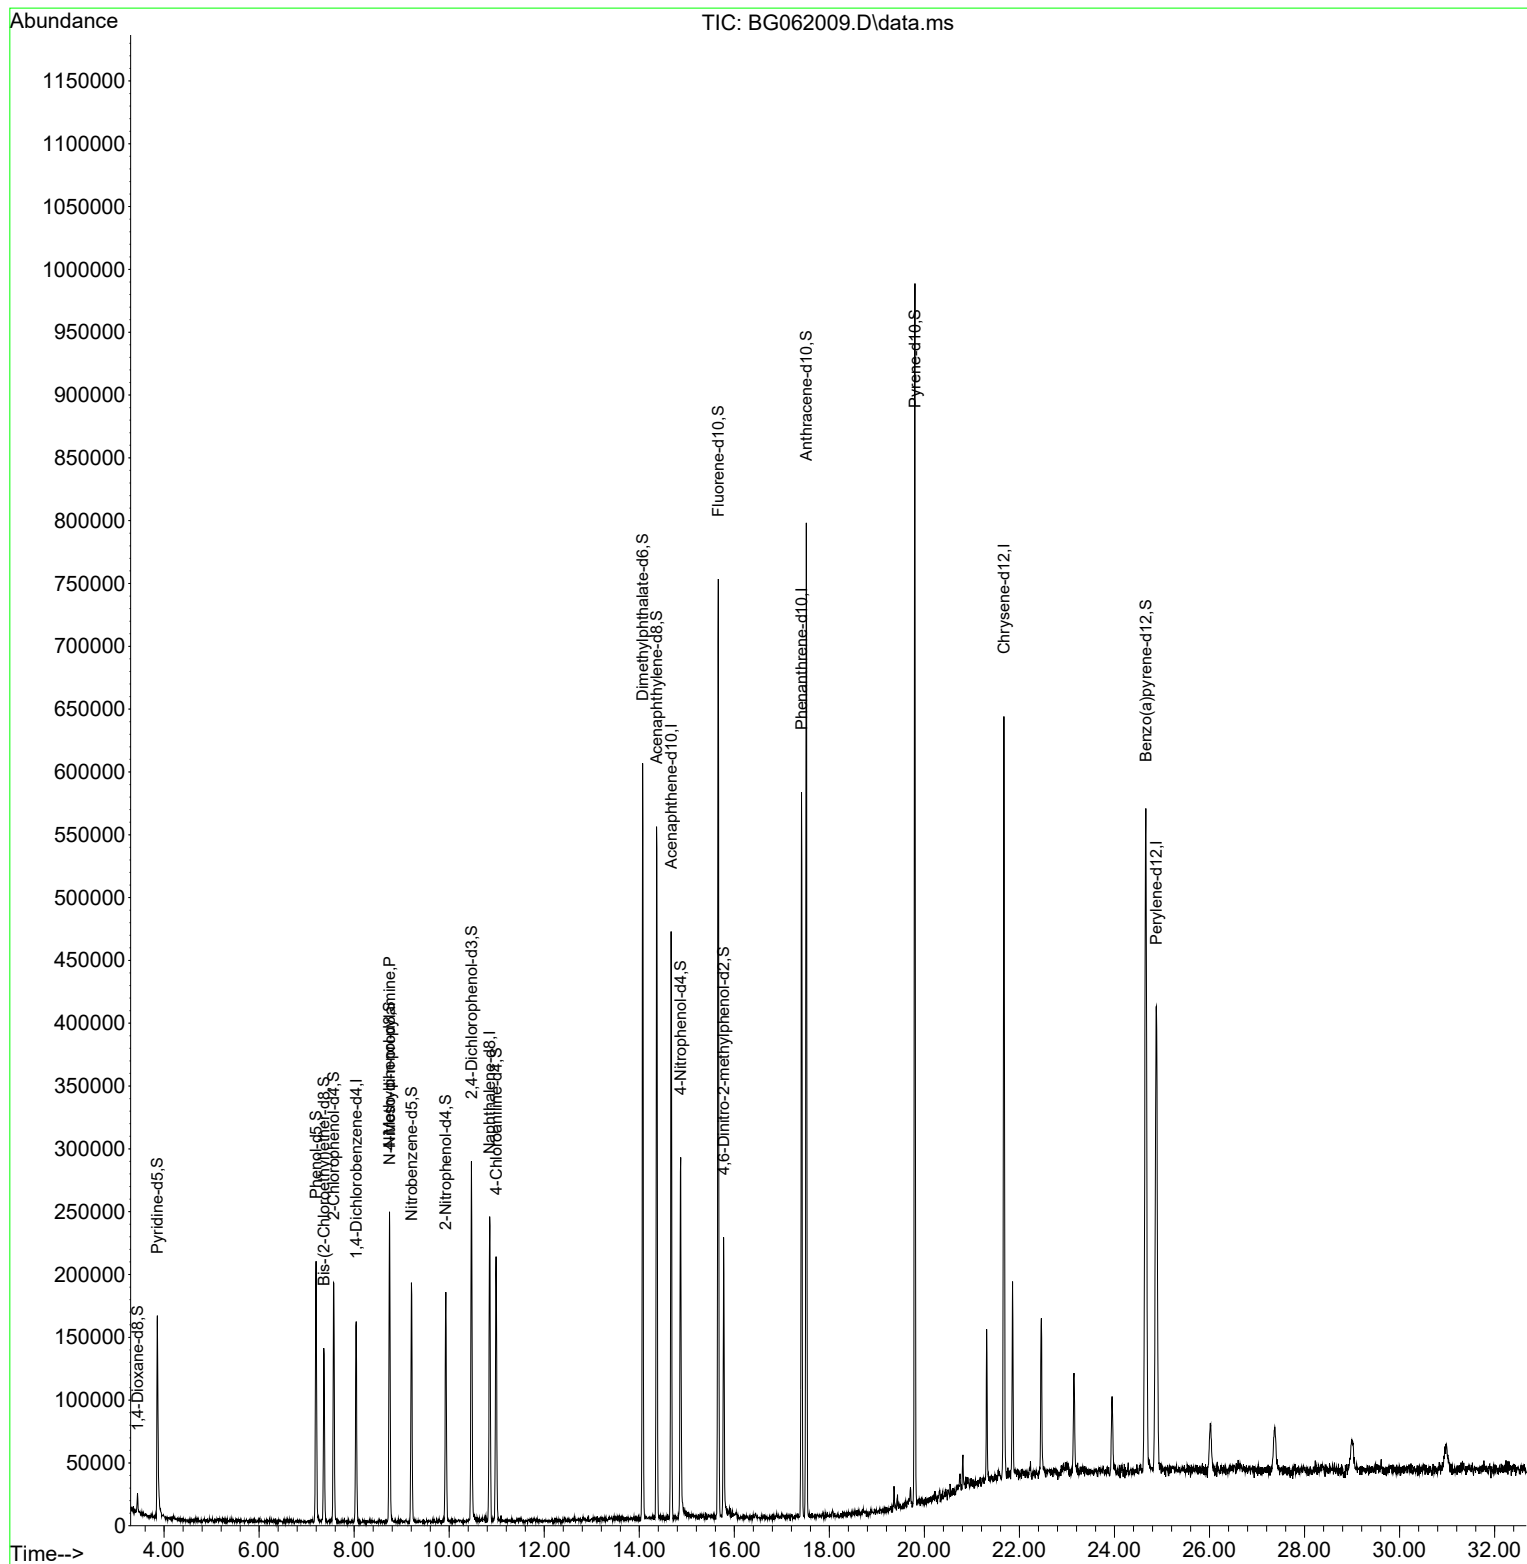

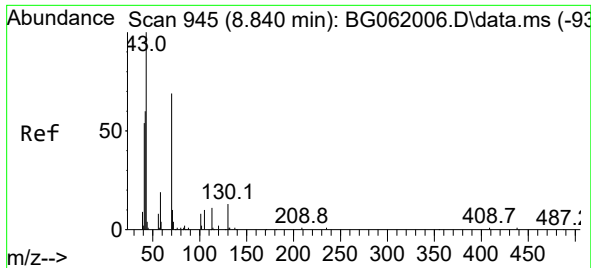

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.008 ng/ul
 RT: 8.746 min Scan# 91
 Delta R.T. -0.093 min
 Lab File: BG062009.D
 Acq: 11 Jul 2024 14:13

Instrument :
 BNA_G
 ClientSampleId :
 SBLK824

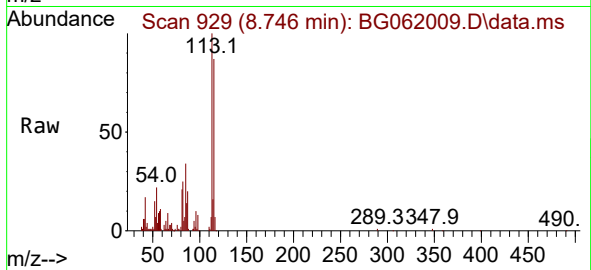

Tgt Ion: 70 Resp: 2855

Ion	Ratio	Lower	Upper
70	100		
42	436.7	64.7	97.1#
101	0.0	7.3	10.9#
130	0.0	17.0	25.6#

