




Data Path : C:\Users\eUser\Desktop\krunal\
Data File : BG062026.D
Acq On : 12 Jul 2024 1:56
Operator : MA/JU
Sample : PB161949BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK949

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/15/2024

Quant Time: Jul 12 10:05:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 11 12:11:32 2024
Response via : Initial Calibration

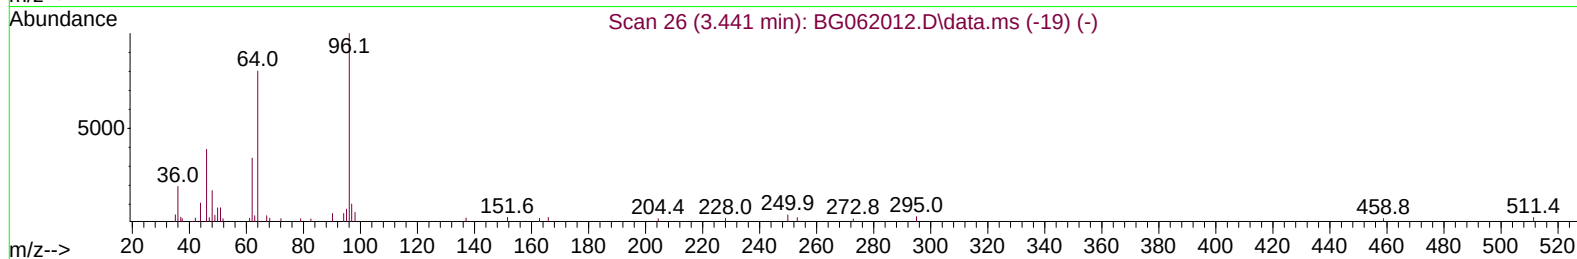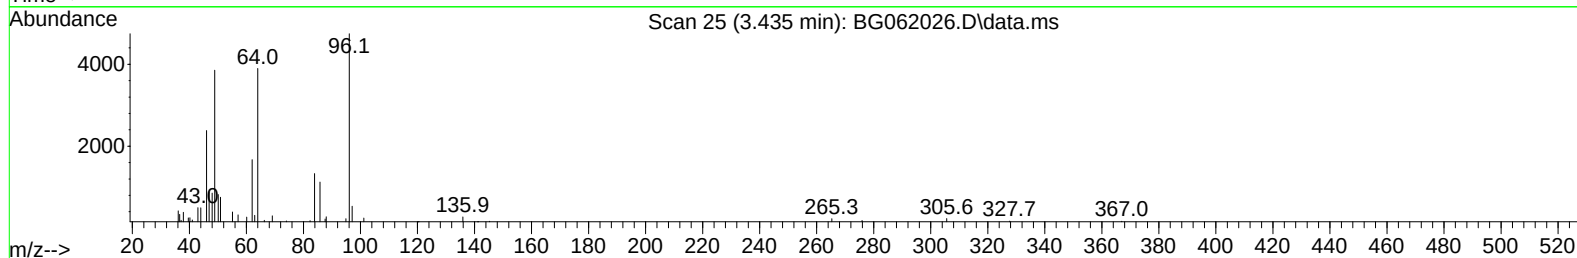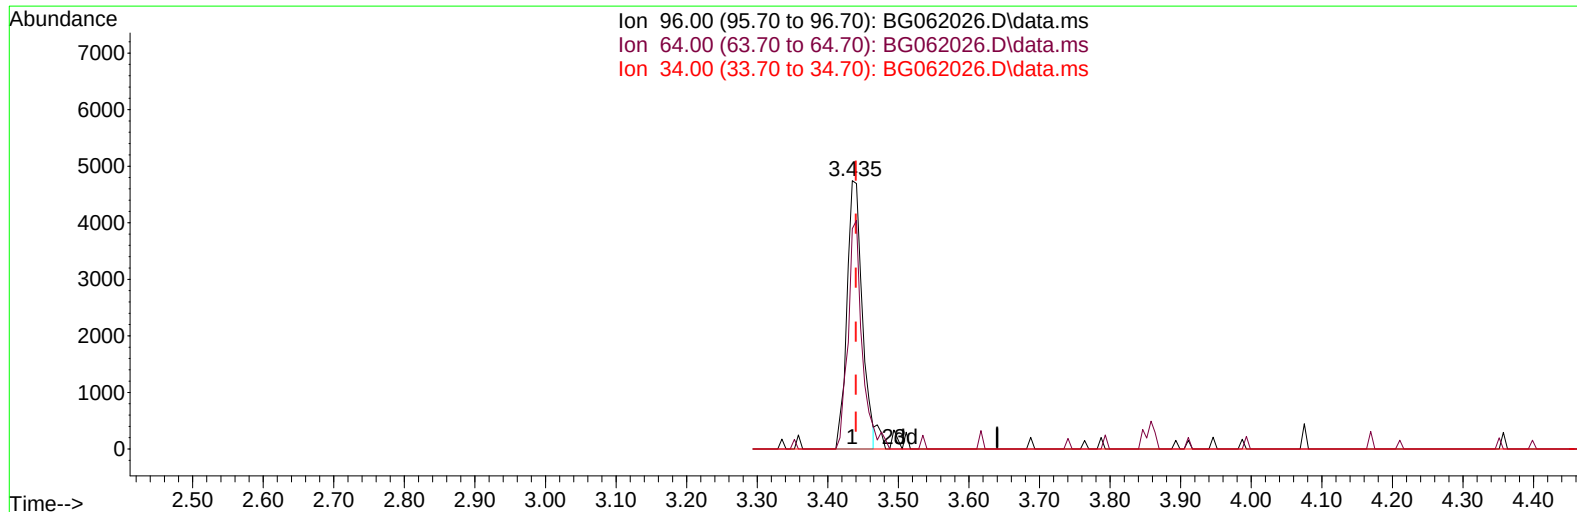

TIC: BG062026.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.435min (-0.005) 4.83 ng/uL

response 7161

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	104.80	82.11#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071124\
 Data File : BG062026.D
 Acq On : 12 Jul 2024 1:56
 Operator : MA/JU
 Sample : PB161949BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK949

Manual IntegrationsAPPROVED

Quant Time: Jul 12 09:27:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 11 12:11:32 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
 Supervised By :mohammad ahmed 07/15/2024

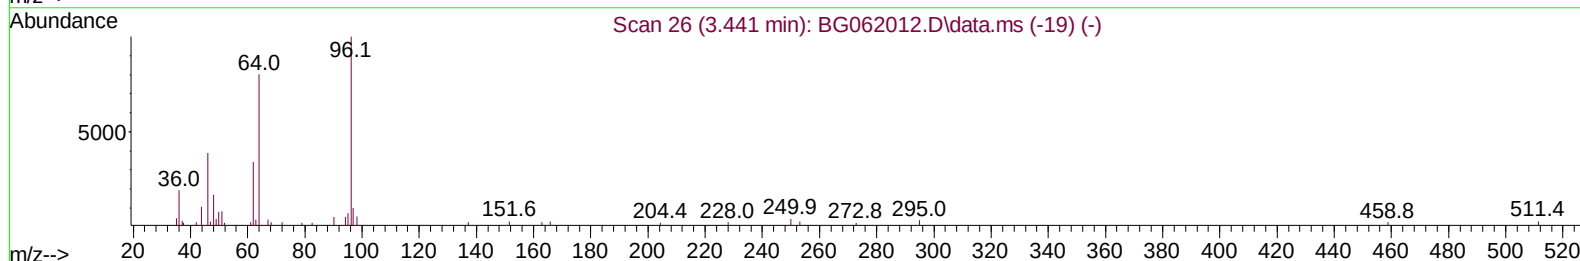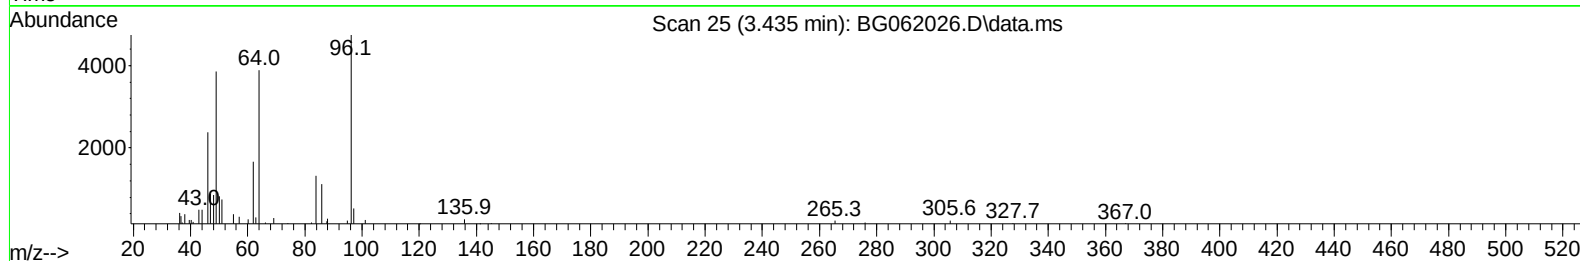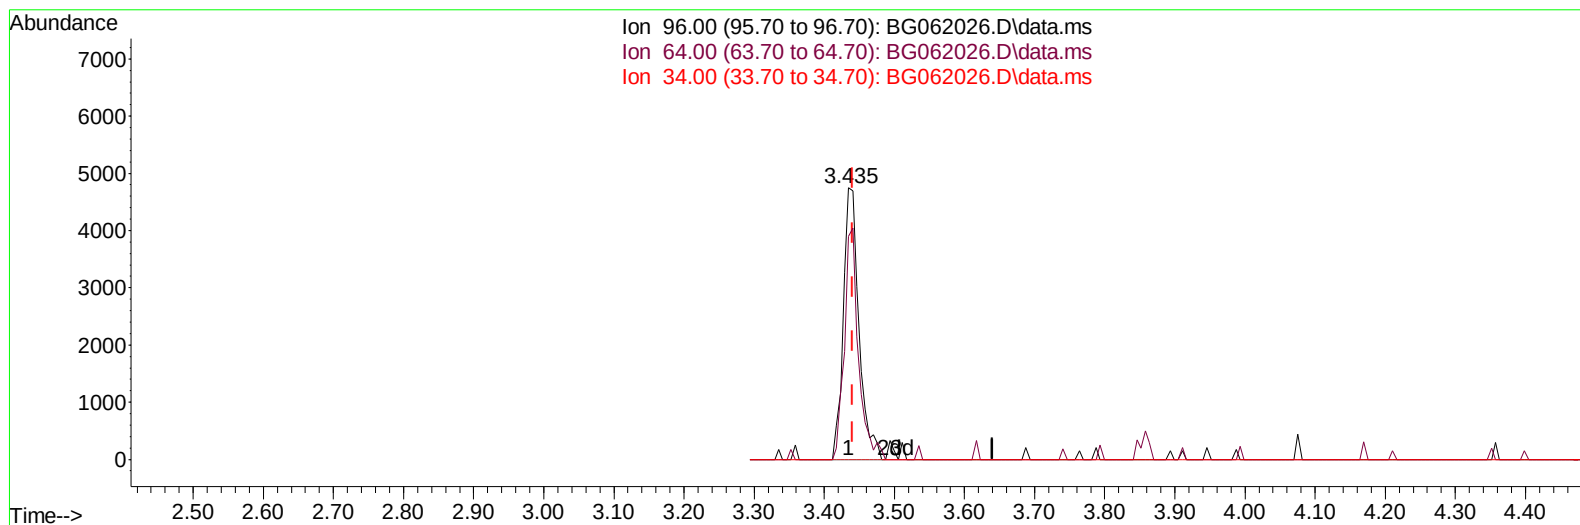

TIC: BG062026.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.435min (-0.005) 5.00 ng/uL m

response 7411

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	104.80	82.11#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071124\
 Data File : BG062026.D
 Acq On : 12 Jul 2024 1:56
 Operator : MA/JU
 Sample : PB161949BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK949

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/12/2024
 Supervised By :mohammad ahmed 07/15/2024

Quant Time: Jul 12 09:27:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 11 12:11:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.041	152	55691	20.000	ng/ul	0.00
20) Naphthalene-d8	10.850	136	249418	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.669	164	183046	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.413	188	424689	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.672	240	386225	20.000	ng/ul	0.00
88) Perylene-d12	24.880	264	444718	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.435	96	7411m	5.001	ng/uL	0.00
4) Pyridine-d5	3.852	84	111235	24.411	ng/ul	0.00
7) Phenol-d5	7.201	99	152393	25.004	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.366	67	89521	23.195	ng/ul	0.00
11) 2-Chlorophenol-d4	7.571	132	109257	26.134	ng/ul	0.00
15) 4-Methylphenol-d8	8.746	113	122064	25.437	ng/ul	0.00
21) Nitrobenzene-d5	9.205	128	55694	29.360	ng/ul	0.00
24) 2-Nitrophenol-d4	9.927	143	66014	30.474	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.468	165	124736	29.853	ng/ul	0.00
31) 4-Chloroaniline-d4	10.985	131	164729	27.155	ng/ul	0.00
46) Dimethylphthalate-d6	14.075	166	402688	26.759	ng/ul	0.00
49) Acenaphthylene-d8	14.363	160	447418	28.433	ng/ul	0.00
54) 4-Nitrophenol-d4	14.874	143	65117	27.096	ng/ul	0.00
60) Fluorene-d10	15.662	176	362159	28.587	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.779	200	59115	26.504	ng/ul	0.00
73) Anthracene-d10	17.512	188	590040	29.758	ng/ul	0.00
81) Pyrene-d10	19.798	212	690853	30.411	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.663	264	667939	30.284	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071124\
Data File : BG062026.D
Acq On : 12 Jul 2024 1:56
Operator : MA/JU
Sample : PB161949BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK949

Manual IntegrationsAPPROVED

Quant Time: Jul 12 09:27:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 11 12:11:32 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/15/2024

