

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071124\
 Data File : BG062026.D
 Acq On : 12 Jul 2024 1:56
 Operator : MA/JU
 Sample : PB161949BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK949

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.441	23	26	31	rVB5	19819	25651	1.46%	0.126%
2	3.576	47	49	54	rVB3	5227	5328	0.30%	0.026%
3	3.635	56	59	62	rBV4	3034	4926	0.28%	0.024%
4	3.817	87	90	93	rBV4	2417	3770	0.21%	0.019%
5	3.858	93	97	109	rVV	232705	415387	23.58%	2.046%
6	4.005	121	122	125	rVV2	4145	3795	0.22%	0.019%
7	4.034	125	127	132	rVB4	3889	5031	0.29%	0.025%
8	4.193	150	154	159	rVV6	5326	8795	0.50%	0.043%
9	4.275	167	168	173	rBV2	3809	3781	0.21%	0.019%
10	4.445	194	197	199	rBV2	3073	3336	0.19%	0.016%
11	4.516	207	209	212	rVB4	5567	3256	0.18%	0.016%
12	4.569	215	218	221	rVB3	4141	3917	0.22%	0.019%
13	4.675	233	236	241	rVB4	3473	6178	0.35%	0.030%
14	4.980	285	288	290	rBV3	4694	4367	0.25%	0.022%
15	5.280	336	339	340	rVB3	4811	4519	0.26%	0.022%
16	5.303	340	343	344	rBV3	3835	3770	0.21%	0.019%
17	5.403	357	360	362	rBV2	4864	3476	0.20%	0.017%
18	5.432	362	365	369	rVB4	2935	3804	0.22%	0.019%
19	5.779	423	424	427	rBV2	3374	3278	0.19%	0.016%
20	5.873	436	440	442	rBV3	4586	4554	0.26%	0.022%
21	5.950	452	453	456	rVB2	4010	3678	0.21%	0.018%
22	5.979	456	458	459	rBV2	4419	3248	0.18%	0.016%
23	6.020	462	465	467	rVV2	3863	3818	0.22%	0.019%
24	6.190	493	494	497	rVB	4321	3278	0.19%	0.016%
25	6.355	519	522	524	rBV3	2900	3943	0.22%	0.019%
26	6.537	549	553	554	rBV3	2710	3570	0.20%	0.018%
27	6.737	583	587	589	rBV2	4738	5577	0.32%	0.027%
28	7.201	658	666	674	rVV	336821	563136	31.96%	2.774%
29	7.366	686	694	702	rVB	202641	333935	18.95%	1.645%
30	7.571	722	729	736	rVB	293216	504286	28.62%	2.484%
31	7.900	784	785	789	rVB2	2894	3283	0.19%	0.016%
32	8.041	800	809	817	rVB	229839	401134	22.77%	1.976%
33	8.746	921	929	939	rBV	404021	672277	38.16%	3.311%
34	8.846	943	946	950	rVB3	3578	4593	0.26%	0.023%
35	9.081	984	986	990	rVB2	3386	3857	0.22%	0.019%
36	9.111	990	991	995	rBV3	3718	4011	0.23%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071124\
 Data File : BG062026.D
 Acq On : 12 Jul 2024 1:56
 Operator : MA/JU
 Sample : PB161949BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK949

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

37	9.205	999	1007	1015	rVV	300960	536194	30.43%	2.641%
38	9.293	1020	1022	1027	rVB3	2937	4293	0.24%	0.021%
39	9.492	1055	1056	1060	rBV2	4418	4256	0.24%	0.021%
40	9.616	1072	1077	1079	rBV2	2705	3751	0.21%	0.018%
41	9.669	1083	1086	1089	rBV2	2963	3451	0.20%	0.017%
42	9.927	1122	1130	1138	rBV	288277	505974	28.72%	2.492%
43	10.203	1174	1177	1181	rBV3	2519	3312	0.19%	0.016%
44	10.468	1215	1222	1230	rBV	391680	708960	40.24%	3.492%
45	10.797	1275	1278	1280	rBV4	3766	4995	0.28%	0.025%
46	10.850	1280	1287	1295	rVB	332597	609319	34.59%	3.001%
47	10.985	1302	1310	1319	rBV	379838	690611	39.20%	3.402%
48	11.167	1337	1341	1342	rBV3	2342	3240	0.18%	0.016%
49	11.331	1365	1369	1372	rVB2	3211	4239	0.24%	0.021%
50	11.355	1372	1373	1375	rBV	5087	3403	0.19%	0.017%
51	11.443	1386	1388	1391	rVB3	4064	3554	0.20%	0.018%
52	11.537	1401	1404	1408	rBV3	2278	3644	0.21%	0.018%
53	11.613	1414	1417	1419	rBV2	3791	3884	0.22%	0.019%
54	12.436	1552	1557	1559	rBV5	8183	12733	0.72%	0.063%
55	12.765	1609	1613	1616	rVB3	2876	3958	0.22%	0.019%
56	12.847	1625	1627	1632	rVB2	3280	3841	0.22%	0.019%
57	12.883	1632	1633	1638	rBV2	3078	3151	0.18%	0.016%
58	13.182	1682	1684	1688	rBV2	2767	3444	0.20%	0.017%
59	13.834	1792	1795	1797	rBV2	2776	3295	0.19%	0.016%
60	13.893	1803	1805	1808	rBV3	3185	3624	0.21%	0.018%
61	14.069	1828	1835	1841	rBV	679578	999034	56.71%	4.921%
62	14.363	1878	1885	1893	rVB	682918	1110965	63.06%	5.472%
63	14.628	1927	1930	1931	rBV2	4051	3593	0.20%	0.018%
64	14.669	1931	1937	1944	rVB	526887	853859	48.47%	4.206%
65	14.874	1965	1972	1980	rBV	372385	605887	34.39%	2.984%
66	15.074	2003	2006	2008	rBV4	5010	5476	0.31%	0.027%
67	15.139	2015	2017	2024	rVB4	6477	9457	0.54%	0.047%
68	15.203	2024	2028	2029	rBV3	3233	3754	0.21%	0.018%
69	15.297	2041	2044	2048	rVB3	3300	4594	0.26%	0.023%
70	15.403	2060	2062	2065	rVB2	4155	3907	0.22%	0.019%
71	15.427	2065	2066	2071	rBV3	2730	4074	0.23%	0.020%
72	15.662	2100	2106	2114	rVV	939122	1405705	79.79%	6.924%
73	15.773	2119	2125	2133	rBV	337311	511274	29.02%	2.518%
74	15.891	2141	2145	2146	rBV4	6285	6554	0.37%	0.032%
75	16.085	2174	2178	2179	rBV3	2783	4111	0.23%	0.020%
76	16.149	2187	2189	2192	rVB2	4846	3871	0.22%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071124\
 Data File : BG062026.D
 Acq On : 12 Jul 2024 1:56
 Operator : MA/JU
 Sample : PB161949BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK949

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

77	16.261	2206	2208	2211	rVB2	4187	3836	0.22%	0.019%
78	16.331	2218	2220	2224	rVB4	2933	3528	0.20%	0.017%
79	16.443	2238	2239	2243	rVB3	5571	5276	0.30%	0.026%
80	16.478	2243	2245	2246	rBV2	5311	3731	0.21%	0.018%
81	16.614	2266	2268	2269	rBV2	4841	3497	0.20%	0.017%
82	16.661	2273	2276	2279	rVV2	4892	6530	0.37%	0.032%
83	16.708	2282	2284	2285	rVB2	5776	3318	0.19%	0.016%
84	16.760	2290	2293	2296	rBV2	3940	4239	0.24%	0.021%
85	17.413	2398	2404	2410	rBV	700500	1080460	61.33%	5.322%
86	17.512	2415	2421	2428	rVB	1053490	1555501	88.29%	7.662%
87	17.606	2435	2437	2439	rBV2	8931	7614	0.43%	0.038%
88	17.683	2448	2450	2453	rVB3	5465	4986	0.28%	0.025%
89	17.718	2453	2456	2457	rBV3	4890	4219	0.24%	0.021%
90	17.753	2460	2462	2464	rBV3	5939	5375	0.31%	0.026%
91	17.836	2472	2476	2478	rBV4	7259	9690	0.55%	0.048%
92	17.924	2489	2491	2493	rBV3	5226	6398	0.36%	0.032%
93	17.953	2495	2496	2498	rVV2	4661	3305	0.19%	0.016%
94	17.977	2498	2500	2503	rVV4	4610	4557	0.26%	0.022%
95	18.065	2513	2515	2520	rVB6	6258	6403	0.36%	0.032%
96	18.182	2533	2535	2536	rBV2	5678	4293	0.24%	0.021%
97	19.798	2804	2810	2818	rVB	1253856	1761795	100.00%	8.678%
98	21.672	3123	3129	3140	rVB2	705095	1146719	65.09%	5.648%
99	24.663	3628	3638	3648	rBV2	621741	1728729	98.12%	8.515%
100	24.880	3667	3675	3686	rVB	440529	1231532	69.90%	6.066%




Sum of corrected areas: 20301315

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071124\
Data File : BG062026.D
Acq On : 12 Jul 2024 1:56
Operator : MA/JU
Sample : PB161949BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK949

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

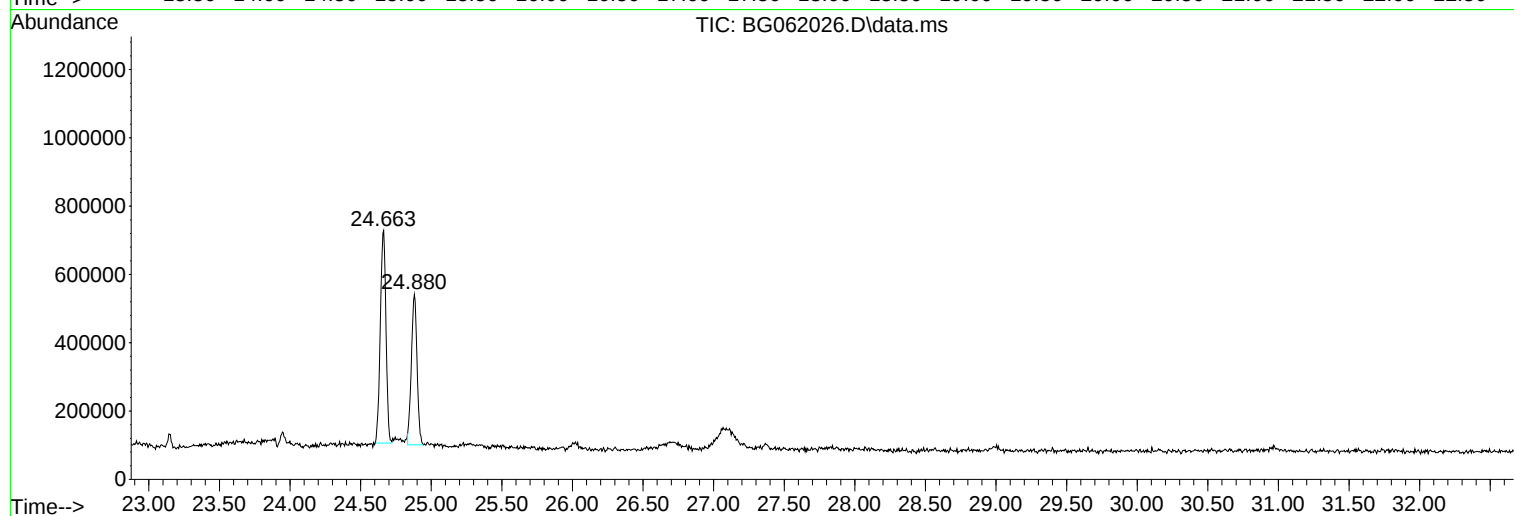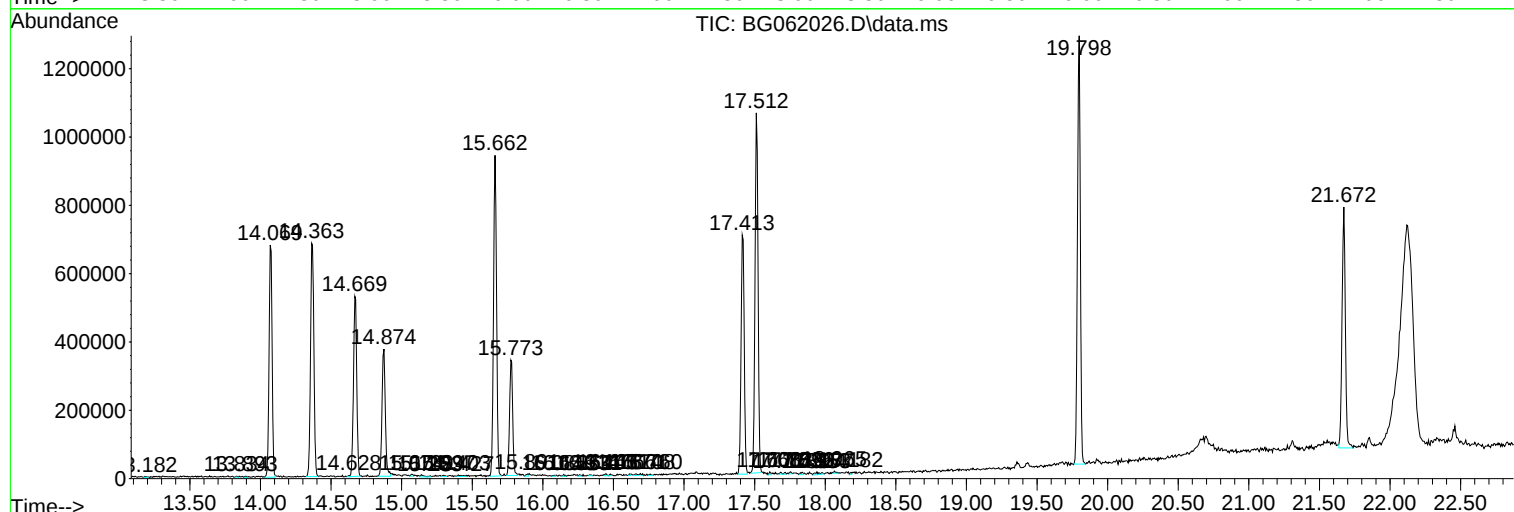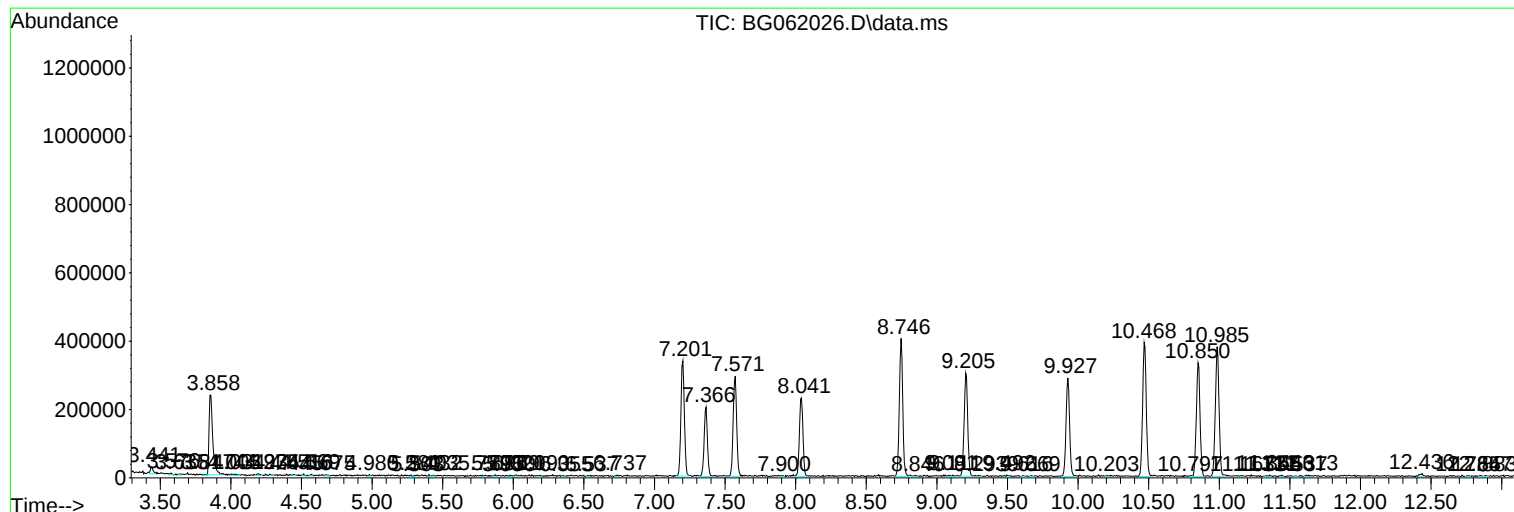

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071124\
Data File : BG062026.D
Acq On : 12 Jul 2024 1:56
Operator : MA/JU
Sample : PB161949BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK949

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071124\
Data File : BG062026.D
Acq On : 12 Jul 2024 1:56
Operator : MA/JU
Sample : PB161949BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK949

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc