

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071124\
 Data File : BG062036.D
 Acq On : 12 Jul 2024 10:02
 Operator : MA/JU
 Sample : PB161914BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK914

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.441	22	26	30	rBV4	14231	21519	1.31%	0.119%
2	3.858	93	97	107	rBV	222439	384570	23.44%	2.122%
3	4.199	151	155	157	rBV5	4966	5128	0.31%	0.028%
4	4.293	168	171	172	rBV	3090	3671	0.22%	0.020%
5	4.498	205	206	209	rVB3	4037	3085	0.19%	0.017%
6	4.657	231	233	239	rVB4	4108	7725	0.47%	0.043%
7	4.704	239	241	242	rBV2	4188	3768	0.23%	0.021%
8	4.786	251	255	258	rBV4	3165	5212	0.32%	0.029%
9	4.816	258	260	263	rVB3	3685	3046	0.19%	0.017%
10	5.109	307	310	313	rVB3	4119	4968	0.30%	0.027%
11	5.139	313	315	317	rBV3	4314	3912	0.24%	0.022%
12	5.291	339	341	344	rBV3	2925	3009	0.18%	0.017%
13	5.515	376	379	381	rBV2	2542	3372	0.21%	0.019%
14	5.579	387	390	392	rBV3	4548	5405	0.33%	0.030%
15	6.055	467	471	474	rBV3	2950	3998	0.24%	0.022%
16	6.343	519	520	522	rBV2	4900	3305	0.20%	0.018%
17	6.590	559	562	564	rBV3	2561	3057	0.19%	0.017%
18	6.743	585	588	590	rBV2	2693	2999	0.18%	0.017%
19	6.796	595	597	600	rVB3	4232	3333	0.20%	0.018%
20	6.995	628	631	634	rBV2	4797	4076	0.25%	0.022%
21	7.095	643	648	650	rVB4	2524	3557	0.22%	0.020%
22	7.207	659	667	673	rBV	343614	606141	36.95%	3.345%
23	7.365	687	694	703	rVV	211414	344722	21.02%	1.902%
24	7.448	706	708	711	rBV2	2637	3068	0.19%	0.017%
25	7.571	722	729	739	rBV	313072	533689	32.54%	2.945%
26	7.771	759	763	764	rBV	2923	3468	0.21%	0.019%
27	8.041	802	809	817	rVB	257431	431968	26.33%	2.384%
28	8.129	821	824	826	rBV4	3083	4116	0.25%	0.023%
29	8.535	890	893	897	rBV3	4226	5631	0.34%	0.031%
30	8.752	922	930	937	rBV2	400536	697378	42.51%	3.849%
31	9.093	983	988	989	rVB2	2731	3895	0.24%	0.021%
32	9.210	1000	1008	1015	rBV	332929	564482	34.41%	3.115%
33	9.299	1020	1023	1026	rVB2	3045	3157	0.19%	0.017%
34	9.516	1058	1060	1061	rVV	3819	3150	0.19%	0.017%
35	9.539	1061	1064	1065	rVV2	4325	3412	0.21%	0.019%
36	9.563	1065	1068	1072	rVV3	3382	5416	0.33%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071124\
 Data File : BG062036.D
 Acq On : 12 Jul 2024 10:02
 Operator : MA/JU
 Sample : PB161914BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK914

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

37	9.610	1072	1076	1079	rVV2	3888	5214	0.32%	0.029%
38	9.933	1120	1131	1140	rBV2	302022	536288	32.69%	2.960%
39	10.156	1166	1169	1171	rVB3	3244	3099	0.19%	0.017%
40	10.315	1193	1196	1198	rVB2	4619	4613	0.28%	0.025%
41	10.474	1214	1223	1232	rVB	410175	731354	44.59%	4.036%
42	10.656	1248	1254	1256	rBV	1709	3488	0.21%	0.019%
43	10.856	1280	1288	1295	rVB2	336463	609839	37.18%	3.366%
44	10.991	1303	1311	1317	rBV	341734	616275	37.57%	3.401%
45	11.279	1358	1360	1365	rVB4	1861	2972	0.18%	0.016%
46	11.343	1369	1371	1375	rBV2	2586	3169	0.19%	0.017%
47	11.613	1414	1417	1418	rBV2	5172	3384	0.21%	0.019%
48	11.637	1418	1421	1424	rVB3	3069	3580	0.22%	0.020%
49	11.725	1433	1436	1438	rBV2	3366	2908	0.18%	0.016%
50	12.430	1554	1556	1557	rBV2	8288	5785	0.35%	0.032%
51	12.530	1568	1573	1574	rBV3	2451	3507	0.21%	0.019%
52	12.548	1574	1576	1582	rVB2	3663	5001	0.30%	0.028%
53	12.653	1588	1594	1595	rBV3	2218	3531	0.22%	0.019%
54	12.906	1634	1637	1639	rVB	3834	3487	0.21%	0.019%
55	12.935	1639	1642	1645	rBV2	2662	3018	0.18%	0.017%
56	13.006	1651	1654	1656	rBV2	2602	3754	0.23%	0.021%
57	13.100	1668	1670	1671	rBV	3995	3161	0.19%	0.017%
58	13.165	1679	1681	1683	rVB3	3551	3054	0.19%	0.017%
59	13.212	1686	1689	1692	rVV3	3799	5428	0.33%	0.030%
60	13.411	1719	1723	1724	rVB2	3706	2936	0.18%	0.016%
61	13.435	1724	1727	1729	rBV	2805	3278	0.20%	0.018%
62	13.570	1746	1750	1751	rBV2	3774	2961	0.18%	0.016%
63	13.617	1755	1758	1760	rBV3	2217	2917	0.18%	0.016%
64	13.658	1763	1765	1768	rBV2	3475	3903	0.24%	0.022%
65	13.729	1774	1777	1780	rBV	6266	7545	0.46%	0.042%
66	14.075	1829	1836	1842	rBV	701329	999824	60.95%	5.518%
67	14.369	1879	1886	1895	rBV	722077	1122291	68.42%	6.194%
68	14.522	1911	1912	1915	rBV	2911	3241	0.20%	0.018%
69	14.628	1926	1930	1932	rBV3	4256	5823	0.35%	0.032%
70	14.675	1932	1938	1945	rVV	536265	815983	49.75%	4.503%
71	14.733	1946	1948	1951	rVB3	7251	5365	0.33%	0.030%
72	14.874	1966	1972	1984	rBV	346400	577354	35.20%	3.186%
73	15.133	2014	2016	2019	rVB2	3363	3468	0.21%	0.019%
74	15.168	2019	2022	2027	rBV5	3747	5077	0.31%	0.028%
75	15.333	2048	2050	2052	rBV3	5017	3897	0.24%	0.022%
76	15.356	2052	2054	2056	rBV2	4331	4486	0.27%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071124\
 Data File : BG062036.D
 Acq On : 12 Jul 2024 10:02
 Operator : MA/JU
 Sample : PB161914BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK914

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

77	15.444	2068	2069	2071	rBV	3281	2915	0.18%	0.016%
78	15.562	2086	2089	2090	rBV3	3996	3366	0.21%	0.019%
79	15.609	2096	2097	2099	rBV	5776	3367	0.21%	0.019%
80	15.662	2099	2106	2114	rVV	869144	1360336	82.93%	7.507%
81	15.779	2121	2126	2132	rBV2	161498	235958	14.38%	1.302%
82	16.284	2209	2212	2213	rBV3	4790	4107	0.25%	0.023%
83	16.343	2220	2222	2224	rBV3	4080	3656	0.22%	0.020%
84	16.431	2235	2237	2239	rBV3	6269	6154	0.38%	0.034%
85	16.484	2245	2246	2249	rBV3	4027	4229	0.26%	0.023%
86	16.596	2264	2265	2267	rBV	4750	3352	0.20%	0.018%
87	16.719	2283	2286	2289	rBV5	7155	11748	0.72%	0.065%
88	16.749	2289	2291	2292	rVB2	6907	3921	0.24%	0.022%
89	16.766	2292	2294	2295	rBV2	6399	4560	0.28%	0.025%
90	16.819	2301	2303	2304	rBV2	4388	3173	0.19%	0.018%
91	17.172	2361	2363	2365	rBV3	6176	3828	0.23%	0.021%
92	17.313	2385	2387	2388	rBV2	5960	4109	0.25%	0.023%
93	17.418	2399	2405	2412	rBV	664165	964768	58.82%	5.324%
94	17.518	2416	2422	2428	rVB	955403	1449178	88.35%	7.998%
95	17.665	2443	2447	2448	rBV4	17568	21149	1.29%	0.117%
96	17.859	2478	2480	2481	rVB2	6916	3072	0.19%	0.017%
97	18.065	2513	2515	2516	rBV2	8934	5819	0.35%	0.032%
98	19.804	2805	2811	2816	rBV	1105689	1579436	96.29%	8.717%
99	21.678	3125	3130	3136	rVB2	622155	964684	58.81%	5.324%
100	24.669	3632	3639	3651	rVB2	596814	1640328	100.00%	9.053%




Sum of corrected areas: 18119879

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071124\
Data File : BG062036.D
Acq On : 12 Jul 2024 10:02
Operator : MA/JU
Sample : PB161914BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK914

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

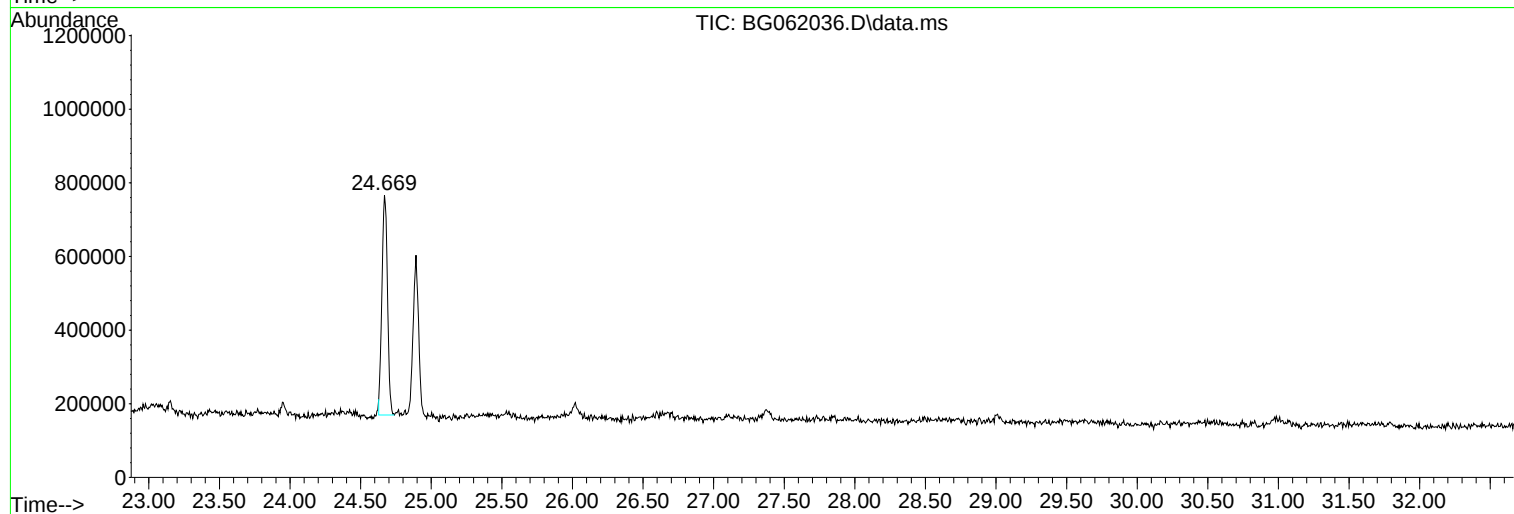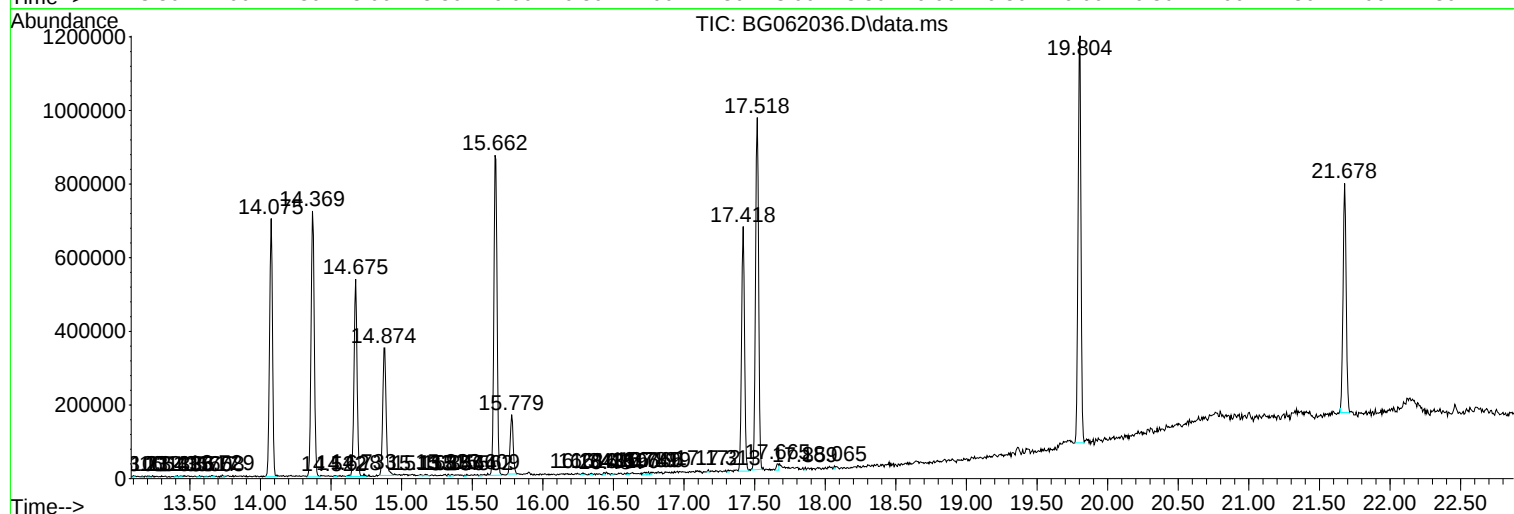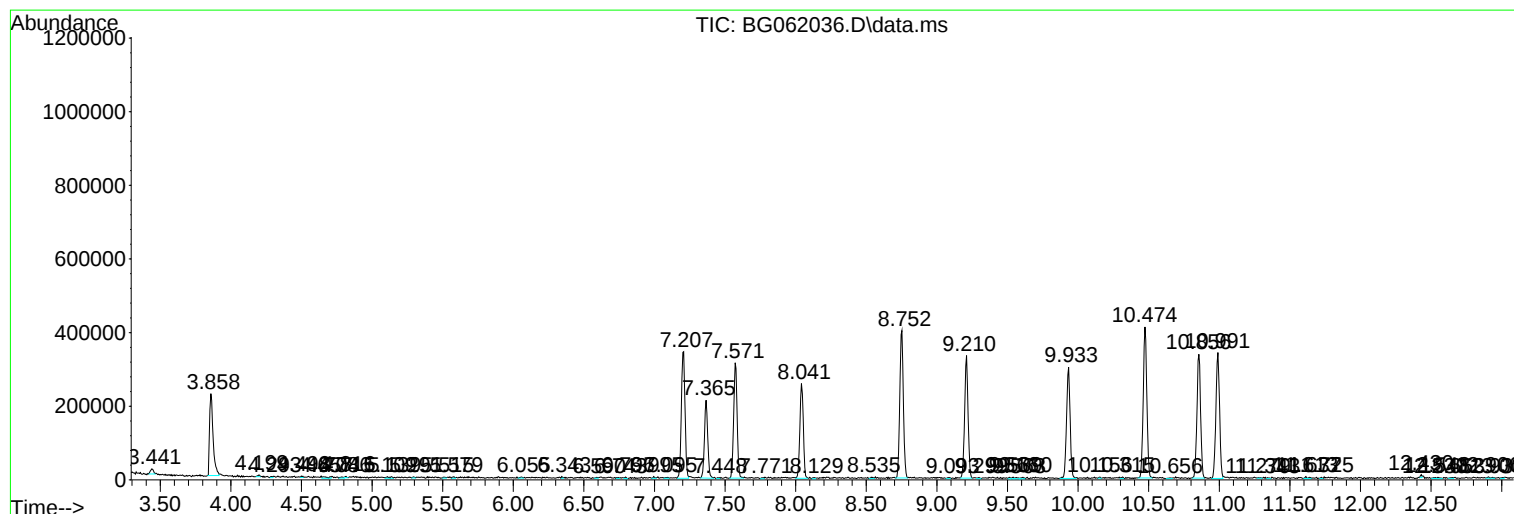

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071124\
Data File : BG062036.D
Acq On : 12 Jul 2024 10:02
Operator : MA/JU
Sample : PB161914BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK914

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071124\
Data File : BG062036.D
Acq On : 12 Jul 2024 10:02
Operator : MA/JU
Sample : PB161914BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK914

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc