
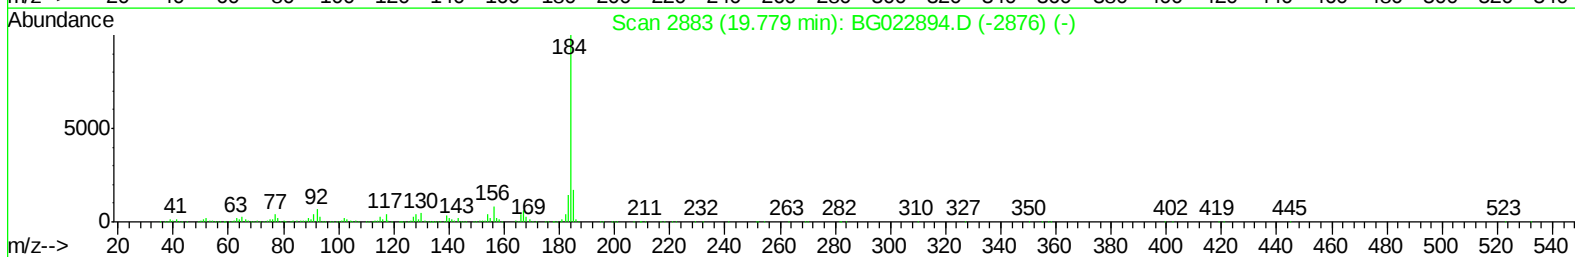
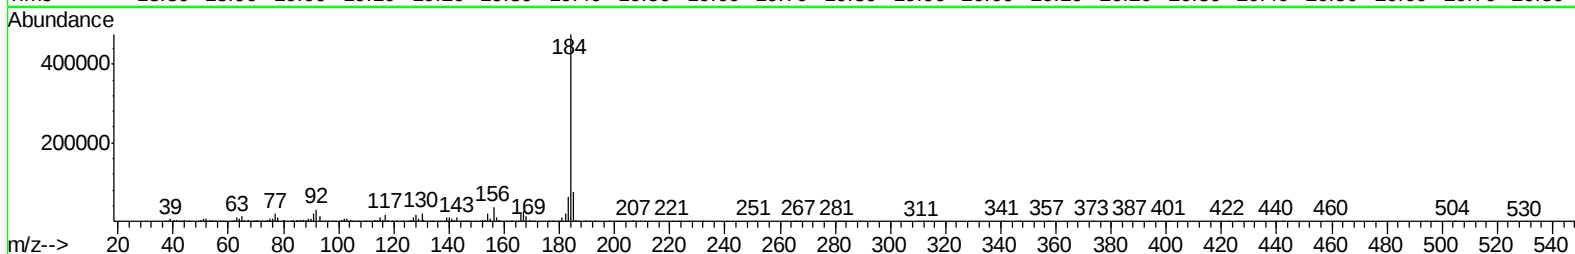


Data Path : Z:\HPCHEM1\BNA_G\Data\BG071216\
Data File : BG023034.D
Acq On : 12 Jul 2016 13:25
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 09:05:43 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 18:30:58 2016
Response via : Initial Calibration

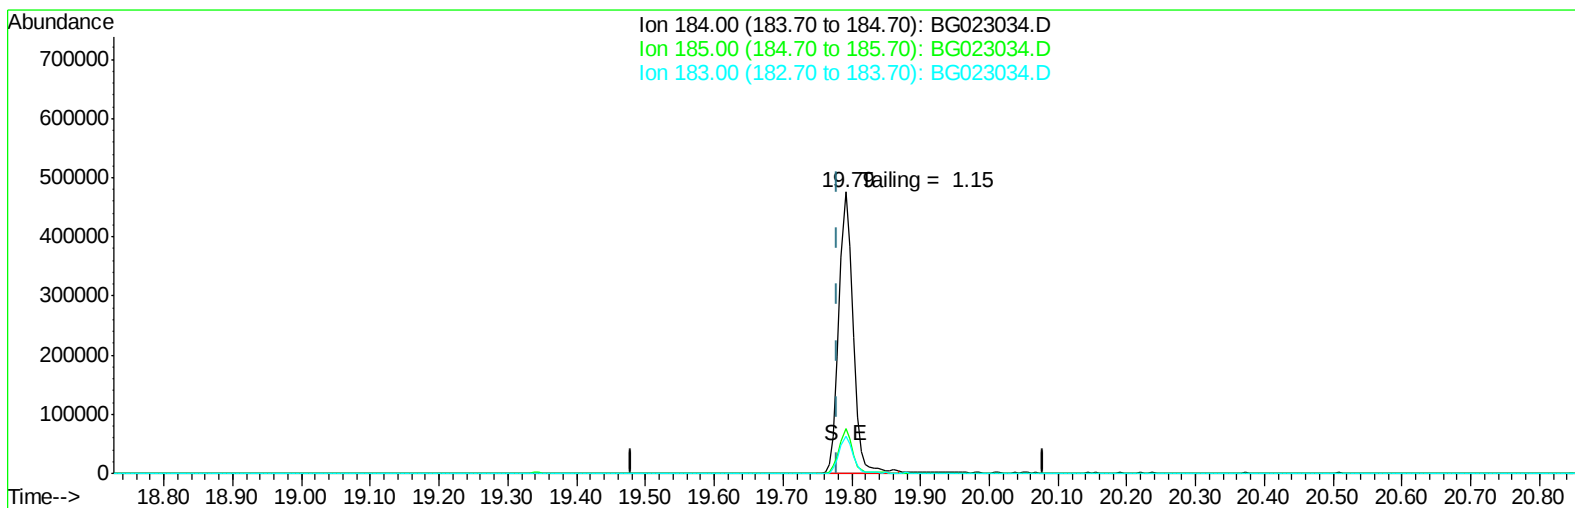

TIC: BG023034.D

(76) Benzidine




19.791min (+0.011) 14681.24ng

response 677213

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.71
183.00	13.40	13.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG071216\
Data File : BG023034.D
Acq On : 12 Jul 2016 13:25
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 09:05:43 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 18:30:58 2016
Response via : Initial Calibration

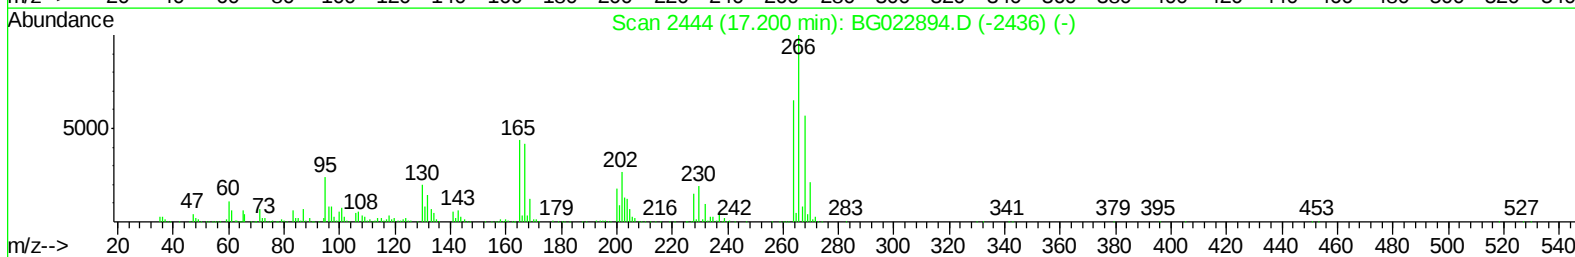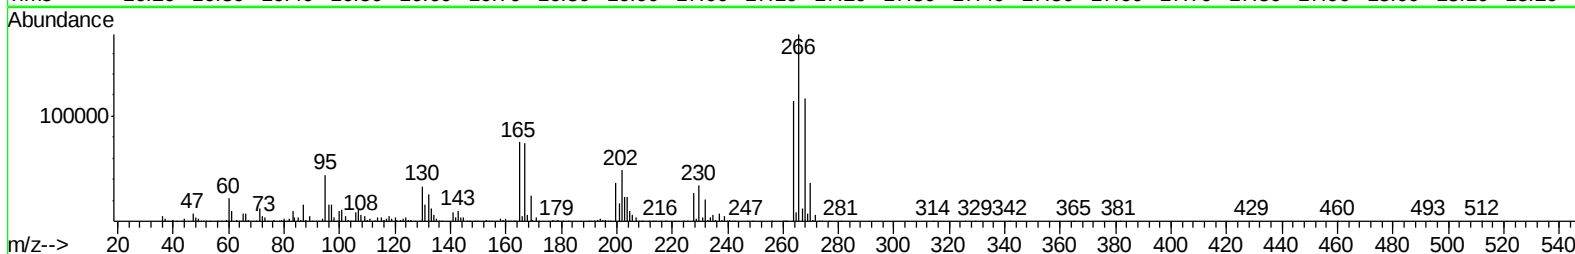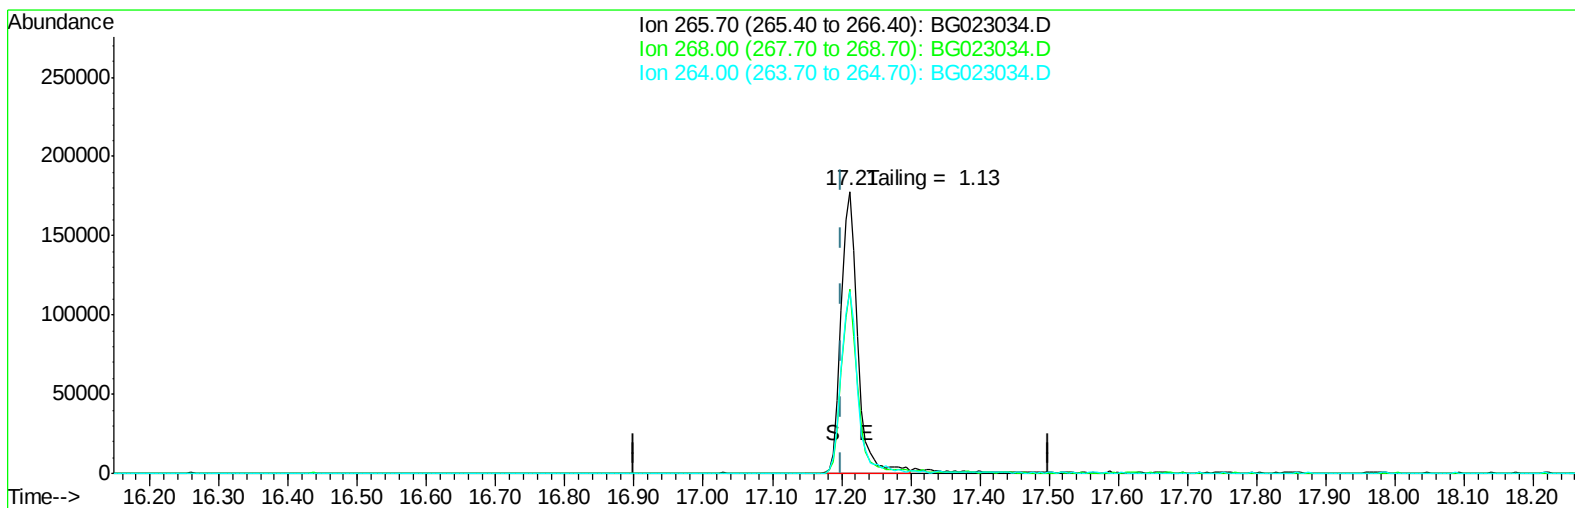

TIC: BG023034.D

(69) Pentachlorophenol (C)

17.211min (+0.011) 31901.58ng

response 290495

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	65.62
264.00	63.20	64.76
0.00	0.00	0.00