
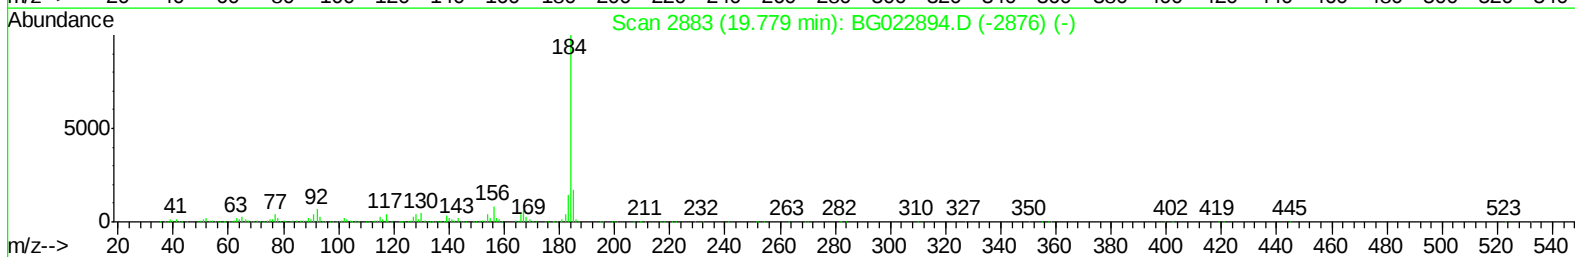
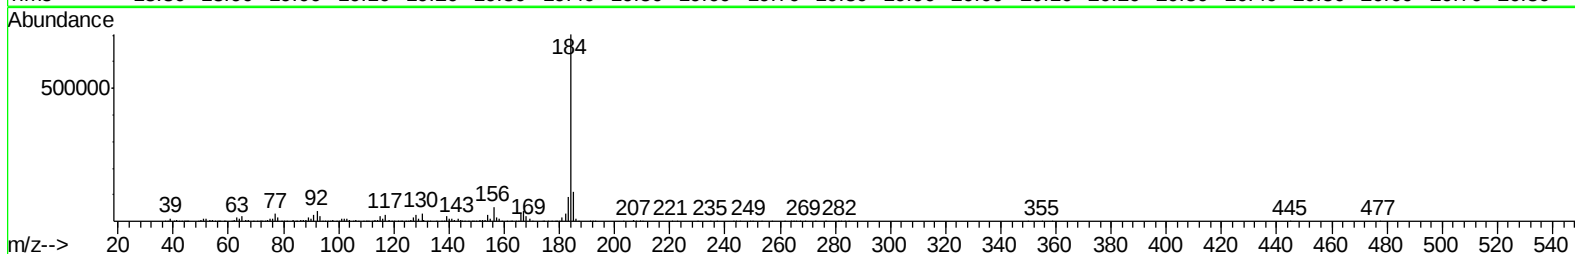


Data Path : Z:\HPCHEM1\BNA_G\Data\BG071216\
Data File : BG023049.D
Acq On : 13 Jul 2016 00:06
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 09:06:23 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 18:30:58 2016
Response via : Initial Calibration

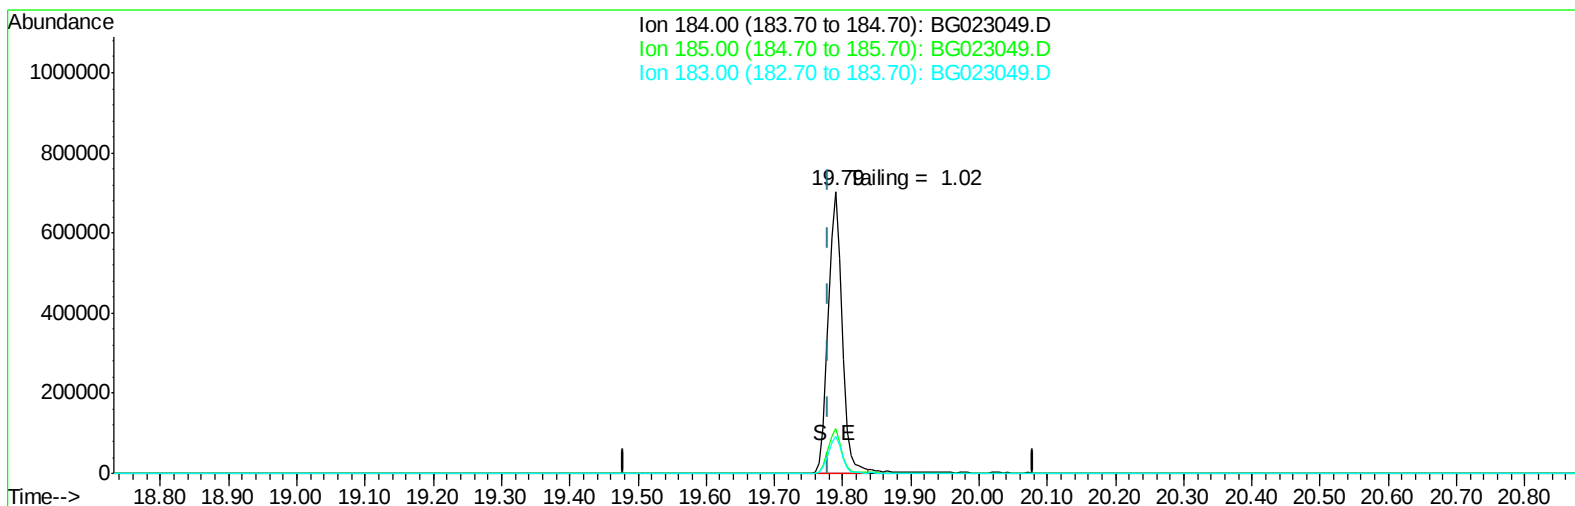

TIC: BG023049.D

(76) Benzidine




19.789min (+0.010) 36845.43ng

response 1000323

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.75
183.00	13.40	13.22
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG071216\
Data File : BG023049.D
Acq On : 13 Jul 2016 00:06
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 09:06:23 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 18:30:58 2016
Response via : Initial Calibration

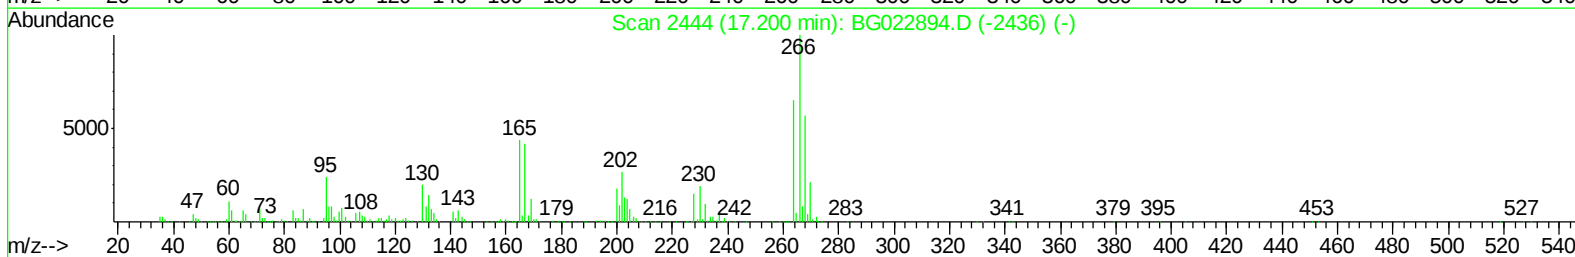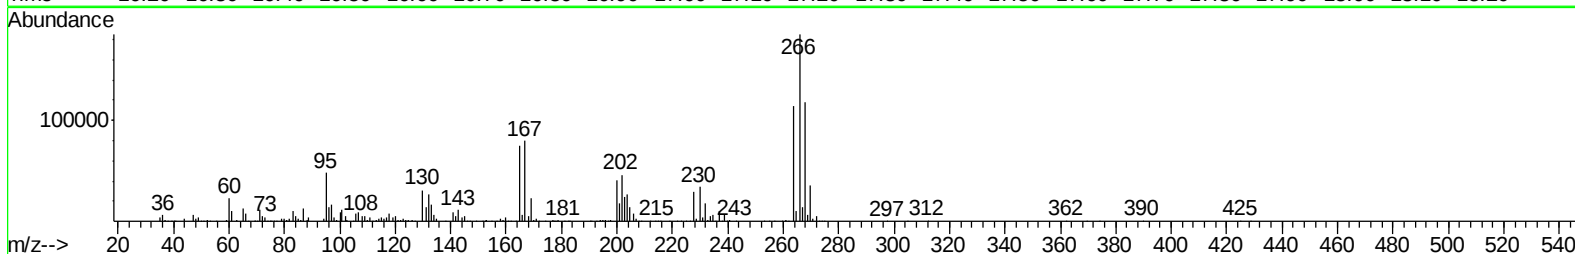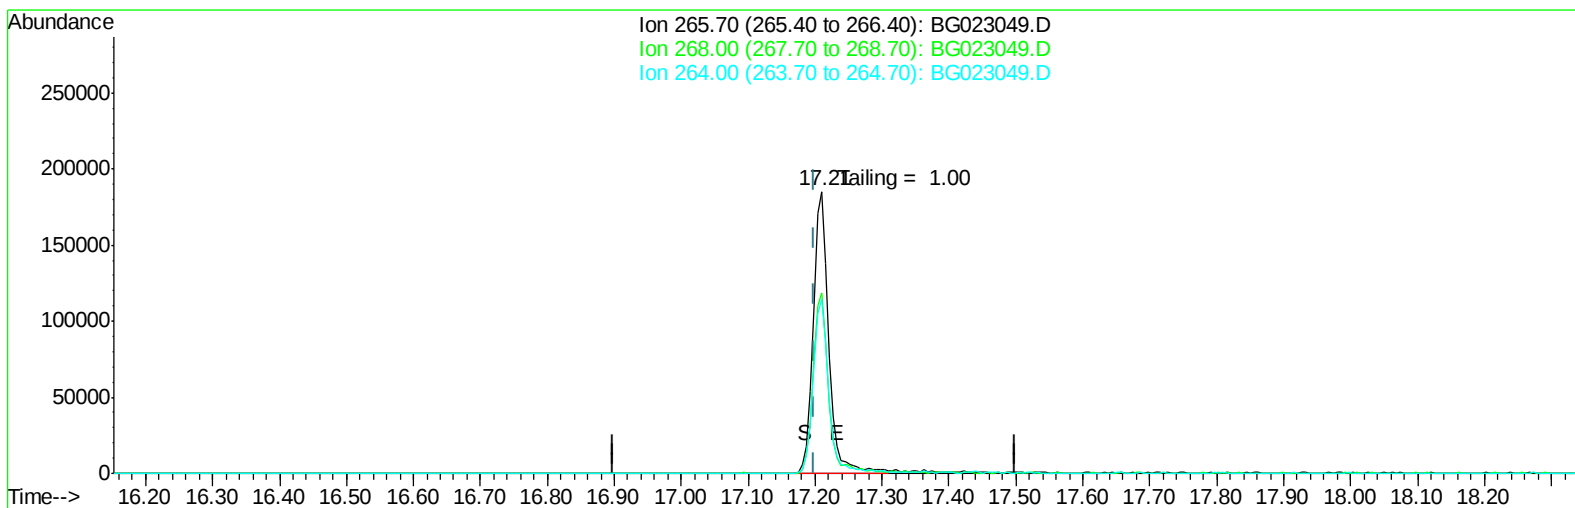

TIC: BG023049.D

(69) Pentachlorophenol (C)

17.210min (+0.010) 81339.11ng

response 307744

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	64.00
264.00	63.20	61.64
0.00	0.00	0.00