


Data Path : Z:\HPCHEM1\BNA G\DATA\BG071216\
 Data File : BG023034.D
 Acq On : 12 Jul 2016 13:25
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 12 18:30:58 2016

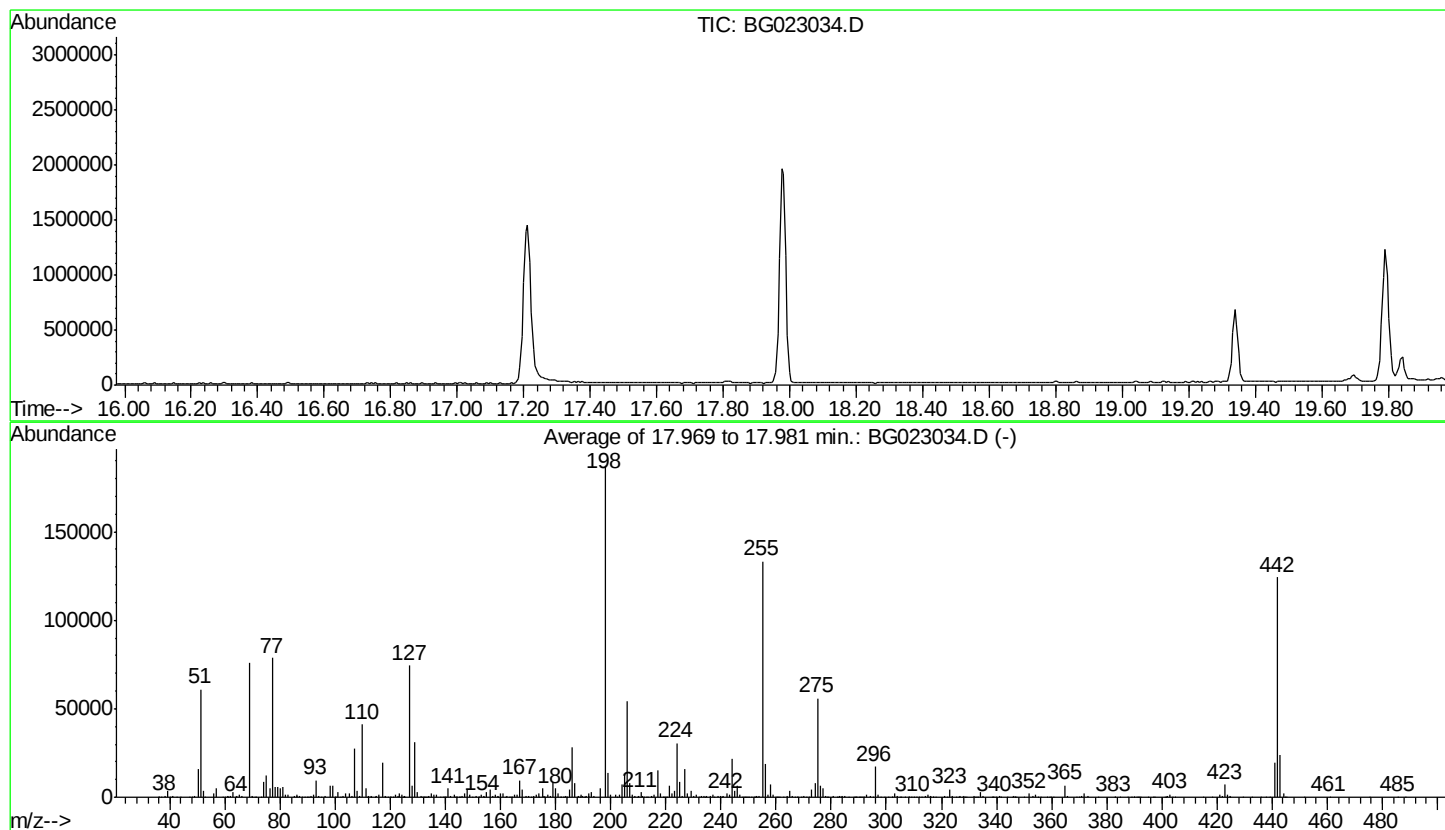

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	60885	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.6	76088	PASS
70	69	0.00	2	0.6	420	PASS
127	198	10	80	39.8	74490	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	187346	PASS
199	198	5	9	7.2	13537	PASS
275	198	10	60	29.8	55848	PASS
365	198	1	100	3.5	6624	PASS
441	442	0.01	24	15.7	19432	PASS
442	198	50	100	66.2	124072	PASS
443	442	15	24	19.1	23685	PASS